
TECHNICAL MANUAL

**OPERATOR'S, ORGANIZATIONAL, DIRECT SUPPORT, AND
GENERAL SUPPORT MAINTENANCE MANUAL
(INCLUDING REPAIR PARTS AND SPECIAL TOOLS LISTS)**

FOR

**PLUG-IN UNIT, RF SECTION
HEWLETT-PACKARD MODEL 86601A
(NSN 6625-00-005-1226)**

**HEADQUARTERS, DEPARTMENT OF THE ARMY
OCTOBER 1979**

This manual contains copyright material reproduced by permission of the Hewlett-Packard Company.

TM 11-6425-2837-14&P-6

TECHNICAL MANUAL

No. 11-6425-2837-14&P-6

HEADQUARTERS
DEPARTMENT OF THE ARMY
WASHINGTON, DC, 20315 October 1979

**OPERATOR'S, ORGANIZATIONAL, DIRECT SUPPORT, AND GENERAL SUPPORT MAINTENANCE
MANUAL INCLUDING REPAIR PARTS AND SPECIAL TOOLS LISTS
FOR
PLUG-IN UNIT, RF SECTION
HEWLETT-PACKARD MODEL 86601A
(NSN 6625-00-005-1226)**

REPORTING OF ERRORS

You can improve this manual by recommending improvements using DA Form 2028-2 located in the back of the manual. Simply tear out the self-addressed form, fill it out as shown on the sample, fold it where shown, and drop it in the mail.

If there are no blank DA Forms 2028-2 in the back of your manual, use the standard DA Form 2028 (Recommended Changes to Publications and Blank Forms) and forward to the Commander, US Army Communications and Electronics Material Readiness Command, ATTN: DRSEL-ME-MQ, Fort Monmouth, NJ 07763.

In either case a reply will be furnished direct to you.

This manual is an authentication of the manufacturer's commercial literature which, through usage, has been found to cover the data required to operate and maintain this equipment. Since the manual was not prepared in accordance with military specifications, the format has not been structured to consider levels of maintenance.

CONTENTS

Section	Page	Section IV.	Page
0. INTRODUCTION	0 - 1		
I. GENERAL INFORMATION	1-1	4-17. Signal-To-AM Noise Ratio	4-9
1-2. Introduction	1-1	4-18. Residual FM	4-10
1-6. Instruments Covered by Manual	1-1	4-19. Amplitude Modulation	4-10
1-8. Description	1-1	4-20. Amplitude Modulation: On/Off Ratio	4-11
1-12. Options	1-1	4-21. Amplitude Modulation Carrier Envelope Distortion	4-12
1-13. Accessories Available	1-2	4-23. Incidental Phase Modulation	4-16
1-13. Test Equipment and Accessories	1-2	4-23. Frequency Modulation	4-16
		4-24. Frequency Switching Time	4-17
II. INSTALLATION	2-1	4-25. Output Level Switching Time	4-19
2-1. Initial Inspection	2-1	4-26. Incidental AM	4-20
4-2. Mechanical Check	2-1	V. ADJUSTMENTS	5-1
2-5. Electrical Check	2-1	5-1. Introduction	5-1
2-7. Checks for Damage	2-1	5-7. Recommended Test Equipment	5-1
2-10. Preparation for Use	2-1	5-10. Service Kit	5-1
2-12. Power Requirements	2-1	5-13. Checks and Adjustments	5-1
2-14. Operating Environment	2-1	5-14. RF Output Meter Calibration	5-2
2-16. Storage and Shipment	2-1	5-15. Harmonic Distortion Checks and Adjustments	5-4
2-18. Original Packaging	2-1	5-16. Amplitude Modulation Calibration	5-6
2-23. Other Packaging Material	2-1	5-17. A12 Filter Assy Checks and Adjustments	5-9
III. OPERATION	3-1	5-18. 480 MHz Active Filter Checks and Adjustments	5-10
3-1. Introduction	3-1	VI. REPLACEABLE PARTS	6-1
3-4. Panel Features	3-1	6-1. Introduction	6-1
3-6. Operating Principles	3-1	6-6. Ordering Information	6-1
3-11. Operator's Checks	3-1	VII. MANUAL CHANGES	7-1
IV. PERFORMANCE TESTS	4-1	7-1. Introduction	7-1
4-1. Introduction	4-1	7-5. Manual Change Instructions	7-1
4-3. Purpose	4-1	VIII. SERVICE	8-1
4-8. Performance Tests	4-1	8-1. Introduction	8-1
4-9. Frequency Range	4-1	8-3. Principles of Operation	8-1
4-10. Frequency Accuracy and Stability	4-2	8-10. Recommended Test Equipment	8-1
4-11. Output Accuracy and Level	4-2	8-12. Troubleshooting	8-1
4-12. Output Flatness	4-3	8-17. Repair	8-1
4-13. Impedance: 50 Ohms	4-4		
4-14. Harmonic Signals	4-5		
4-15. Spurious Signals	4-6		
4-15. Signal-to-Phase Noise Ratio	4-7		

ILLUSTRATIONS

Figure	Page	Figure	Page
1-1. Model 86601A RF Section	1-0	4-2. Output Accuracy and Level Test Setup	4-2
1-2. Instrument Identification	1-1	4-3. Output Flatness Test Setup	4-3
1-3. 15 kHz Lowpass Filter	1-6	4-4. Impedance Test Setup	4-4
1-4. 100 kHz Lowpass Filter	1-6	4-5. Harmonic Signal Test Setup	4-5
1-5. 40 dB Amplifier	1-6	4-6. Spurious Signal Test Setup	4-6
3-1. Front and Rear Panel Controls, Indicators, and Connectors	3-0	4-7. Signal-to-Phase Noise Test Setup	4-8
4-1. Frequency Range and Accuracy Test Setup	4-1	4-8. Signal-to-AM Noise Ratio Test Setup	4-9
		4-9. Amplitude Modulation Test Setup	4-10

ILLUSTRATIONS (cont'd)

Figure	Page	Figure	Page
4-10. Amplitude Modulation ON/OFF Ratio Test Setup	4-12	8-4. Integrated Circuit Packaging	8-6
4-11. Amplitude Modulation Carrier Envelope Distortion Test Setup	4-13	8-5. Integrated Circuits used in Model 86601A	8-7
4-12. Incidental FM Test Setup	4-15	8-6. Chassis Mounted Parts and Assembly Locations	8-7
4-13. Frequency Modulation Test Setup	4-16	8-7. Model 86601A Troubleshooting Tree	8-8
4-14. Frequency Switching Time Test Setup	4-18	8-8. Model 86601A w/cover Removed	8-10
4-15. Output Level Switching Time Test Setup	4-19	8-9. Mixer Schematic Diagram	8-11
4-16. Incidental AM Test Setup	4-20	8-10. Mother Board Component Locations	8-11
5-1. RF Output Meter Calibration Setup	5-2	8-11. Input Connector	8-11
5-2. Amplitude Modulation Calibration Setup	5-3	8-12. Model 86601A Block Diagram	8-11
5-3. Harmonic Distortion Adjustment Setup	5-4	8-13. 450 MHz Band Pass Filter Component Locations	8-12
5-4. A12A1 Filter Adjustment Setup	5-6	8-14. Modulator Assembly Component Locations	8-13
5-5. Preliminary Adjustment Setup (450/460 Bandpass Filter)	5-9	8-15. Dual Filter Adjustment Locations	8-13
5-6. Active Filter Adjustment Setup	5-10	8-16. Modulator Assembly Component Locations	8-13
7-1. RF Output Meter Calibration Setup	7-3	8-17. Filters, Mixers and Modulator Schematic	8-13
7-2. Partial Logic Schematic	7-5	8-18. Preamplifier Component Locations	8-15
7-3. A5 Modulator Assembly 86601-60001	7-5	8-19. Power Amplifier and AGC Component Locations	8-15
7-4. Modulator Assembly Component Locations	7-7	8-20. Pre-Amp and PWR-Amp Schematic	8-15
7-5. Reference Assembly	7-8	8-21. Front Panel Component Locations	8-16
7-6. Reference Assembly Component Locations	7-9	8-22. Feedback Amplifier Component Locations	8-17
7-7. Feedback Amplifier	7-10	8-23. Reference Assembly Component Locations	8-17
7-8. Feedback Amplifier Component Locations	7-11	8-24. Feedback Amplifier and Reference Assembly Schematic	8-17
8-1. Model 86601A Simplified Block Diagram	8-0	8-25. Logic Assembly Component Locations	8-19
8-2. Diagram of Module Exchange Program	8-3	8-26. Logic and Driver Circuit Schematic	8-19
8-3. Model 86601A with Circuit Board Extended for Maintenance	8-4	8-27. Attenuator Driver Component Locations	8-21
		8-28. Attenuator Driver Schematic	8-21

TABLES

Table	Page	Table	Page
1-1. Model 86601A Specifications	1-2	6-3. Replaceable Parts	6-3
1-2. Test Equipment and Accessories List	1-4	6-4. Manufacture's Code List	6-15
1-3. 40 dB Amplifier Specifications	1-6	6-5. Part Number-National Stock Number Cross Reference Index	6-16
4-1. Spurious checks	4-7	7-1. Manual Changes by Serial Number	7-1
4-2. Carrier Envelope Distortion Test	4-14	7-2. Assembly-Change Cross Reference Index	7-4
4-3. Performance Test Record	4-22	8-1. Schematic Diagram Notes	8-5
5-1. Harmonic Distortion Level Checks	5-5	8-2. Assembly Locations	8-7
6-1. Part Numbers for Assembly Exchange Orders	6-1	8-3. 1 dB Attenuation Checks	8-16
6-2. Reference Designators and Abbreviations Used in Parts List	6-2	8-4. Attenuator Driver Levels	8-20

APPENDIXES

A. REFERENCES	A-1	E. REPAIR PARTS AND SPECIAL TOOLS LISTS	E-1
B. COMPONENTS OF END ITEM LIST (NA)		F. EXPENDABLE SUPPLIES AND MATERIALS LIST (NA)	
C. ADDITIONAL AUTHORIZATION LIST (NA)			
D. MAINTENANCE ALLOCATION	D-1		

SECTION 0

INTRODUCTION

0-1. SCOPE

This manual describes Plug-in Unit, Rf section, Hewlett-Packard Model 86601A and provides instructions for operation and maintenance.

0-2. INDEXES OF PUBLICATIONS

a. DA Pam 310-4. Refer to the latest issue of DA Pam 310-4 to determine whether there are new editions, changes, or additional publications pertaining to the equipment.

b. DA Pam 310-7. Refer to DA Pam 310-7 to determine whether there are modification work orders (MWO's) pertaining to the equipment.

0-3. MAINTENANCE FORMS, RECORDS,
AND REPORTS

a. Reports of Maintenance and Unsatisfactory Equipment. Department of the Army forms and procedures used for equipment maintenance will be those described by TM 38-750, The Army Maintenance Management System.

b. Report of Packaging and Handling Deficiencies. Fill out and forward DD Form 6 (Packaging Improvement Report) as prescribed in AR 700-58/NAVSUP-INST 4030.29/AFR 71-13/MCO P4030.29A, and DLAR 4145.8.

c. Discrepancy in Shipment Report (DISREP) (SF 361). Fill out and forward Discrepancy in Shipment

Report (DISREP) (SF 361) as prescribed in AR 55-38/NAVSUPINST 4610.33B/AFR 75-18/MCO P4610.19C and DLAR 4500.15.

0-4. REPORTING EQUIPMENT
IMPROVEMENT RECOMMENDATIONS
(EIR).

EIR can and must be submitted by anyone who is aware of an unsatisfactory condition with the equipment design or use. It is not necessary to show a new design or fit a better way to perform a procedure; just simply tell why the design is unfavorable or why a procedure is difficult. EIR may be submitted on SF 368 (Quality Deficiency Report). Mail direct to Commander, US Army Communications and Electronics Materiel Readiness Command, ATTN: DRSEL-ME-MQ, Fort Monmouth, NJ 07703. A reply will be furnished to you.

0-5. ADMINISTRATIVE STORAGE

Administrative storage ~~equipment~~ **equipment issued to and used by Army activities shall be in accordance with paragraph 2-16.**

0-6. DESTRUCTION OF ARMY ELECTRONICS
MATERIEL

Destruction of Army electronics materiel to prevent enemy use shall be in accordance with TM 750-244-2.

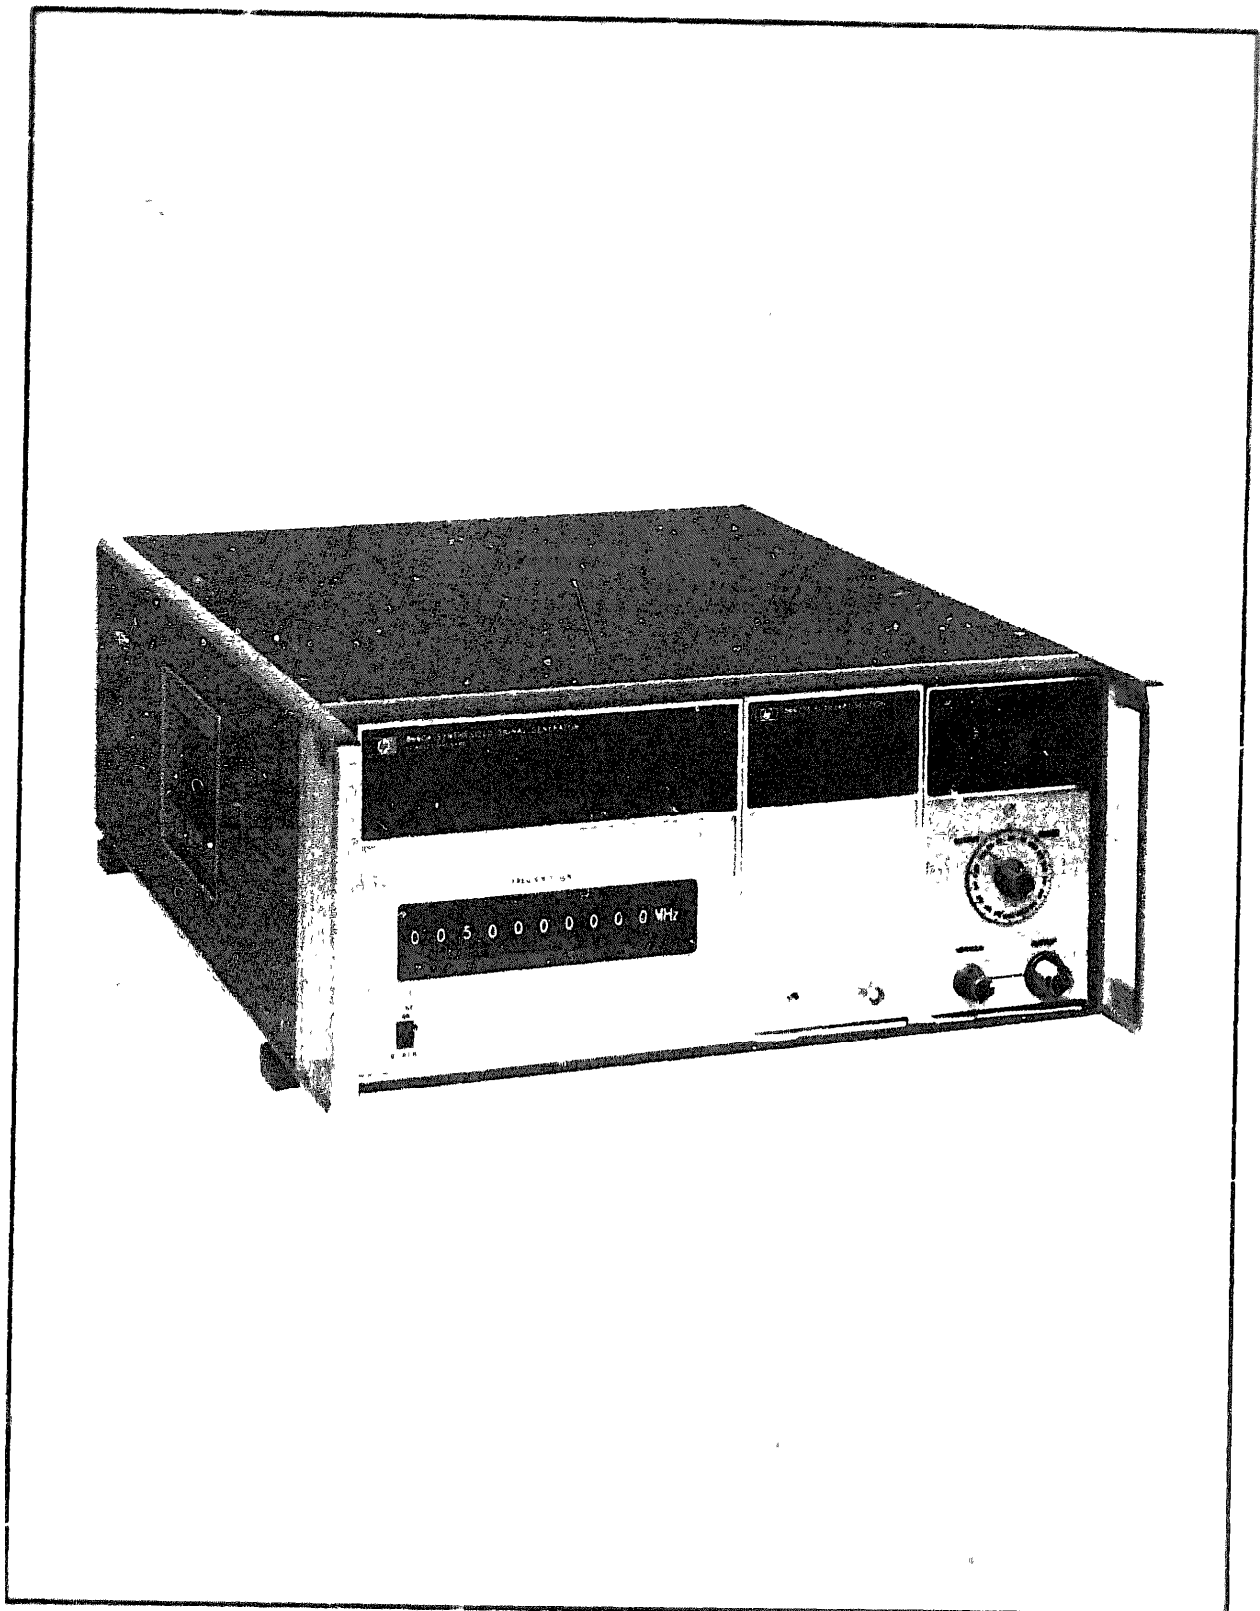


Figure 1-1. Model 88601A RF Section

SECTION I

GENERAL INFORMATION

1-1. INTRODUCTION

1-2. The Hewlett-Packard Model 86601A RF Section is an rf output plug-in designed for use with the Hewlett-Packard Model 8660 Synthesized Signal Generator mainframes.

1-3. This manual contains all information required to install, operate, test, adjust, and service the HP Model 86601A. This section covers instrument identification, specifications and other basic information.

1-4. Figure 1-1 shows a front view of the HP Model 86601A installed in the HP Model 8660A mainframe ready for use.

1-5. The various sections of this manual provide information as follows:

a. SECTION II, INSTALLATION, provides information relative to incoming inspection, power requirements, mounting, packing and shipping, etc.

b. SECTION III, OPERATION, provides information relative to operating the instrument.

c. SECTION IV, PERFORMANCE TESTS, provides information required to ascertain that the instrument is performing, in accordance with published specifications.

d. SECTION V, ADJUSTMENTS, provides information required to properly adjust and align the instrument after repairs are made.

e. SECTION VI REPLACEABLE PARTS provides ordering information for all parts and assemblies.

f. SECTION VII, MANUAL CHANGES, normally will contain no relevant information in the original issue of a manual. This section is reserved to provide backdated and updated information in manual revisions or reprints.

g. SECTION VIII, SERVICE, includes all information required to service the instrument.

1-6. INSTRUMENTS COVERED BY MANUAL

1-7. A ten-digit number (see Figure 1-2) is affixed to the rear panel of all Hewlett-Packard instruments. When the first five digits (serial prefix) of

your instrument matches serial prefix number 1335A, the contents of this manual applies directly to it. An instrument manufactured after the printing of this manual may have a different serial prefix number; if so, refer to Section VII and make the applicable manual changes.

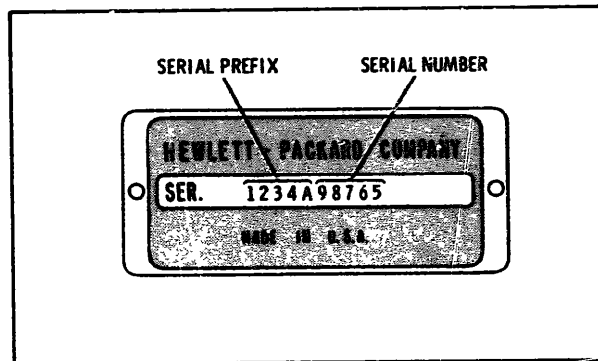


Figure 1-2. Instrument Identification

1-8. DESCRIPTION

1-9. The HP Model 86601A RF Section output plug-in provides a .01 to 109.999999 MHz output when installed in one of the HP Model 8660 mainframes. The output frequency may be selected in increments as low as 1 Hz or 100 Hz depending on the mainframe used.

1-10. The only operator controls on the Model 86601A are the attenuator (OUTPUT RANGE and VERNIER) controls. These controls provide a means of setting the rf output at any level between -146 dBm and +13 dBm. In remote operation these controls are inhibited; attenuation is controlled by a remote programming device in 1 dB and 10 dB steps.

1-11. Complete specifications for the Model 86601A are provided in Table 1-1.

1-12. OPTIONS

Option 001: No RF output attenuator. Output level adjustable from +13 to 0 dBm.

1-13. ACCESSORIES AVAILABLE

1-14. An extender cable, HP Part Number 11672-60001, is required to extend the plug-in for maintenance purposes. This extender cable is a part of the HP 11672A Service Kit, but may be ordered Separately.

1-15. TEST EQUIPMENT AND ACCESSORIES

1-16. Table 1-2 lists the test equipment and accessories recommended to test, adjust and service the Model 86601A. Refer to the Maintenance Allocation Chart in the Appendix for the required test equipment.

Table 1-1. Model 86602A Specifications

FREQUENCY CHARACTERISTICS	
<p>Frequency Range: 0.01 to 109.999999 MHz. Selectable in 1 Hz or 100 Hz steps (depending on mainframe used).</p> <p>Frequency Accuracy and Stability: CW frequency accuracy and long term stability are determined by the reference oscillator in the 8660 mainframe or by an external reference if used.</p> <p>Switching Time: Less than 5 ms to be within 100 Hz of any new frequency selected. Less than 100 ms to be within 5 Hz of any new frequency selected. Maximum stepping rate: 1 ms per step.</p> <p>Harmonic Signals: (Output terminated in 50 Ohms) All harmonically related signals are at least 40 dB below the selected output signal.</p>	<p>Spurious Signals: All nonharmonically related spurious signals are at least 80 dB below the selected output signal. Power line related spurious signals are at least 70 dB below the carrier.</p> <p>Signal-to-phase Noise Ratio: Greater than 50 dB in a 30 kHz band centered on the carrier excluding a 1 Hz band centered on the carrier.</p> <p>Residual FM: < 1 Hz rms in 2 kHz bandwidth centered on carrier.</p> <p>Signal-to-AM Noise Ratio: Greater than 70 dB in a 30 kHz band centered on the carrier, excluding a 1 Hz BW centered on the carrier.</p>
OUTPUT CHARACTERISTICS	
<p>Output Level: Continuously adjustable from +13 to -146 dBm (1.0 V to 0.01 μVrms) into 50-ohm resistive load; output attenuator calibrated in 10 dB steps from 1.0 V (+13 dBm) full scale to 0.03 μV (-137 dBm) full scale; vernier provides continuous adjustment between attenuator ranges; output level indicated on output level meter calibrated in volts and dBm into 50 ohms.</p> <p>Output Accuracy: (Local and Remote Modes) \pm 1 dB from +13 dBm to -66 dBm. \pm 2 dB from -67 dBm to -146 dBm.</p>	<p>Flatness: Output level variation with frequency is less than \pm 0.5 dB across the entire frequency range.</p> <p>Output Level Switching Time. Any level change may be accomplished in less than 50 ms. Any change to another level on the same attenuator range may be accomplished in 5 ms in Remote mode.</p> <p>Impedance: 50 ohms. SWR less than 2.0 on +10 dBm (1.0 V) attenuator range, less than 1.3 on 0 dBm (0.3 V) range and below</p>

Table 1-1. Model 86601A Specifications (Cont'd)

MODULATION CHARACTERISTICS (With the Model 86632A AM/FM Modulation Section)

Amplitude Modulation:*

Modulation Depth: 0 to 95% on all output ranges.

ON/OFF Ratio: At least 25 dB with output meter at 0 dB or above.

Carrier Envelope Distortion: (Modulating signal distortion < 0.3%). Less than 1% at 30% AM. Less than 3% at 70% AM. Less than 5% at 90% AM.

Incidental FM: Less than 0.2 radians peak at 30% AM.

Incidental FM: 0.2 x fmod.

AM 3 dB Bandwidth:

Center Frequency	0 to 30% AM	70% AM	90% AM
Fc < 0.4 MHz	200 Hz	125 Hz	100 Hz
0.4 < Fc < 4 MHz	10 kHz	6 kHz	5 kHz
Fc > 4 MHz	100 kHz	60 kHz	50 kHz

AM Distortion: (at 400 Hz and 1 kHz rates)

Frequency Range	30%	70%	90%
0.4-110 MHz	<1%	<3%	<5%

Typical distortion for other conditions is show in curves below.

The graph shows Modulation Depth (%) on the y-axis (0 to 100) and Modulation Rate on the x-axis. The x-axis has two scales: the top scale is in Hz (0 to 500 Hz) and the bottom scale is in kHz (0 to 500 kHz). Three curves are shown: 5% Distortion (top), 3% Distortion (middle), and 1% Distortion (bottom). All curves show a slight decrease in modulation depth as the modulation rate increases.

Typical 86601A AM distortion curves

Frequency Modulation:**

Rate: DC to 1 MHz.

Maximum Deviation: 1 MHz.

Incidental AM: With 75 kHz peak deviation at 1 kHz rate, AM modulation sidebands are < -60 dB.

The graph shows FM Rate (MHz) on the y-axis (0.1 to 1.0) and Peak Deviation (MHz) on the x-axis (0.1 to 1.0). Four regions are defined by diagonal lines: <1% Distortion (bottom-left), 2% Distortion, <3% Distortion, and 5% Distortion (top-right).

Typical 86601A FM distortion curves

GENERAL

Leakage:
Meets radiated and conducted limits of MIL-I-6181D.

Size: Plut-in to fit Model 8660 mainframe.

Weight: Net, 11 lbs (5 kg). Shipping 15 lbs (6,8 kg).

*Uncalibrated amplitude modulation is also possible with the Model 86631A Auxillary Section installed.

**In the FM mode, carrier frequency stability is determined by a free-running modulation oscillator in the Model 86632 Modulation Section. The oscillator can be phase-locked momentarily to remove drift by depressing the Model 86632A CF CAL button. Oscillator drift is less than 5 kHz/day after warmup.

Table 1-2. Test and Equipment and Accessories List

ITEM	MINIMUM SPECIFICATIONS	SUGGESTED MODEL	USE*
Digital Voltmeter	Accuracy: $\pm .2\%$ Range: .00 to 60 Volts	HP 3440A with HP 3442A plug-in	S
AC Voltmeter	5 kHz to 500 kHz 1 mV to 10 Volts	HP 403A	P
RF Millivoltmeter	1 MHz to 600 MHz 10 mV to 1 Volt	HP 411A	A
High Frequency dB Voltmeter	$\pm .2$ dB from 10 kHz to 500 kHz +20 to -20 dB	HP 400GL	A, P
Vector Voltmeter	$\pm .2$ dB from 1 MHz to 600 MHz +10 to -50 dB	HP 8405A	P, S
Broadband Sampling Voltmeter	$\pm 5\%$ from 100 kHz to 150 MHz +20 to -20 dB	HP 3406A	A, P
Oscilloscope	DC to 50 MHz, delayed sweep, time base 50 ns to 1s	HP 180A with HP 1801A and HP 1821A plug-ins	P, S
10 \div 1 divider probes (two)	10:1 divider 10 Megohm 10 pF	HP 10004	
Spectrum Analyzer	$\pm .5$ dB from 10 kHz to 110 MHz Measurement Accuracy ± 2 dB	HP 140S with HP 8553B and HP 8552B plug-ins	A, P
Spectrum Analyzer	± 1 dB from 1 MHz to 700 MHz Measurement Accuracy ± 2 dB	HP 140S with HP 8554L and HP 8552B plug-ins	A, P, S
Tracking Generator Spectrum Analyzer System	± 1.75 dB from 1 MHz to 700 MHz Measurement Accuracy ± 3.25 dB	HP 8444A with HP 8554L Spectrum Analyzer	A, P
Test Oscillator	10 Hz to 20 kHz .1 V to 1 V	HP 651B	A, P
Synthesized Signal Generator	± 1 Hz from .01 MHz to 110 MHz ± 2 dB from +10 to -90 dBm	HP 8660 with HP 86631A and HP 86601A plug-ins	P
Modulator Section	1 kHz FM with 1 MHz peak deviation	HP 86632A	P
Electronic Counter/ Frequency Converter	Range: 0-50 MHz; 0-500 MHz with the plug-in	HP 5245M with HP 5253B plug-in	A, P, S
Computing Counter	50 kHz to 50 MHz with a 1 ms count gate and and external trigger	HP 5360A with HP 5365A plug-in	P
Wave Analyzer	20 Hz to 10 kHz	HP 302A	P
Crystal Detector	100 kHz to 10 MHz	HP 8471A	P
Power Supply	0-10 volts	HP 721	P, S
Marked Card Programmer	Negative true output ground - true +5 V - false	HP 3260A (only) Opt 001	P, S
Frequency Meter/ FM Discriminator	100 kHz to 10 MHz with 1 volt sensitivity	HP 5210A	P
Variable Coaxial Attenuator	Refer to calibration curve	HP H38-355D (only)	A, P
Double Balanced Mixer	1 MHz to 110 MHz	HP 10514A	P
BNC Tee		UG 274 B/U	A, P, S

*USE - A = Adjustments; P = Performance Tests; S = Service

Table 1-2. Test Equipment and Accessories List (cont'd)

ITEM	MINIMUM SPECIFICATIONS	SUGGESTED MODEL	USE*
50 Ohm Dummy Load		HP 1250-0207	A, P, S
Variable Phase Generator	Distortion less than 3% Range: 1 kHz to 20 kHz	HP 203A	r
15 kHz Lowpass Filters (two)	Special	(see Figure 1-3)	P
100 kHz Lowpass Filter	Special	(see Figure 1-4)	P
40 dB Amplifier	Special	(see Figure 1-5)	P
Service Kit	Consisting of: Adapter: BNC female to OSM male Adapter: BNC female, Seaelectro female Adapter: BNC female, Seaelectro female Adapter: Right angle OSM male/female Seaelectro jack (printed circuit mount) Adapter: Seaelectro Tee Tool: Adjustment Cable: Extender, 66 pin, gray Cable: Extender, 42 pin, gray Cable Assy: Seaelectro male and female, 24 inches long, gray Cable Assy: Seaelectro male and female right angle connectors 24" long, red Cable Assy: Seaelectro right angle female, BNC male, 24" long, gray Cable Assy: Seaelectro male and female, 24" long, gray with blue stripe	HP 11672A 1250-1200 1250-1236 1250-1237 1250-1249 1250-1255 1250-1391 8830-0024 11672-60001 11672-60002 11672-60003 11672-60004 11672-60005 11672-60006	A, S

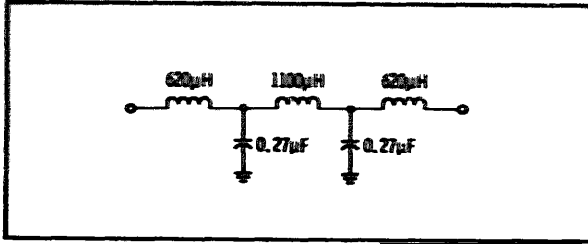


Figure 1-3. 15 kHz Lowpass Filter

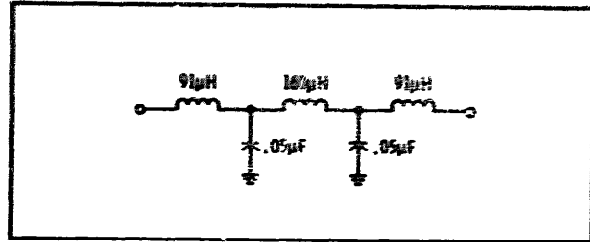


Figure 1-4. 100 kHz Lowpass Filter

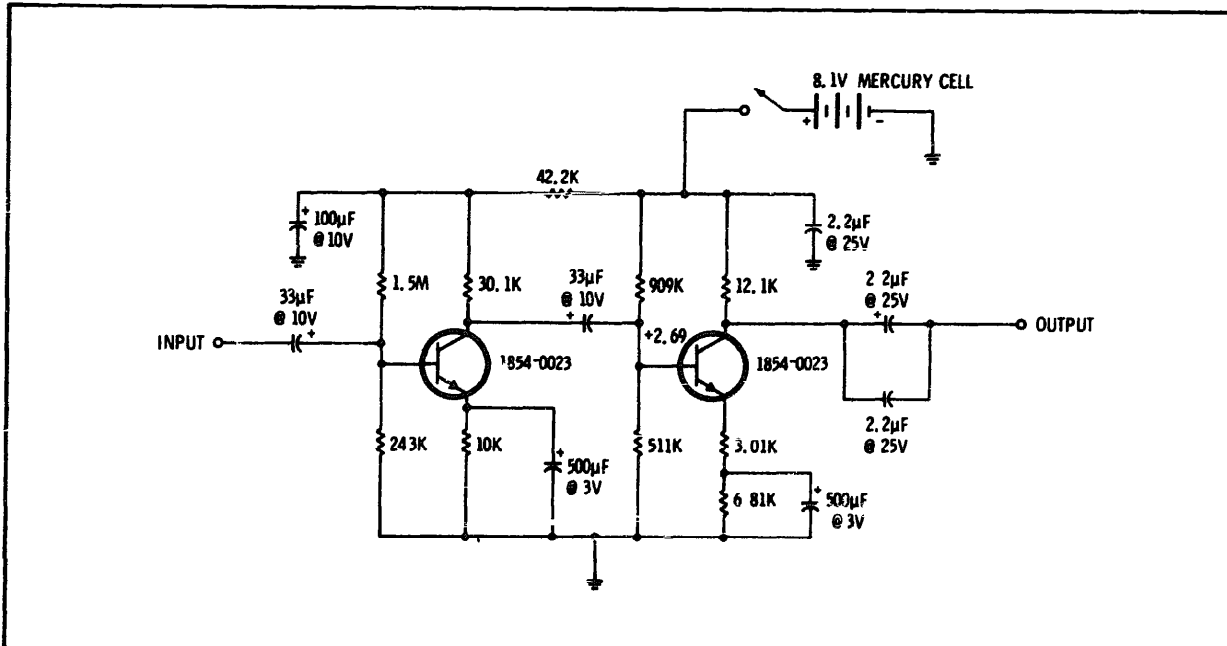


Figure 1-5. 40 dB Amplifier

Table 1-3. 40 dB Amplifier Specifications

Gain	44 dB at 25°C
Bandwidth	100 kHz (3 dB down)
Noise Bandwidth	157 kHz
Input Impedance	75 K
Output Impedance	12 K
Current Drain	260 μA
Output (Maximum)	1V
Dynamic Range	66 dB

SECTION II INSTALLATION

2-1. INITIAL INSPECTION

2-2. Mechanical Check

2-3. **If the shipping carton shows visible signs of damage when received, the carrier's agent should be present when the instrument is unpacked. If the agent is not present, retain the packaging material to aid in evaluating the cause of damage if the instrument is physically damaged or is not functioning properly.**

2-4. **Inspect the instrument** for physical damage such as bent or broken parts and dents or scratches. If damage is found refer to paragraph 2-7 for recommended claim procedure. If the instrument appears to be free of damage, perform the electrical check (see paragraph 2-5). The packaging material should be retained for possible future use.

2-5. Electrical Check

2-6. The electrical performance check consists of performing the performance test procedures in Section IV of this manual. These procedures enable the operator to determine that the instrument is, or is not, operating within the specifications listed in Table 1-1. The initial performance and accuracy of the instrument are certified as stated on the inside front cover of this manual. If the instrument does not operate as specified, refer to paragraph 2-7 for the recommended claim procedure.

2-7. Claim for Damage

2-8. If physical damage is found when the instrument is unpacked, notify the carrier and the nearest Hewlett-Packard Sales/Service office immediately. The HP Sales/Service office will arrange for repair or replacement without waiting for a claim to be settled with the carrier.

2-9. Deleted.

2-10. Preparation for Use

2-11. **There are no special requirements for preparation for use for the Model 86601A. Be sure that the main frame preparation for use requirements are met.**

2-12. Power Requirements

2-13. **All power required for operation of the Model 86601A is furnished by the mainframe.**

2-14. Operating Environment

2-15. **Cooling air is provided by a fan in the mainframe. This assures that the ambient temperature of the instrument stays within reasonable temperature limits when the instrument is operated at room temperature, between 0 and 55 degrees C (32 to 131 degrees F).**

2-16. Storage and Shipment

2-17. If the instrument is to be stored for an extended period of time it should be enclosed in a clean sealed enclosure.

2-18. Original Packaging

2-19. The same containers and materials used in factory packaging can be obtained through any Hewlett-Packard Sales/Service office 1

2-20. If the instrument is being returned to Hewlett-Packard for service attach a tag indicating the type of service required, return address, model number and full serial number. Also mark the container FRAGILE to assure careful handling.

2-21. In any correspondence refer to the instrument by model number and full serial number.

2-22. Other Packaging Material

2-23. The following general instructions should be followed when repackaging with commercially available materials :

a. Wrap the instrument in heavy paper or plastic. (If shipping to a Hewlett-Packard Service office or center, attach a tag indicating the type of service required, return address, model number and full serial number.)

b. **Use a strong shipping container. A double-wall carton made of 350 pound test material is adequate.**

c. **Use enough shock-absorbing material (three to four inch layer) around all sides of the instrument to provide firm cushion and prevent movement inside the carton. Protect the control panel with cardboard.**

d. **Seal the shipping container securely and mark it FRAGILE to assure careful handling.**

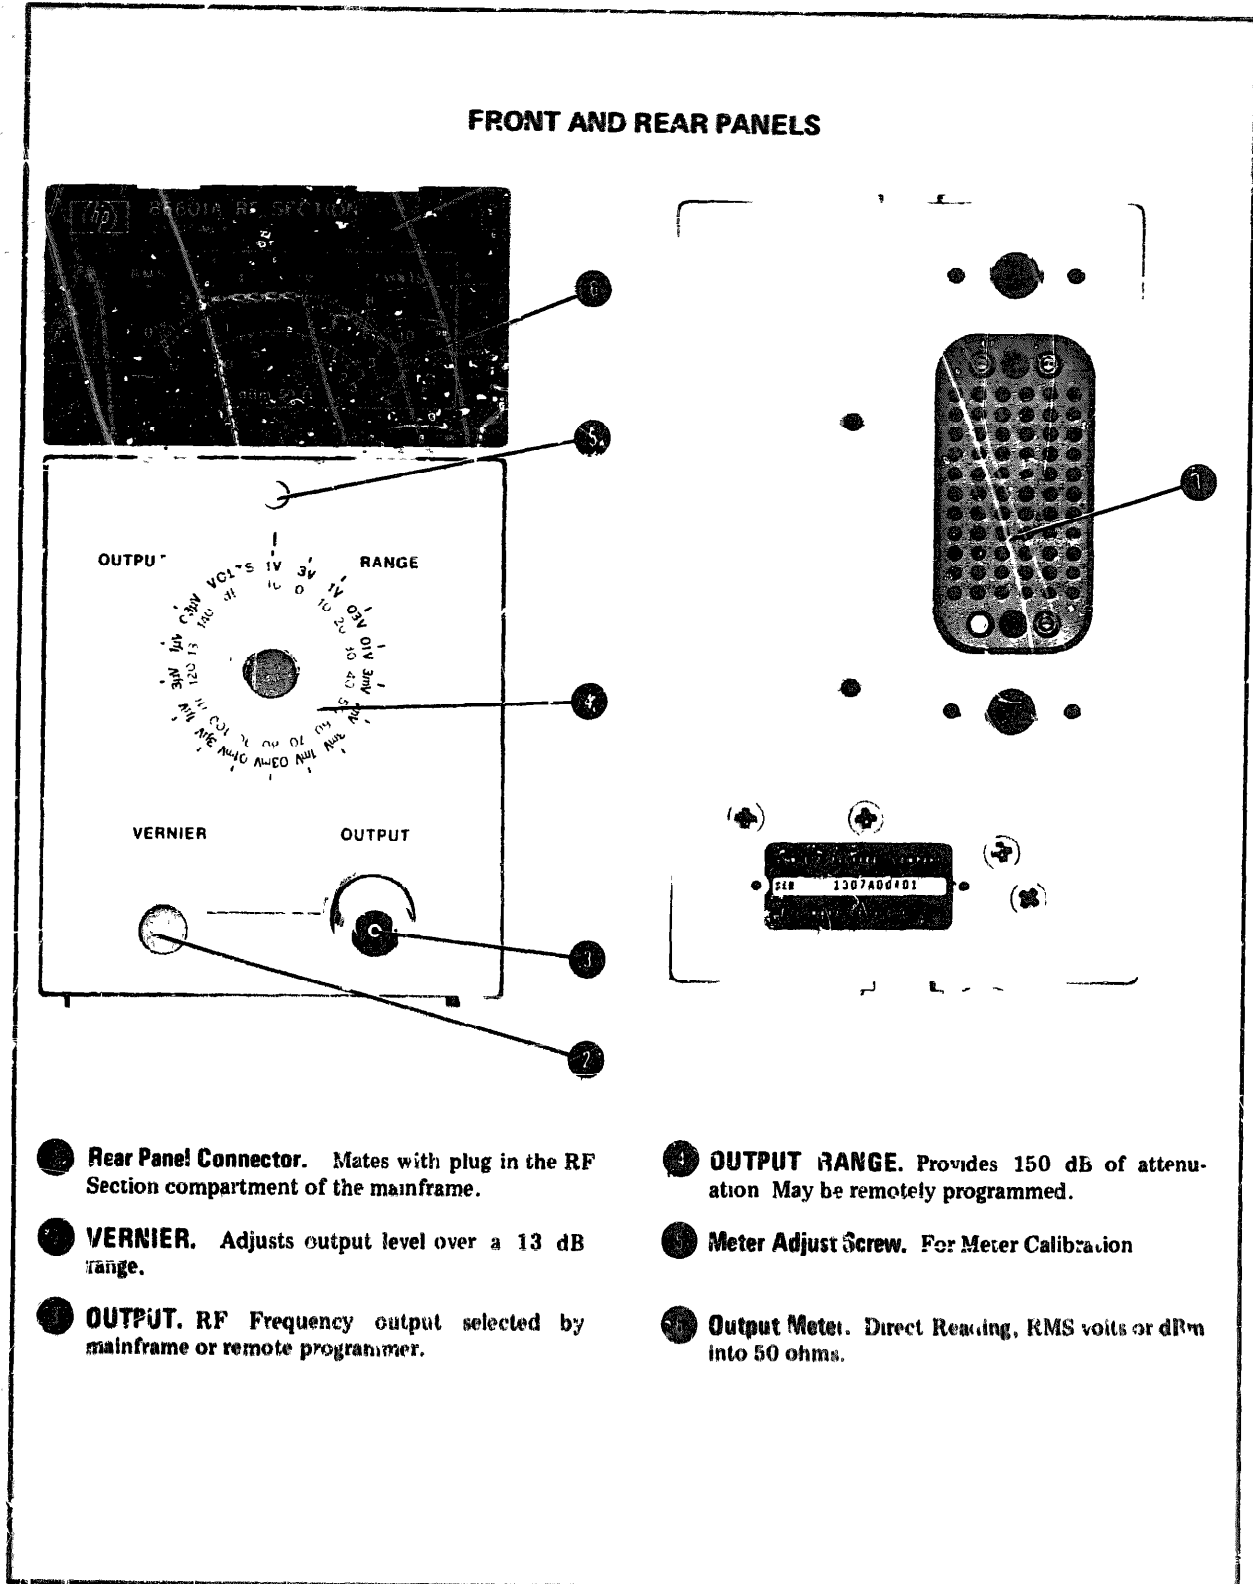


Figure 3-1. Front and Rear Panel Controls, Indicators and Connectors

SECTION III OPERATION

3-1. INTRODUCTION

3-2. This section provides operating instructions for the Hewlett-Packard Model 86601A RF Section.

3-3. The Model 86601A was designed to accept the precise digitally controlled signals from the Model 8660 mainframe and convert them to the selected output frequency by means of mixing and filtering. It will be necessary to have the Operating Manuals for the mainframe and the modulation section (if used) to efficiently operate the instrument.

NOTE

If a modulation plug-in section is not used it will be necessary to have the Model 86631A Auxiliary Section in place in the modulation plug-in drawer.

3-4. PANEL FEATURES

3-5. Front and rear panel controls, indicators and connectors of the Model 86601A are shown in Figure 3-1.

3-6. OPERATING PRINCIPLES

3-7. The Model 86601A may be operated by front panel controls in the local mode or externally programmed in the remote mode.

NOTE

The remote mode is selected by the external programming device which places a ground on pin 5 of the blue ribbon connector (J3) on the rear panel of the Model **8660A/B mainframe**.

3-8. The only operator controls on the Model 86601A are the attenuator controls. These controls enable the operator to set the output level at any point between -146 and $+13$ dBm.

3-9. The front panel attenuator controls are inhibited when the instrument is operated in the remote mode.

NOTE

Model 86601A Option 001 instruments do not include the 150 dB (10 dB steps) programmable attenuator.

3-10. In Option 001 instruments the output of the Model 86601A may be adjusted, in the local mode, from $+13$ to 0 dBm by means of the **VERNIER** control; in the remote mode the output may be reduced by 9 dB in 1 dB steps.

3-11. OPERATOR'S CHECKS

3-12. During checkout at the factory the Model 86601A RF Section is adjusted for proper operation. No adjustment should be required when the instrument is received.

3-13. The Operator's Checks specified in Section III of the mainframe are adequate for checking the output frequency of the Model 86601A.

3-14. If a plug-in Modulation Section is being used, the checks specified in Section III of the Modulation Section Manual should also be performed.

SECTION IV
PERFORMANCE TESTS

4-1. INTRODUCTION

4-2. This section provides instructions for performance testing the Model 86601A RF Section plug-in. It is assumed in all tests that the Model 86601A is interconnected with a mainframe that is known to be functioning properly.

4-3. Purpose.

4-4. The performance test procedures are used to check instrument performance for incoming inspection and periodic evaluation. The tests are designed to verify published specifications for the instrument. Each test applies directly to a listed specification (see Table I-1).

4-5. **Each performance test procedure begins by quoting the specification which it verifies. Next, a description of the test and any special instructions are listed.**

4-6. **Test Equipment Required** The test equipment required for performance testing is listed in Table 1-2 and in the individual tests. Test instruments other than those listed may be used providing their performance equals or exceeds the specifications listed in Table 1-2.

4-7. Front Panel Checks and Adjustments. Refer to paragraph 3-11, Operator's Checks.

4-8. PERFORMANCE TESTS

PERFORMANCE TESTS

4-9. FREQUENCY RANGE

SPECIFICATION: 0.01 to 109.999999 MHz selectable in 1 Hz steps (OPT 004 mainframes; 100 Hz steps).

DESCRIPTION: This test verifies the output frequency range of the Model 86601A RF Section plug-in.

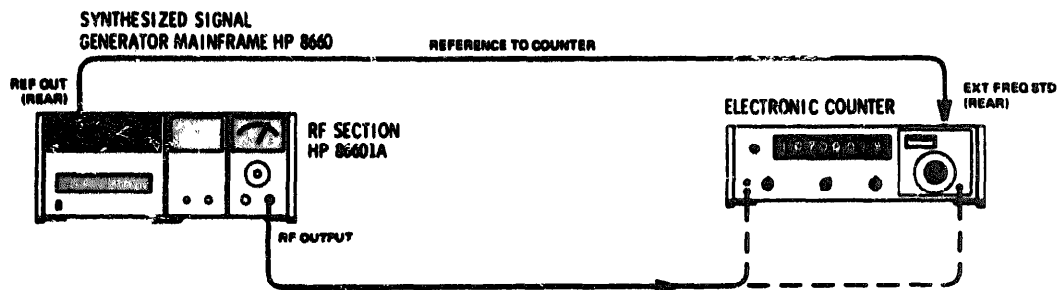


Figure 4-1. Frequency Range and Accuracy Test Setup

RECOMMENDED TEST EQUIPMENT:

Electronic Counter/Frequency Converter Plug-in HP 5245M/5253B

PROCEDURE:

1. **Connect the mainframe REFERENCE OUTPUT to the counter EXT STD FREQ input and set the counter mode switch to EXT STD.**
2. **Set the mainframe center frequency to 10.000 kHz and check the output frequency with the counter (Allow for the accuracy of the counter used, model recommended is specified at ±1 count)**

PERFORMANCE TESTS

4-9. **FREQUENCY RANGE (cont'd)**

3. Set the center frequency to 109.999999 MHz (Opt. 004 mainframe set to 109.9999 MHz) at 0 dBm and check with the counter and the frequency converter plug-in.

4-10. **FREQUENCY ACCURACY AND STABILITY**

SPECIFICATION: CW frequency accuracy and long term stability are determined by the crystal oscillator in the mainframe or by an external reference standard.

NOTE

If there is any reason to doubt the accuracy or stability of the internal crystal oscillator refer to Section IV of the mainframe manual.

4-11. **OUTPUT ACCURACY AND LEVEL**

SPECIFICATION: ± 1 dB from +13 dBm to -66 dBm and ± 2 dB from -67 dBm to -146 dBm.
Output Level: +13 dBm to -146 dBm into 50 ohms.

DESCRIPTION: This test checks output amplitude accuracy from +10 dBm to -70 dBm by comparing the internal attenuator to a precision external attenuator.

NOTE

All sections of the internal programmable attenuator are checked separately. In addition, the 10 dB, 20 dB, and 40 dB sections are checked in all possible combinations. The sum of the inaccuracies of the -60 dBm and -70 dBm tests should not exceed ± 2 dBm.

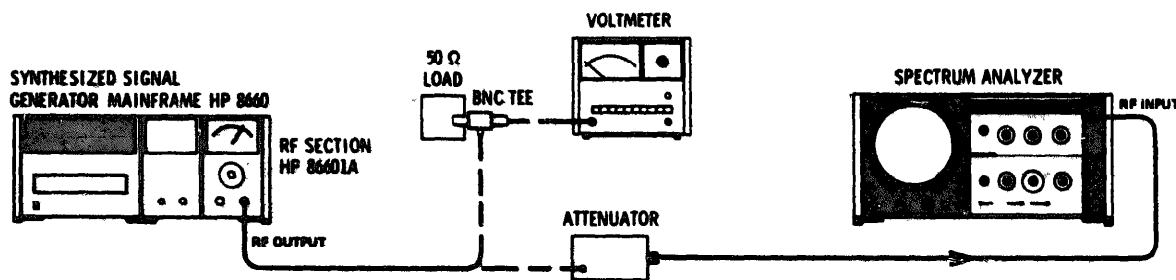


Figure 4-2. Output Accuracy and Level Test Setup

RECOMMENDED TEST EQUIPMENT:

Broadband Sampling Voltmeter	HP 3406A
50 Ohm Termination	1250-0207
Variable Coaxial Attenuator (Precision)	HP H38-355D
BNC Tee	UG 274B/U
Spectrum Analyzer	HP 8553B/8552B/140S

PROCEDURE:

1. Set the Model 86601A OUTPUT RANGE and VERNIER to +10 dBm.
2. Set the mainframe center frequency to 30 MHz.

PERFORMANCE TESTS

4-11. OUTPUT ACCURACY AND LEVEL (cont'd)

- 3 . **Connect the rf output of the Model 86601A to the sampling voltmeter. Terminate with 50 ohms. The sampling voltmeter should indicate +10 dBm ±1 dBm (if it does not, refer to paragraph 5-14 and calibrate the metering circuit). Change VERNIER in 1 dB increments and verify that the sampling voltmeter indicates the correct level ±1 dB. Disconnect the sampling voltmeter.**
4. Set the external attenuator to 50 dB and connect it between the Model 86601A OUTPUT and the Spectrum Analyzer RF INPUT. Set the Model 86601A output level to +10 dBm.
5. Set a convenient reference level on the Spectrum Analyzer with the vertical scale (LOG 2 dB/Div).
6. Change the external attenuator to 70 dB and the Model 86601A OUTPUT RANGE to 0 dBm. The Spectrum Analyzer display should be within ± 1 dB of the established reference level.
7. Continue decreasing the attenuation of the external attenuator and the Model 86601A OUTPUT RANGE in 10 dB steps until the OUTPUT RANGE is set to -70 dBm and the external attenuator is set to 0 dB. The spectrum Analyzer display should remain within ±1 dB for levels down to -70 dBm. These tests assure the specification of ±2 dB from -67 dBm to -146 dBm.

4-12. OUTPUT FLATNESS

SPECIFICATION: Output flatness: Output level variations with frequency ± 0.5 dBm across the frequency range.

DESCRIPTION: This test verifies flatness of the output signal from 10 kHz to 109.9 MHz.

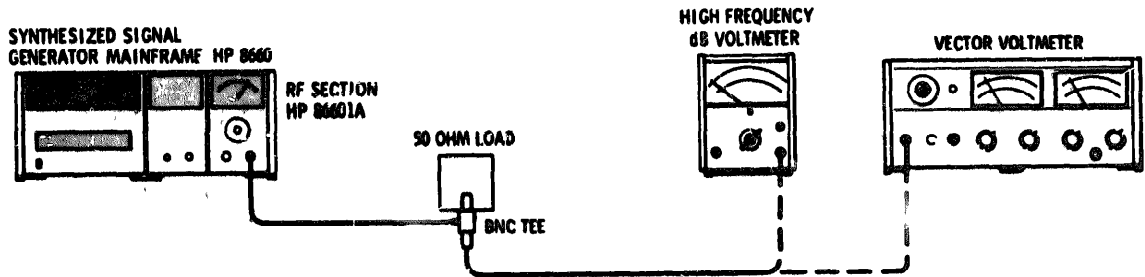


Figure 4-3. Output Flatness Test Setup

RECOMMENDED TEST EQUIPMENT:

High Frequency dB Voltmeter	HP 400 GL
Vector Voltmeter	HP 8405A
50 Ohm Dummy Load	HP 1250-0207
BNC Tee	UG274B/U

PROCEDURE:

- 1 . **Set the mainframe center frequency to 10 kHz.**
- 2 . **Set the Model 86601A OUTPUT RANGE and VERNIER for a front panel meter reading of +10 dBm.**

PERFORMANCE TESTS

4-12. OUTPUT FLATNESS (con'd)

3. **Connect the Model 86601A OUTPUT to the High Frequency dB Voltmeter through a BNC Tee terminated in 50 ohms.**
4. **Set the meter RANGE switch for a convenient mid-scale reading** on the High Frequency dB voltmeter.
5. **Change the mainframe center frequency to 50 kHz, then 100 kHz, and finally 500 kHz. The level read on the High Frequency dB Voltmeter should remain** within a ± 0.5 dB window.
6. **Disconnect the High Frequency dB Voltmeter and connect the Vector Voltmeter to the Model 86601A OUTPUT (terminated in 50 ohms).**
7. **Select** a Vector Voltmeter range that will provide a convenient mid-scale reference with the mainframe center frequency set to 1 MHz.
8. **Change the** mainframe center frequency to 10 MHz, then 50 MHz, and finally 109.9 MHz. The reference level indicated on the Vector Voltmeter should remain within the ± 0.5 dB window.

4-13. IMPEDANCE: 50 OHMS

SPECIFICATION: SWR less than 2:1 on +10 dBm output range; less than 1.3:1 on 0 dBm output range and below.

DESCRIPTION: The Model 86601A RF OUTPUT is measured with a voltmeter, first with no external load, then with a 50 ohm external dummy load. The source resistance R_S is determined and the SWR is calculated by dividing R_O by R_S (or R_S by R_O if R_O is $< R_S$).

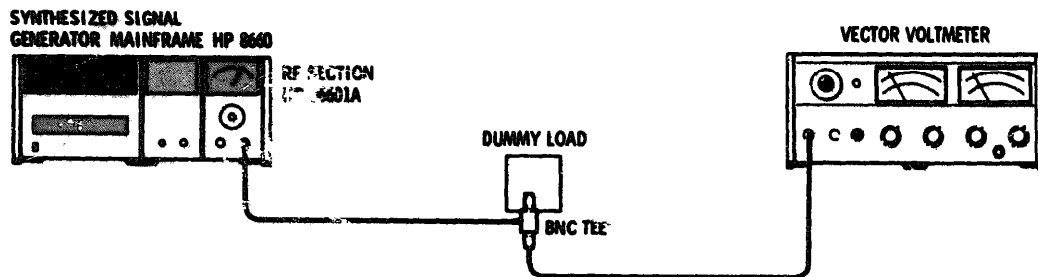


Figure 4-4. Impedance Test Setup

RECOMMENDED TEST EQUIPMENT:

Vector Voltmeter	HP 8405A
50 Ohm Dummy Load	HP 1250-0207
BNC Tee	UG 274 B/U

PROCEDURE:

1. **Set the mainframe center frequency to 50 MHz. Set the Model 86601A OUTPUT RANGE to +10 dBm.**

PERFORMANCE TESTS

4-13. IMPEDANCE: 50 OHMS (cont'd)

2. **Connect the Model 86601A OUTPUT to the Vector Voltmeter through a BNC Tee (unterminated).**

3. Record the RF output level.

V_{OC} _____ mVrms

4. Terminate the BNC Tee 50 ohms.

5. Record the RF output level.

V_1 _____ mVrms

6. The Model 86601A source resistance is found by using the following formula:

$$R_s = \frac{R_o V_{oc}}{V_1} - R_o$$

V_{oc} = 1st measurement (step 3)

V_1 = 2nd measurement (step 5)

R_o = 50 ohm termination

7. Determine SWR. $SWR = \frac{R_o}{R_s}$ or $\frac{R_s}{R_o}$. SWR should be < 2.0:1.

8. Record SWR

9. Reduce the Model 86601A OUTPUT RANGE to 0 dBm.

10. Repeat steps 2 through 8 at 0 dBm. SWR should be < 1.3:1.

11. Record SWR

4-14. HARMONIC SIGNALS

SPECIFICATION: With the Model 86601A terminated in 50 ohms all harmonically related signals are at least 40 dB below the selected frequency.

DESCRIPTION: This test checks second and third harmonics across the entire output frequency range of the Model 86601A.



Figure 4-5. Harmonic Signal Test Setup

PERFORMANCE TESTS

4-14. HARMONIC SIGNALS (cont'd)

RECOMMENDED TEST EQUIPMENT:

Spectrum Analyzer HP 8554L/8552B/140S

PROCEDURE:

1. Set the Model 86601A OUTPUT RANGE to -10 dBm and set the VERNIER control to +3 dBm.
2. Connect the Model 8660A OUTPUT to the Spectrum Analyzer RF INPUT and set the Spectrum Analyzer INPUT ATTENUATION to 20 dB.
3. Check second and third harmonics at the following center frequencies: 10 kHz, 400 kHz, 4 MHz, 10 MHz, and 109.9 MHz. All harmonic signals should be more than 40 dB below the level of the fundamental frequencies.

4-15. SPURIOUS SIGNALS

SPECIFICATION: All nonharmonically related spurious signals are at least 80 dB below the selected output signal. Power line related spurious signals are at least 70 dB below the carrier.

DESCRIPTION: This test checks for common spurious signals by mixing the signal from the unit under test with a reference signal offset by 1 kHz. The Wave Analyzer measures common spurious signals generated in the unit under test.

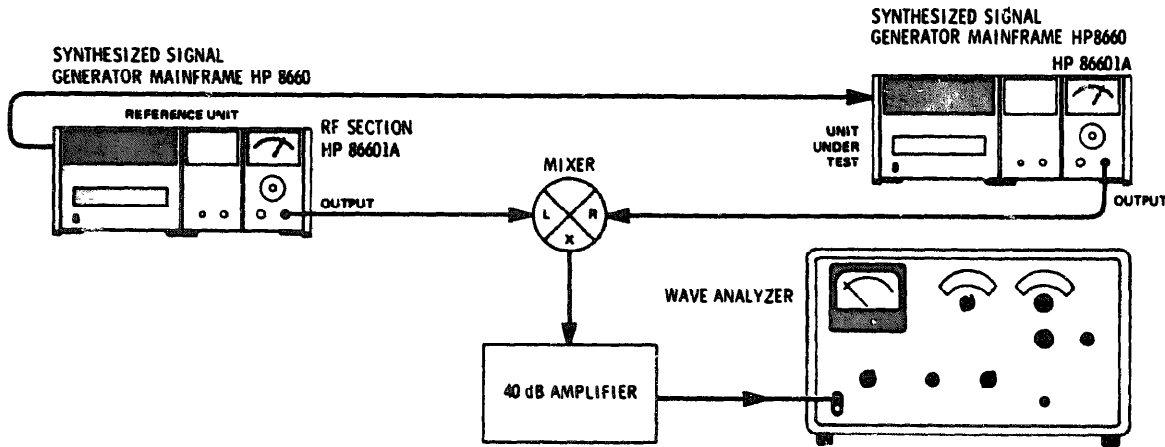


Figure 4-6. Spurious Signal Test Setup

RECOMMENDED TEST EQUIPMENT:

Synthesized Signal Generator HP 8660 86601A/86631A
 Double Balanced Mixer HP 10514A
 Wave Analyzer HP 302A
 40 dB Amplifier (special) see details in Figure 1-5.

PROCEDURE:

1. Connect the rear panel REFERENCE OUTPUT from the reference unit to the rear panel REFERENCE INPUT of the unit under test and set the REFERENCE SELECTOR of the unit under test to EXT.

PERFORMANCE TESTS

4-15. SPURIOUS SIGNALS (cont'd)

2. Connect the equipment as shown in Figure 4-6.
3. Set the reference unit center frequency to 50.001 MHz and the output level to +13 dBm.
4. Set the center frequency of the unit under test to 50 MHz and the output level to -87 dBm.
5. Set the Wave Analyzer; mode switch to NORMAL and scale value to RELATIVE.
6. Set the wave Analyzer to 1 kHz and adjust levels for a 0 dB reading on the scale.
7. Set the unit under test OUTPUT RANGE and VERNIER to -7 dBm.
8. Set the reference unit and the unit under test as shown in Table 4-1 and note that spurious levels are lower than -80 dB (0 dB on Wave Analyzer scale).
9. Corrected reading is -80 dB minus the Wave Analyzer meter reading.

Table 4-1. Spurious Signal Checks

Unit Under Test MHz	Reference Unit MHz	Spurious Level
101	47.001	_____
109.99	20.031	_____
103.1	81.401	_____
29.595	29.451	_____
29.595	29.801	_____
29.595	29.587	_____

4-16. SIGNAL-TO-PHASE NOISE **RATIO**

SPECIFICATION: Lower than -50 dB in a 30 kHz **band centered on the carrier excluding a 1 Hz band** centered on the carrier.

DESCRIPTION: This test checks the signal-to-phase noise ratio across the Model 86601A output frequency range. The AC Voltmeter specified excludes 1 Hz.

4-10. SIGNAL-TO-PHASE NOISE RATIO

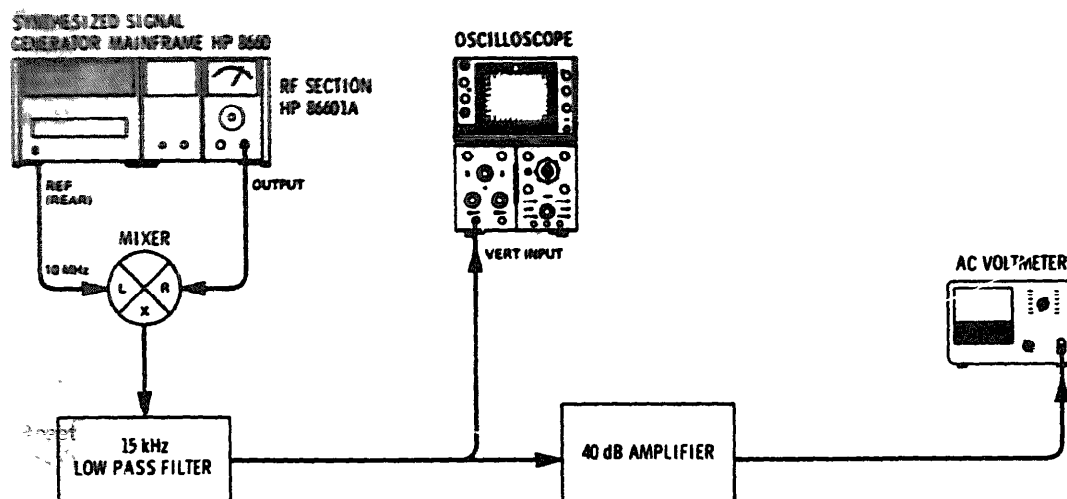


Figure 4-7. Signal-to-Phase Noise Test Setup

RECOMMENDED TEST EQUIPMENT:

Oscilloscope	HP 180A/1801A/1821A
Double Balanced Mixer	HP 10514A
AC Voltmeter	HP 403A
40 dB Amplifier (special) see details in Figure 1-5.	
Low Pass Filter (special) see details in Figure 1-3.	

PROCEDURE:

1. **Connect** the equipment as shown in Figure 4-7.
2. **Set the** mainframe center frequency to 10.001 MHz. Set the Model 86601A OUTPUT RANGE to -60 dBm and the VERNIER for a meter reading of +3 dBm.
3. Set the RF Voltmeter Function Switch to 1 CPS-1 MC and record the reading. _____ dB
4. Set the mainframe center frequency to 10.000100 MHz and the OUTPUT RANGE to -10 dBm.
5. Adjust the oscilloscope for an **eight-division amplitude display of the 100 Hz signal.**
6. **Set the mainframe center frequency to 10.0000001 MHz and note that the oscilloscope baseline alternately rises and falls over the eight-division display.**
7. **Reset the mainframe center frequency to 10.000000 MHz at a time that will cause the oscilloscope baseline trace to stop at the center graticule line.**
8. **Repeat steps 6 and 7 until the oscilloscope baseline trace is stopped within $\pm 1/10$ div. of the center graticule line.**
9. **Read the noise level on the AC Voltmeter. Noise = -50 dB \pm the difference in meter readings. The meter reading should be lower than the reference established in step 3. (Example: Meter reading is 3 dB lower, noise is -53 dB.)**
10. **Noise should be lower than -50 dB. Record noise level.** _____ dB

PERFORMANCE TESTS

4-17. SIGNAL-TO-AM NOISE RATIO

SPECIFICATION: Lower than -70 dB in a 30 kHz band centered on the carrier excluding a 1 Hz bandwidth centered on the carrier.

DESCRIPTION: This test checks AM noise across the Model 86601A frequency range. The AC voltmeter specified excludes 1 Hz.

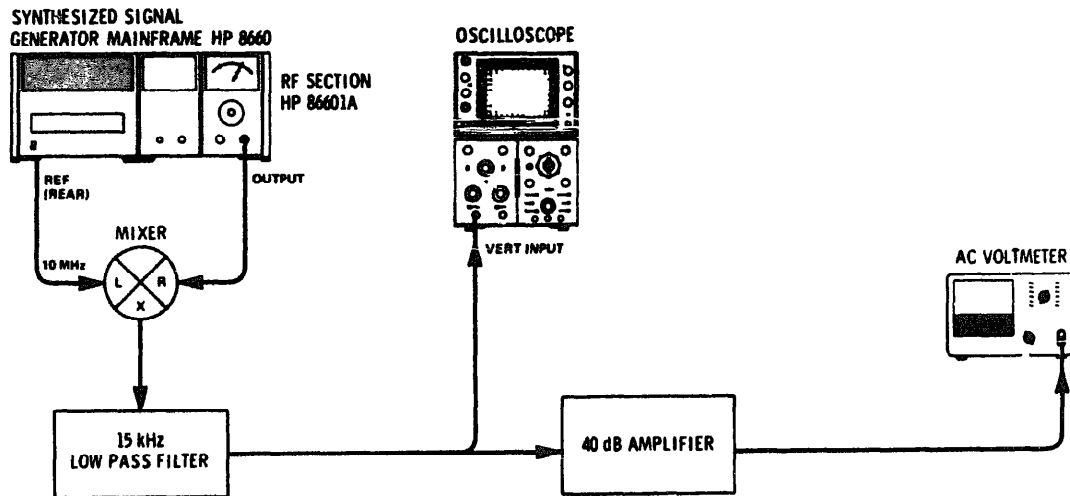


Figure 4-8. Signal-to-AM Noise Ratio Test Setup

RECOMMENDED TEST EQUIPMENT

Oscilloscope	HP 180A/1801A/1821A
Double Balanced Mixer	HP10514A
AC Voltmeter	HP 403A
40 dB Amplifier (special); see details in Figure 1-5.	
Low Pass Filter (special); see details in Figure 1-3.	

PROCEDURE:

1. Connect the equipment **as shown in Figure 4-8.**
2. **Set the mainframe center frequency to 10.001000 MHz**
3. **Set the Model 86601A OUTPUT RANGE to -80 dBm and the VERNIER to +3 dBm**
4. **Set the AC Voltmeter range for an on-scale reading with the function switch set to 1 CPS 1 MC**
Record the Meter Reading _____ dB
5. **Set the mainframe center frequency to 10.000100 MHz and the OUTPUT RANGE to -10 dBm**
6. **Adjust the oscilloscope for an eight-division amplitude display of the 100 Hz signal**
7. **Set the mainframe center frequency to 10.000001 MHz and note that the oscilloscope baseline alternately rises and falls over the eight division display**

PERFORMANCE TESTS

4-17. SIGNAL-TO-AM NOISE RATION (cont'd)

- 8 . **Reset the mainframe center frequency to 10.00000 MHz** at a time that will cause the oscilloscope baseline trace to stop at the top graticule line of the CRT.
- 9 . **Repeat steps 7 and 8 until the oscilloscope baseline trace is stopped at the top graticule line $\pm 1/10$ div.**
- 10 . **Read the noise level** on the AC Voltmeter. Noise = -70 dB \pm the difference in meter readings. The **meter reading should be lower than the reference established in step 4.** Example: Meter reading is 3 dB lower, noise level is **-73 dB.**
- 11 . **Noise** should be lower than -70 dB.

Record Noise Level dB

4-18. RESIDUAL FM

SPECIFICATION: <1 Hz rms in 2 kHz bandwidth centered on the carrier.

DESCRIPTION: Residual FM is checked indirectly in the checks for signal-to-phase noise across the Model 86601A frequency range.

4-19. AMPLITUDE MODULATION

SPECIFICATION: 0 to 95% on all output ranges (with Model 86632A or 86631A Modulation Section in place).

DESCRIPTION: This test checks AM frequency response with the mainframe center frequency set to 50 MHz, 3 MHz, and 300 kHz. AM rate is provided from a test oscillator and measured on a Spectrum Analyzer and Oscilloscope.

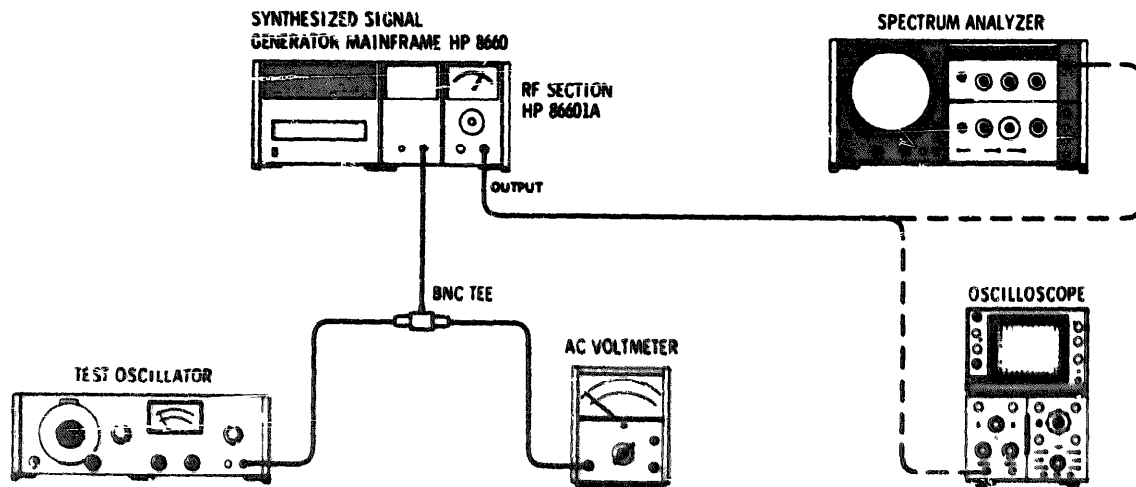


Figure 4-9. Amplitude Modulation Test Setup

PERFORMANCE TESTS

4-19. AMPLITUDE MODULATION (cont'd)

RECOMMENDED TEST EQUIPMENT:

Spectrum Analyzer	HP 8553B/8552B/140S
High Frequency dB Voltmeter	HP 400 GL
Oscilloscope	HP 180A/1801A/1821A
Test Oscillator	HP 651B
BNC Tee	UG 274 B/U

PROCEDURE:

1. Connect the equipment as shown in Figure 4-9.
2. Set the Spectrum Analyzer as follows: INPUT ATTENUATION 30 dB, BANDWIDTH 1 kHz, SCAN WIDTH 10 kHz, CENTER FREQUENCY 50 MHz, LOG-LINEAR 2 dB/Div, SCAN TIME 20 mSec/Div and VIDEO FILTER to OFF,
3. Set the mainframe center frequency to 50 MHz and the Model 86601A output level to +3 dBm.
4. Set the Model 86631A AM switch to ON (if the Model 86632A is being used, set the MODE switch to AM and the SOURCE switch to EXTERNAL AC and AM to 50%).
5. Set the Test Oscillator output to 10 kHz at .5 Vrms as read on AC Voltmeter.
6. Adjust the spectrum analyzer until the carrier is at the top graticule line. Amplitude Modulation should be 50% ±5% with sidebands down -12 dB ±0.5 dB.
7. Adjust the Test Oscillator frequency from 10 Hz to 50 kHz. The AM % should be flat ± 4 db from 10 Hz to 20 kHz and down 3 dB at about 50 kHz.
8. Set the mainframe center frequency to 3 MHz and analyze scan width to 2 kHz. Adjust the Test Oscillator frequency from 10 Hz to 10 kHz. The side bands should be flat ±.2 dB to 2 kHz; down 2 dB at about 5 kHz; down 8 dB at about 10 kHz.
9. Set the mainframe center frequency to 300 kHz. Disconnect the rf OUTPUT from the Spectrum Analyzer and connect it to the Oscilloscope.
10. **Set the Test Oscillator to 25 Hz and adjust the Oscilloscope for 8 division vertical display of the envelope only. Set the Test Oscillator frequency to 100 Hz. The Oscilloscope display should be > 7 divisions.**

4-20. AMPLITUDE MODULATION: ON/OFF RATIO

SPECIFICATION: At least 25 dB with output meter at 0 dBm or above.

DESCRIPTION: This test verifies the Amplitude Modulation ON/OFF ratio of the Model 86601. AM is shut off with a power supply and rf output level change is measured on an AC Voltmeter

PERFORMANCE TESTS

4-20. AMPLITUDE MODULATION: ON/OFF RATIO

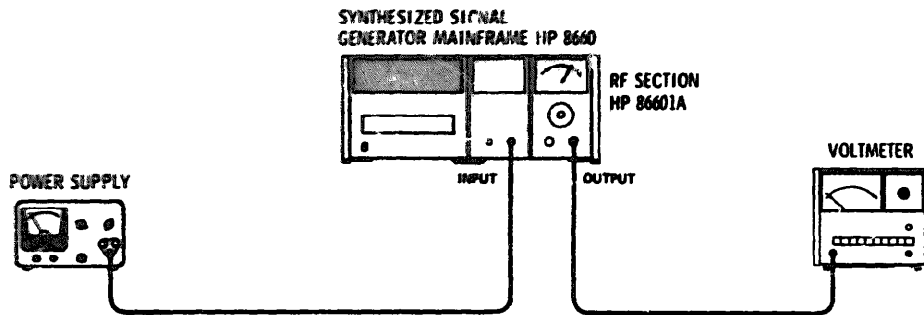


Figure 4-10. Amplitude Modulation ON/OFF Ratio Test Setup

RECOMMENDED TEST EQUIPMENT:

Broadband Sampling Voltmeter
Power Supply

HP 8406A
HP 721A

PROCEDURE:

1. Connect the equipment as shown in Figure 4-10 (with the Model 86631A AM switch off).
2. Set the power supply to +4 Vdc.
3. Set the mainframe center frequency to 50 MHz and output level of the Model 86601A to +13 dBm. Set a reference point on the Voltmeter.
4. Switch the Model 86631A AM switch to ON.
5. The Model 86601A output level should drop to <-12 dBm. (25 dB ON/OFF ratio).

4-21. **AMPLITUDE MODULATION CARRIER ENVELOPE DISTORTION**

SPECIFICATION: Envelope distortion should be less than 1% at 30% AM. Less than 3% at 70% AM. Less than 5% at 90% AM.

DESCRIPTION: Amplitude Modulation distortion is checked at 30%, 70% and 90%.

PERFORMANCE TESTS

4-21. AMPLITUDE MODULATION CARRIER ENVELOPE DISTORTION (cont'd)

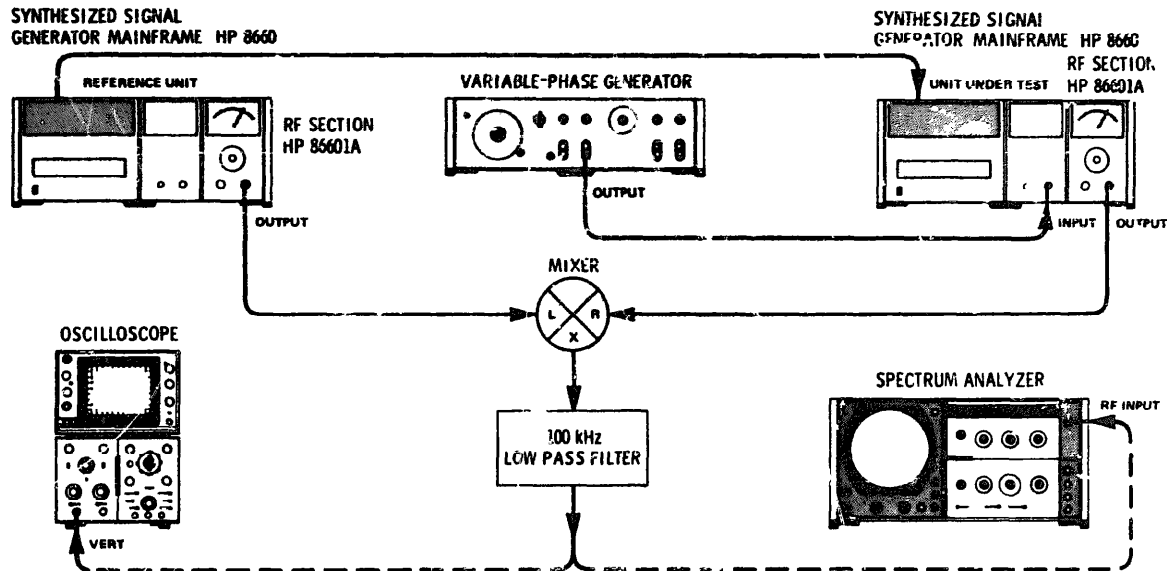


Figure 4-11. Amplitude Modulation Carrier Envelope Distortion Test Setup

RECOMMENDED TEST EQUIPMENT:

Double Balanced Mixer	HP 10514A
Spectrum Analyzer	HP 8553B/8552B/140S
Synthesized Signal Generator	HP 8660A/B/866C1A/86631A
Variable Phase Generator	
Oscilloscope	HP 180A/1801A/1821A
Low Pass Filter 100 kHz (special); see details in Figure 1-4.	

PROCEDURE:

1. Connect the equipment as shown in Figure 4-11.
2. Connect the rear panel **REFERENCE OUTPUT** from the reference unit to the rear panel **REFERENCE INPUT** of the unit under test and set the **REFERENCE SELECTOR** of the unit under test to **EXT**.
3. **Set the mainframe center frequency of the unit under test to 109.9 MHz. Set the Model 86601A under test OUTPUT RANGE to -20 dBm and the VERNIER to +3 dBm.**
4. **Connect the Variable-Phase Generator output to the Model 86631A AM input. Set the Variable Phase Generator output to 10 kHz and place the Model 86631A AM switch in the OFF position.**
5. **Set the reference mainframe center frequency to 109.91 MHz and the Model 86601A output level to +13 dBm.**
6. **Set the DC Coupled Oscilloscope to .005 V/Div.**
7. **Set the Spectrum Analyzer controls as follows: INPUT ATTENUATION 40 dB, SCAN WIDTH PER DIVISION 10 kHz, SCAN TIME PER DIVISION 20 mSec, BANDWIDTH 1 MHz, LOG SCALE 10 dB/Div. Adjust vertical level until the 10 kHz signal is at the top graticule line of the Spectrum Analyzer. Set the Oscilloscope for 8 divisions of vertical deflection.**

PERFORMANCE TESTS

4-21. AMPLITUDE MODULATION CARRIER ENVELOPE DISTORTION (cont'd)

8. Set the reference unit mainframe center frequency to 109.900001 MHz and note that the Oscilloscope baseline alternately rises and falls over the 8-division display.
9. Reset the reference unit mainframe center frequency to 109.900000 MHz at a time that will cause the Oscilloscope baseline trace to stop at the top graticule line of the CRT.
10. Repeat steps 8 and 9 until the oscilloscope baseline trace is stopped at the top graticule line $\pm 1/10$ div.
11. Set the Model 86631A EXTERNAL AM switch to ON and adjust the Variable Phase Generator output level until the 10 kHz signal on the Spectrum Analyzer is 10.5 dB below the reference level (30% AM).
12. Using the AM fundamental as a reference, measure the second, third and fourth harmonics on the spectrum analyzer. Use Table 4-2 to convert the dB measurements to power ratio. Add power ratios and convert the sum of the power ratios back to dB by using Table 4-2. Total should be > 40 dB from the 30% reference level or about 1%

Example: Second Harmonic -45 dB = .32
 Third Harmonic -45 dB = .31
 Fourth Harmonic -50 dB = .1 } = .73 = -41.5 dB

13. Adjust the Variable Phase Generator until the 10 kHz fundamental is 3 dB below the reference (top graticule line) (70% AM). Using the 10 kHz fundamental as a reference, measure the second, third and fourth harmonics and use Table 4-2 as in step 10. Total harmonics should be > 30 dB below the 70% reference level (3%).

Table 4-2. Carrier Envelope Distortion Test

dB	Power Ratio X10 ⁻⁴	dB	Power Ratio X10 ⁻⁴
20	100.00000	46	.25119
21	79.43282	47	.19953
22	63.09573	48	.15849
23	50.11872	49	.12589
24	39.81072	50	.10000
25	31.62278	51	.07943
26	25.11886	52	.06310
27	19.95262	53	.05012
28	15.84893	54	.03981
29	12.58925	55	.03162
30	10.00000	56	.02512
31	7.94328	57	.01995
32	6.30957	58	.01585
33	5.01187	59	.01259
34	3.98107	60	.01000
35	3.16228	61	.00794
36	2.51189	62	.00631
37	1.99526	63	.00501
38	1.58489	64	.00398
39	1.25893	65	.00316
40	1.00000	66	.00251
41	.79433	67	.00200
42	.63096	68	.00158
43	.50119	69	.00126
44	.39811	70	.00100
45	.31623	71	.00079

PERFORMANCE TESTS

4-21. **AMPLITUDE MODULATION CARRIER ENVELOPE DISTORTION (cont'd)**

14. **Adjust the Variable Phase Generator until the 10 kHz fundamental is 1 dB below the reference (top graticule line) (90% AM). Measure the second, third, and fourth harmonics and use Table 4-2 as in step 10. Total harmonics should be >26 dB below the 90% reference level (5%).**

4-22. INCIDENTAL PHASE MODULATION

SPECIFICATION: Less than 0.2 radians peak at 30% AM.

DESCRIPTION: This test checks the AM to PM ratio. AM is set to 30% Modulation with an external Test Oscillator. The ratio is measured with a Wave Analyzer.

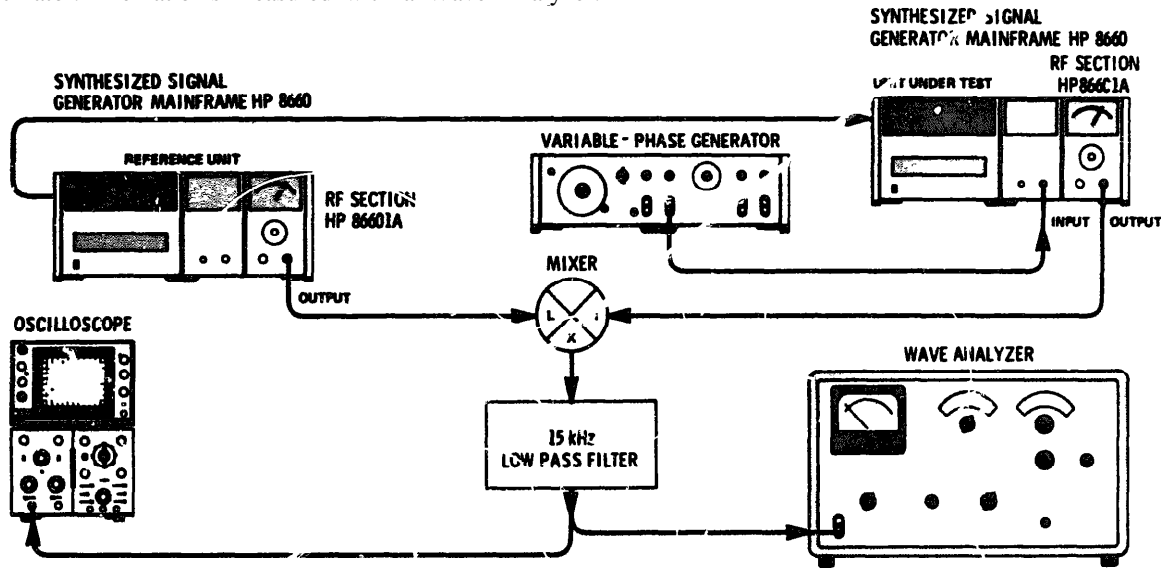


Figure 4-12. Incidental PM Test Setup

RECOMMENDED TEST EQUIPMENT:

Synthesized Signal Generator	HP 8660A/B/86601A/86631A
Oscilloscope	HP 180A/1801A/1821A
Test Oscillator	HP 651B
Wave Analyzer	HP 302A
Double Balanced Mixer	HP 10514A
15 kHz Low Pass Filter (special); see details in Figure 1-3.	
Variable Phase Generator	HP 203A

PROCEDURE:

1. Connect the equipment as shown in **Figure 4-12**.
2. **Connect the rear panel REFERENCE OUTPUT from the reference unit to the rear panel REFERENCE INPUT of the unit under test and set the REFERENCE SELECTOR switch on the unit under test to EXT.**
3. **Set the Oscilloscope to DC couple, .01 V/Div and 5 mSec/Div.**
4. **Set the center frequency of the unit under test to 50 MHz. Set the Model 86601A (unit under test) OUTPUT RANGE to -20 dBm and the VERNIER for a meter reading of +3 dBm.**
5. **Connect the Test Oscillator output to the Model 86631A INPUT. Set the Model 86631A EXTERNAL AM to OFF.**
6. **Set the Test Oscillator frequency to 1 kHz.**

PERFORMANCE TESTS

4-22. INCIDENTAL PHASE MODULATION (cont'd)

- 7 . Set the reference unit mainframe center frequency to 50.000100 MHz at +3 dBm.
- 8 . Adjust the Oscilloscope for an 8-division vertical display of the dc coupled 100 Hz signal.
- 9 . Set the reference unit mainframe center frequency to 50.0000001 MHz and note that the Oscilloscope baseline alternately rises and falls over the 8-division display.
- 10 . Reset the reference unit mainframe center frequency to 50.000000 MHz at a time that will cause the Oscilloscope baseline trace to stop at the top graticule line of the CRT.
- 11 . Repeat steps 9 and 10 until the oscilloscope baseline trace is stopped at the top graticule line $\pm 1/10$ div.
- 12 . Switch the unit under test Model 86631A EXTERNAL AM switch to ON and adjust the Test Oscillator for a 2.4 division deflection on the Oscilloscope (30% AM) with the Oscilloscope ac coupled. Reset Oscilloscope to dc coupled.
- 13 . Set the Wave Analyzer near 1 kHz for a peak and set a convenient 0 dB reference in the relative mode (this is the AM level).
- 14 . Switch the EXTERNAL AM switch on the Model 86631A to OFF.
- 15 . Repeat steps 9 and 10 until oscilloscope baseline trace is stopped at center graticule line $\pm 1/10$ div.
- 16 . Switch the Model 86631A EXTERNAL AM switch to ON and take a reading from the Wave Analyzer for the PM level. The AM to PM ratio should be >5 dB.

4-23. FREQUENCY MODULATION

SPECIFICATION: Rate DC to 1 MHz. Maximum deviation 1 MHz.

DESCRIPTION: This test checks FM distortion and the 1 MHz maximum deviation FM deviation is checked at 1 kHz rate. To check maximum deviation at the maximum rate requires special equipment.

NOTE

This test is valid only when the Model 86632A Modulation Section is used.

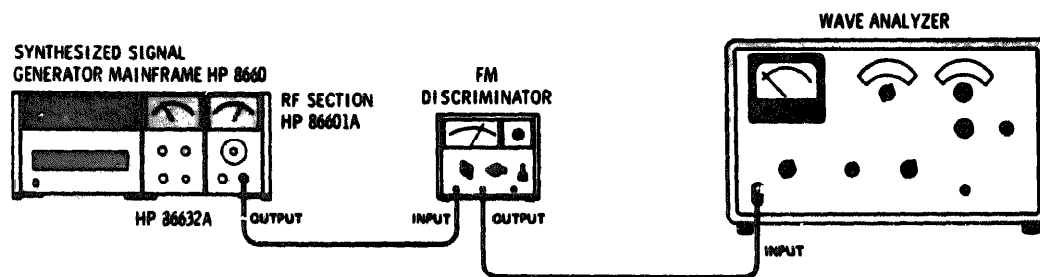


Figure 4-13. Frequency Modulation Test Setup

RECOMMENDED TEST EQUIPMENT:

Frequency Meter/FM Discriminator HP 5210A
 Wave Analyzer HP 302A

PERFORMANCE TESTS

4-23. FREQUENCY MODULATION (cont'd)

PROCEDURE:

1. Connect the equipment as shown in Figure 4-13.
2. Set the Model 86632A MODE switch to FM X10 and the SOURCE switch to INTERNAL 1000. Set the MODULATION LEVEL control for full scale meter deflection and depress the FM CF CAL.
3. Set the center frequency to 8.5 MHz and the Model 86601A output level to +13 dBm.
4. Calibrate the Frequency Meter/FM Discriminator.
5. Install a 20 kHz low pass filter in the Frequency Meter/FM Discriminator. (See the Service Manual for the Frequency Meter/FM discriminator for details.)
6. Set the Frequency Meter/FM Discriminator for 1 V input sensitivity and 10 MHz range.
7. Set the Wave Analyzer near 1 kHz and peak the reading (absolute). The Wave Analyzer meter should indicate 70.7 mVrms (1 MHz = 200 mV p-p or 70.7 mVrms). Set the Wave Analyzer to relative and adjust for a 0 dB reading.
8. Set the Wave Analyzer near 2 kHz (second harmonic). Note the reading in dB on the Wave Analyzer meter.

dB
9. Set the Wave Analyzer near 3 kHz (third harmonic). Note the reading in dB on the Wave Analyzer meter.

dB
10. Use Table 4-2, page 4-14, to obtain power ratios for the levels recorded in steps 8 and 9, then use Table 4-2 to find the dB level corresponding to the sum of the two ratios. This should be down 34 dB from the fundamental frequency level.

Record this level dB

4-24. FREQUENCY SWITCHING TIME

SPECIFICATION: Less than 5 milliseconds to be within 100 Hz of any new frequency selected. Less than 100 milliseconds to be within 5 Hz of any new frequency selected. Maximum stepping rate: 1 millisecond per step.

DESCRIPTION: In this test the Synthesized Signal Generator is remotely programmed and the switching time is detected by a computing counter. The frequencies used in this procedure were selected for worst-case conditions.

PERFORMANCE TESTS

4-24. FREQUENCY SWITCHING TIME (cont'd)

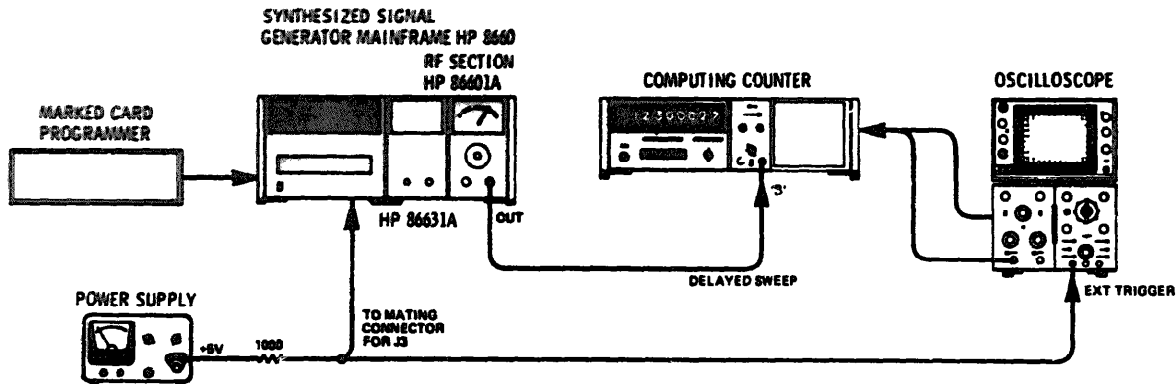


Figure 4-14. Frequency Switching Time Test Setup

RECOMMENDED TEST EQUIPMENT:

DC Power Supply
 Computing Counter
 Marked Card Programmer
 Oscilloscope

HP 721A
 HP 5360A/5365A
 HP 3260A/OPT 001
 HP 180A/1801A/1822A

PROCEDURE:

1. Connect the +5V from the DC Power Supply to pin 17 of the mating connector for J3 through a 1000 ohm resistor. Pin 17 (flag) of the Card Reader's output connector is also used to trigger the main input of the Oscilloscope.
2. Interconnect the Marked Card Programmer with J3 on the rear panel of the Synthesized Signal Generator.
3. Connect the Oscilloscope DELAYED SWEEP OUTPUT (rear panel connector) through a BNC Tee connector to the Oscilloscope vertical Channel A input and to the Ext. Time Measurement Input on the rear panel of the Computing Counter.
4. **Set the Computing Counter controls as follows: rear panel switch to TRIGGER, "B" Channel to X1 sensitivity, Module button depressed, display digits necessary for resolution, measurement time on 1 and counter gate time to 1 millisecond.**
5. **Program the Synthesized Signal Generator to 29.999999 MHz.**
6. **Set the Oscilloscope controls as follows: Trigger ACS EXT -10 — Slope, Trigger level at about 11:00 o'clock, Sweep Mode Auto, Delay Trigger AUTO, Main Sweep 1 mSec, Delay Sweep, .05 μ Sec, and Main sweep mode.**
7. **Set the start of the Oscilloscope trace at the first vertical CRT graticule line. Use the Oscilloscope delay control to set the delay spike 4.5 divisions from the CRT left graticule line.**
8. **Switch the Oscilloscope sweep mode from AUTO to NORMAL.**

PERFORMANCE TESTS

4-24. FREQUENCY **SWITCHING TIME (cont'd)**

9. Program the Synthesized Signal Generator to 30.000000 MHz. The frequency read on the Computing Counter should be 30 MHz \pm 100 Hz.
10. Program the Synthesized Signal Generator to 29.999999 MHz. The frequency read on the Computing Counter should again be within \pm 100 Hz of the programmed frequency.
11. Set the Oscilloscope normal sweep to 10 mSec and the delay sweep to 1 uSec.
12. Set the Oscilloscope sweep mode to auto and the delay control for a delay spike at the center vertical graticule line of the CRT.
13. Set the Oscilloscope main trigger to normal and the Computing Counter gate tune to 100 mSec.
14. Program the Synthesized Signal Generator to 30.000000 MHz. The frequency readout of the Computing Counter should be within \pm 5 Hz of the programmed frequency.
15. Program the Synthesized Signal Generator to 29.999999 MHz. The frequency readout of the Computing Counter should again be within \pm 5 Hz of the programmed frequency.

4-25. OUTPUT LEVEL SWITCHING TIME

SPECIFICATION: Any level change may be accomplished in less than 50 mSec. Any change to another level on the same attenuator range may be accomplished in 5 mSec in the remote mode.

DESCRIPTION: This test checks amplitude switching speeds in the remote mode with center frequencies of 100 kHz and 1 MHz. The Model 86601 rf output is detected and measured on an Oscilloscope.

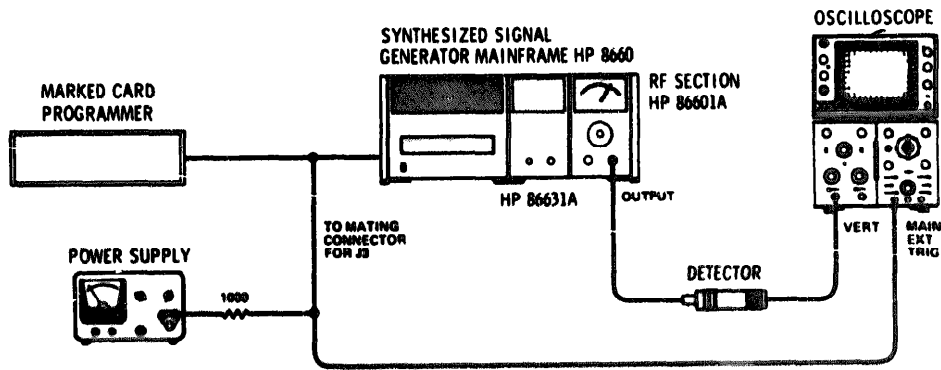


Figure 4-15. Output Level Switching Time Test Setup

RECOMMENDED TEST EQUIPMENT:

Marked Card Programmer	HP 3260A, Opt. 001
Oscilloscope	HP 180A/1801A/1822A
Crystal Detector	HP 8471A

PERFORMANCE TESTS

4-25. OUTPUT LEVEL SWITCHING TIME (cont'd)

PROCEDURE:

1. Connect the equipment as shown in Figure 4-15. Note that the +5 V from the DC Power Supply is connected through a 1000 ohm resistor to pin 17 of the mating connector to J3 and to the External trigger input of the Oscilloscope.
2. Connect the Model 86601A rf output to the channel A input of the Oscilloscope through a Crystal Detector.
3. Set the Oscilloscope as follows: Main Time/Div 5 mSec. Vertical Input DC Coupled, .5V/Div, Normal Sweep, Ext Trigger ± 10 , - Slope, ASC, Trigger level about 11:00 o'clock.
4. Program the mainframe center frequency to 100 kHz. Program the Model 86601A attenuation to the following settings; 0 dB, -5 dB, -9 dB. Switching time should be <5 mSec.
5. Program attenuation to 0 dB, then to -20 dB. Switching time should be <50 mSec.
6. Repeat tests 4 and 5 with center frequency set to 1 MHz.

4-26. INCIDENTAL AM

SPECIFICATION: With 75 kHz peak deviation at a 1 kHz rate, AM modulation sidebands are down 60 dB from the fundamental.

DESCRIPTION: This test measures AM modulation with the unit under test FM modulated at 75 kHz peak deviation. A reference level is set on the Wave Analyzer with the two Synthesized Signal Generators offset by 1 kHz. The unit under test is then programmed to produce a 1 kHz frequency modulated signal with 75 kHz peak deviation.

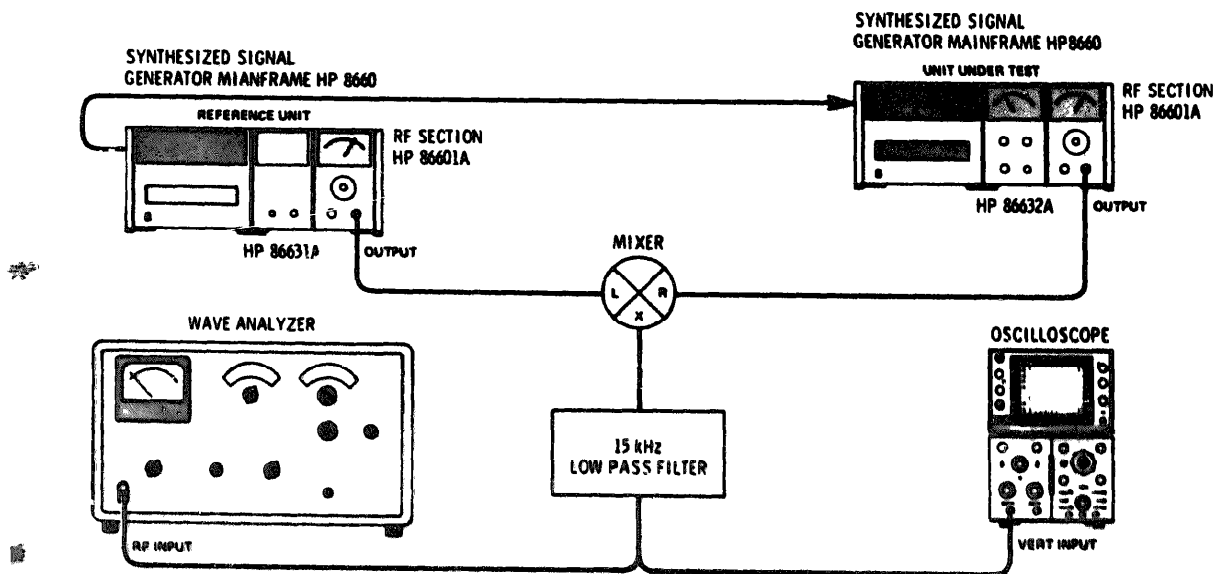


Figure 4-16. Incidental AM Test Setup

PERFORMANCE TESTS

4-26. INCIDENTAL AM (cont'd)

RECOMMENDED TEST EQUIPMENT

Synthesized Signal Generator
Modulation Section
Oscilloscope
Wave Analyzer .
Double Balanced i & &

8660/86631A/86601A
HP 86632A
 HP180A/1801A/P821A
 HP302A
 H P 1 0 5 1 4 A

15kHz Low Pass Filter (special): see details in Table 1-2.

PROCEDURE:

1. Connect equipment as shown in Figure 4-16.
2. Connect the rear panel REFERENCE OUTPUT from the reference unit to the rear panel REFERENCE INPUT of the unit under test and set the REFERENCE SELECTOR of the unit under test to EXT.
3. Set the unit under test center frequency to 50 MHz and the output level to -7 dBm.
4. Set the reference unit center frequency to 50.061 MHz and the output level to +13 dBm.
5. Set the wave Analyzer near 1 kHz and peak the meter, Set the Wave Analyzer meter level to 0 dB in the relative mode. Set the Oscilloscope for 8-division deflection.
6. Set the reference unit mainframe center frequency to 50.0000001 MHz and note that the Oscilloscope baseline alternately rises and falls over the 8 division display.
7. Reset the reference unit mainframe center frequency to 50.000000 MHz at a time that will cause the Oscilloscope baseline trace to stop at the top graticule line of the CRT.
8. Repeat steps 6 and 7 until the baseline stops on the top CRT graticule $\pm 1/10$ div.
9. Set the Model 86632A Modulation Section to 1 kHz FM XI and 75 kHz deviation (75% on the meter).
10. Note the Wave Analyzer reading. Should be > -60 dB down from the reference level.
 Meter Reading dB

Table 4-3. Performance Test Record

Hewlett-Packard Model 86601A RF Section Serial Number _____		Tested By _____ Date _____
Paragraph Number	Test	
4-13	IMPEDANCE Step 8 Record SWR _____ Step 11 Record SWR _____	
4-15	SPURIOUS SIGNALS Record Levels 101 MHz _____ 109.99 MHz _____ 103.1 MHz _____ 25.595 MHz _____	
4-16	SIGNAL TO PHASE NOISE RATIO Step 3 Record Level _____ dB Step 10 Record Level _____ dB	
4-17	SIGNAL TO AM NOISE RATIO Step 4 Record Level _____ dB Step 11 Record Level _____ dB	
4-21	AMPLITUDE MODULATION CARRIER ENVELOPE DISTORTION Step 12 Record Level _____ dB	
4-23	FREQUENCY MODULATION Step 8 Record Level _____ dB Step 9 Record Level _____ dB Step 10 Record Level _____ dB	
4-26	INCIDENTAL AM Step 10 Record Level _____ dB	

SECTION V ADJUSTMENTS

5-1. INTRODUCTION

5-2. This section describes adjustments and checks required to return the Model 86601A to peak operating capability when repairs have been made. Adjustment locations are identified pictorially on Section VIII foldout service sheets referred to in the individual tests.

5-3. If repairs to any filter have been made, it should be necessary to adjust only the circuit in which the component failure occurred.

5-4. If component failure occurs in any circuit other than the logic circuits, it will be necessary to recalibrate the RF output meter circuit (refer to paragraph 5-14).

5-5. If component failure occurs in A3 or A9, the AM input and AGC circuits must be readjusted (refer to paragraph 5-15).

5-6. If component failure occurs in the A6 pre-amplifier or the A2 Power amplifier (other than AGC), the harmonic levels should be readjusted (refer to paragraph 5-16).

5-7. RECOMMENDED TEST EQUIPMENT

5-8. Each adjustment procedure in this section contains a list of test equipment and accessories required to perform the procedure. Each test setup identifies test equipment and accessories by call-outs.

5-9. Minimum specifications for test equipment used in the adjustment procedures are detailed in Table 1-2. Because the Model 86601A is an extremely accurate instrument, minimum specifications in Table 1-2 are particularly important in performing these adjustment procedures.

5-10. SERVICE KIT

5-11. The HP 11678A Service Kit is an accessory item available from Hewlett-Packard for use in maintaining the Model 66601A RF Section.

5-12. Table 1-2 contains a detailed description of the service kit. Any item in the kit may be ordered separately.

NOTES

- a. The RF Section adjustments should be made with the Model 86601A installed in the mainframe with the cover removed whenever possible. It will be necessary to remove the mainframe top cover and the top guide rail for the Model 86601A. To make in-circuit adjustments for the 480 MHz Active bandpass filter or the dual filter (A12), it will be necessary to use the extender cable (1167260001) which is part of the service kit.
- b. A modulation section or an auxiliary section must be installed in the mainframe during these adjustments.
- c. All tests in which a counter is used should be made with the mainframe and the counter driven by a common frequency standard. If the Hewlett-Packard Model 5245M Electronic counter is used, the mainframe internal reference may be used as the common source.

5-13. CHECKS AND ADJUSTMENTS

ADJUSTMENTS

5-14. RF OUTPUT METER CALIBRATION

REFERENCE: Service Sheet 3 and Figures 5-1 and 8-21 of this Manual Changes supplement.

DESCRIPTION: The rf output meter reading is adjusted at +3 and -7 dBm to ensure tracking across the range of the VERNIER control.

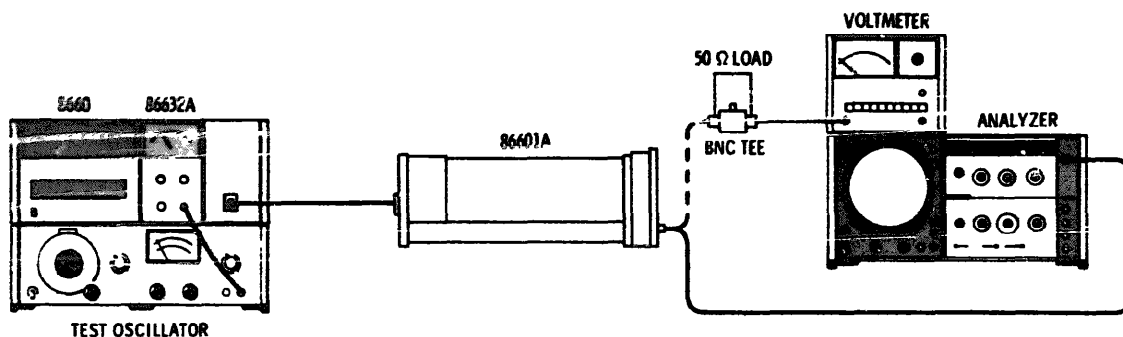


Figure 5-1. RF Output Meter Calibration Setup

RECOMMENDED TEST EQUIPMENT:

Test Oscillator	HP 651B
Broadband Sampling voltmeter	H 3406A
BNC Tee Connector	UG 274 B/U
50 ohm load	HP 1250-0207
Extender Cable	HP 11672-60001
Spectrum Analyzer	HP 140/8552/8553

PROCEDURE:

1. Clean the Model 86601A meter face with anti-static **sc. s. s.** (Recommended: STATNUL manufactured by Weston Instruments Inc. Newark, NJ.)
2. Connect the equipment **as shown in Figure 1.**
3. **Set the OUTPUT RANGE to +10 dBm and the VERNIER full CW. Set the mainframe center frequency to 10 MHz.**
4. **Set the REF ADJ (A9R2) for a +13.5 dBm reading on the voltmeter.**
5. **Set the Model 86601A VERNIER for a +13 dBm reading on the voltmeter. Adjust A9R32 for a +3 dBm reading on the 86601A meter (full scale).**
6. **Disconnect the output rf cable from the BNC Tee and connect it to the spectrum analyzer RF INPUT.**

ADJUSTMENTS

5-14. RF OUTPUT METER CALIBRATION (Cont')

7. Connect the Test Oscillator output to the Model 86632A input (10 kHz, 1V, verify level with the AC Voltmeter). Set the Model 86632A to AM, EXT, AC coupled and 50% modulation as indicated on the Model 86632A meter.
8. Set the spectrum analyzer so that the 10 MHz center frequency is at the top graticule line. Verify that the AM sidebands are -12 dB below the center frequency fundamental (50% modulation).
9. Adjust the Model 86601A VERNIER until the fundamental (10 MHz) is 10 dB below the reference setting. Adjust A1R34 DET for 50% modulation (AM sidebands down -12 dBm from the fundamental).
10. A9R32 and A2R34 interact. Repeat steps 5 through 9 until the modulation displayed on the spectrum analyzer remains at 50%.
11. Disconnect the Test Oscillator and set the Model 86632A to OFF. Disconnect the spectrum analyzer and connect the AC Voltmeter to the Model 86601A OUTPUT.
12. Set the 86601A to +13 dBm as measured by the voltmeter.
13. Adjust A9R32 as necessary for a Model 86601A meter reading of +3 dBm.
14. Turn the Model 86601A VERNIER control CCW until the AC voltmeter reads +3 dBm (10 dB less than step 12).
15. Adjust A9R34 for a Model 86601A meter reading of -7 dBm.
16. Repeat steps 11 through 15 until the Model 86601A meter tracks the AC voltmeter, (from +3 dBm to -7 dBm \pm 25 dBm 86601A Meter).

ADJUSTMENTS

5-15. HARMONIC DISTORTION CHECKS AND ADJUSTMENTS

REFERENCE: Service Sheet 3.

DESCRIPTION: This bias levels for the Preamplifier and the Power Amplifier are set to minimize distortion.

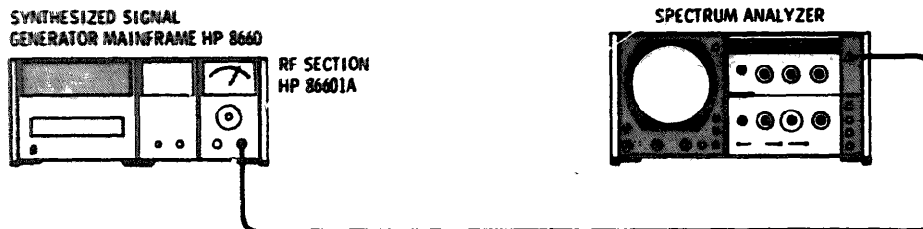


Figure 5-2. Harmonic Distortion Adjustment Setup

RECOMMENDED TEST EQUIPMENT:

Spectrum Analyzer

HP 140/8554L/8552B

PROCEDURE:

1. Connect the equipment as shown in Figure 5-3.
2. Set the mainframe center frequency to 60 MHz and the Model 86601A output amplitude to 0 dBm.
3. Set the Spectrum Analyzer controls as follows: CENTER FREQUENCY - 60 MHz, INPUT ATTENUATION - 20 dB, LOG REP LEVEL - 0 dBm, BANDWIDTH - 100 kHz, SCAN WIDTH PER DIVISION - 50 MHz, SCAN TIME PER DIVISION - 10 MILLISECONDS and LOG/LINEAR - LOG.
4. Adjust the preamplifier BIAS (A6R1) and the power amplifier BIAS (A2R6) until the second harmonic (120 MHz) is more than 50 dB down from the fundamental frequency.
5. Set the mainframe and the Spectrum Analyzer center frequency to 109 MHz.
6. Adjust the power amplifier BIAS (A1R6) until the second harmonic (218 MHz) is more than 44 dB down from the fundamental frequency.
7. **Change the mainframe and the Spectrum Analyzer in 10 MHz steps from 100 MHz to 10 MHz, stopping at each step and checking the harmonic levels on the Spectrum Analyzer. All harmonic levels should be more than 40 dB below the amplitude of the fundamental frequencies.**
8. **Record the harmonic levels in Table 5-1.**

ADJUSTMENTS

5-15. HARMONIC DISTORTION CHECKS AND ADJUSTMENTS (Cont'd)

Table 5-1. Harmonic Distortion Level Checks

Fundamental Frequencies	Harmonic Levels		
	Second	Third	Fourth
109 MHz			
100 MHz			
90 MHz			
80 MHz			
70 MHz			
60 MHz			
50 MHz			
40 MHz			
30 MHz			
20 MHz			
10 MHz			

5-16. AMPLITUDE MODULATION CALIBRATION

REFERENCE: Service Sheets 3 and 4.

DESCRIPTION: The AM input and AGC circuits **are** properly **adjusted to allow the use of any plug-in** Modulation Section without recalibration.

ADJUSTMENTS

5-16. AMPLITUDE MODULATION CALIBRATION (Cont'd)

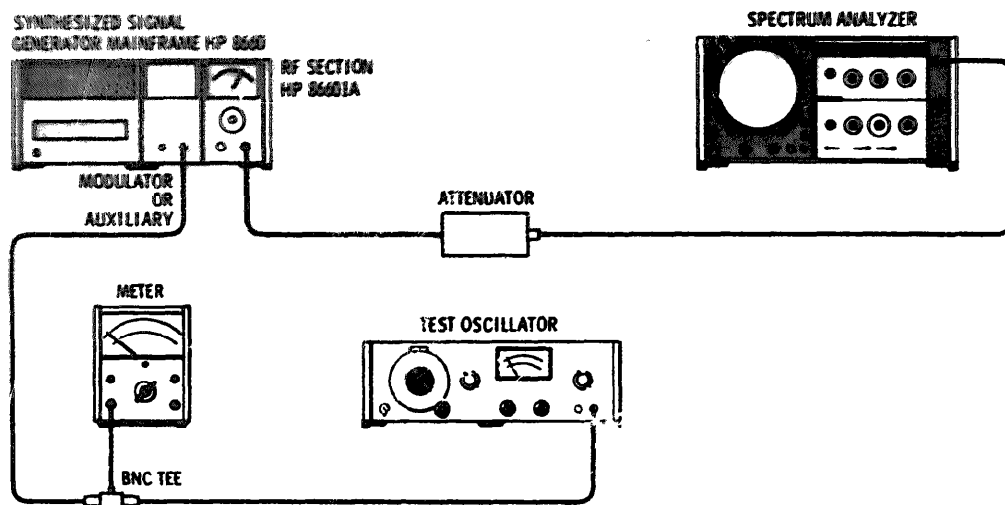


Figure 5-3. Amplitude Modulation Calibration Setup

RECOMMENDED TEST EQUIPMENT:

Precision Attenuator	HP H38-355D
Test Oscillator	HP 651B
Spectrum Analyzer	HP 140/8553B/8552B
High Frequency dB Voltmeter	HP 400GL
BNC Tee Connector	UG 274B/U

PROCEDURE:

Using the 86631A Auxiliary Section. (If the Model 86632A Modulation Section is used, use step 2-a instead of step 2.)

1. Connect the equipment as shown in Figure 5-2.
2. Monitor the output amplitude of the Test Oscillator with the High Frequency dB Voltmeter. Set the Test Oscillator frequency to 1 kHz and the output amplitude to 0.5 volts rms with the Model 86631 EXTERNAL AM switch to ON.
- 2-a. Set the Model 86632A to AM mode; source 1 kHz, internal modulation level for 50% AM on the 86632A meter.
3. Set the mainframe center frequency to 50 MHz, the Model 86601A output amplitude to +13 dBm and the Precision Attenuator to 20 dB.
4. Set the Spectrum Analyzer controls as follows: CENTER FREQUENCY - 50 MHz, INPUT ATTENUATION - 10 dB, LOG REF LEVEL - 0 dBm, LOG/LINEAR - 2 dB LOG, SCAN TIME PER DIVISION - .1 SECONDS, SCAN WIDTH PER DIVISION - .5 kHz, AND BANDWIDTH - .1 kHz.
5. Adjust the AM CAL control (A9R13) for sidebands 12 dB down from the center frequency amplitude (see typical waveform in Figure 5-2).

ADJUSTMENTS

5-17. A12 FILTER ASSEMBLY CHECKS AND ADJUSTMENTS

REFERENCE: **Service Sheet 2.**

DESCRIPTION: The bandpass filters in the A12 assembly are adjusted for minimum insertion loss and maximum flatness over the specified bandwidth.

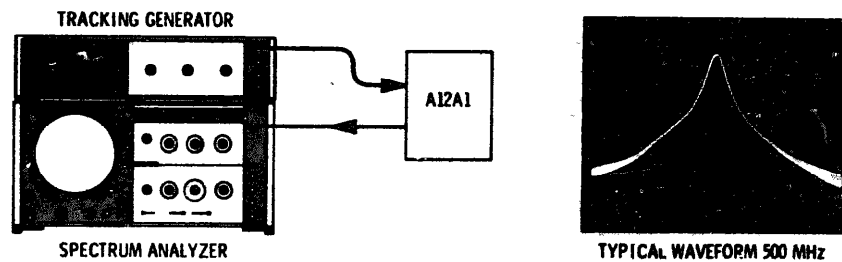


Figure 5-4. A12A1 Filter Adjustment Setup

RECOMMENDED TEST EQUIPMENT:

Tracking Generator
 Spectrum Analyzer
 RF Millivoltmeter
 Electronic Counter
 BNC Tee Connector

HP 8444A
 HP 140/8554L/8552B
 HP 411A
 HP 5245M/5253B
 UG 274B/U

PROCEDURE: 500 MHz Bandpass Filter A12A1

1. Remove the A12 Dual Filter assembly from the Model 86601A.
2. Connect the tracking Generator to the Spectrum Analyzer. (Refer to the Tracking Generator Operating and Service Manual for interconnections.)
3. Set the Spectrum Analyzer controls as follows: INPUT ATTENUATION - 20 dB, LOG/LINEAR - 10 dB LOG, LOG REF LEVEL - +10 dBm, SCAN WIDTH PER DIVISION -- 20 MHz, SCAN TIME PER DIVISION - 10 MILLISECONDS and BANDWIDTH - 300 kHz.
4. Connect the Tracking Generator RF OUTPUT to the Counter with the Spectrum Analyzer in the ZERO scan mode.
5. **Set the Spectrum Analyzer center frequency to 500 MHz as displayed on the Counter and disconnect the counter.**
6. **Set the Tracking Generator LEVEL to 0 dBm as a reference.**
7. **Connect the A12A1 filter to the equipment as shown in Figure 5-4**
8. **Change the Spectrum Analyzer SCAN WIDTH from ZERO to PER DIVISION.**
9. **Adjust A12A1C1 and A12A1C2 for minimum insertion loss and maximum flatness.**
10. **Record the insertion loss and flatness.**

Insertion Loss _____ dB
 Flatness (peak-to-peak) _____ dB

ADJUSTMENTS

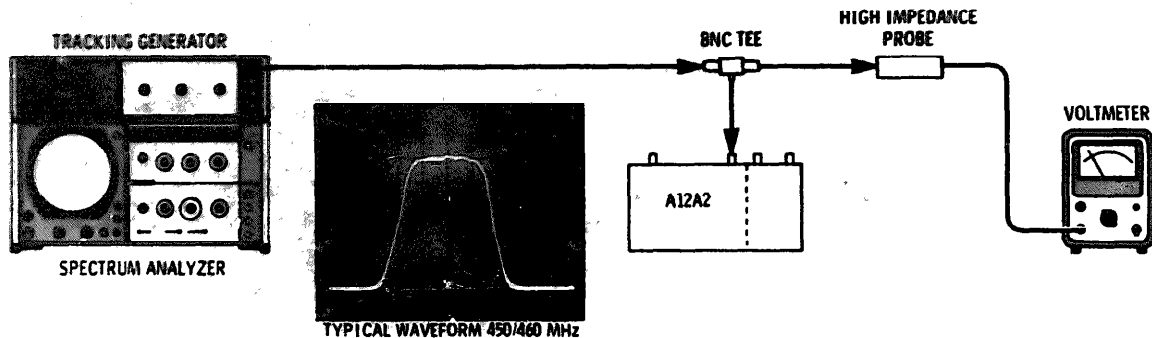
5-17. **A12 FILTER ASSEMBLY CHECKS AND ADJUSTMENTS (cont'd)**11. **Disconnect the cables from the 500 MHz Bandpass Filter.****PROCEDURE: 450/460 Bandpass Filter A12A2**

Figure 5-5. Preliminary Adjustment Setup (450/460 Bandpass Filter)

1. Remove the A12 Dual Filter assembly from the Model 86601A.
2. Connect the Tracking Generator to the Spectrum Analyzer. (Refer to the Tracking Generator Operating and Service Manual for interconnections.)
3. Set the Spectrum Analyzer as follows: INPUT ATTENUATION - 20 dB, LOG/LINEAR - 10 dB LOG, LOG REF LEVEL - 0 dBm, SCAN WIDTH PER DIVISION - 5 MHz, SCAN TIME PER DIVISION - 5 MILLISECONDS and BANDWIDTH - 300 kHz.
4. Connect the Tracking Generator RF OUTPUT to the Counter with the Spectrum Analyzer in the ZERO scan mode.
5. Set the Spectrum Analyzer center frequency to 455 MHz as displayed on the Counter and disconnect the Counter.
6. Set the Tracking Generator LEVEL to -14 dBm as a reference.
7. Connect the equipment together as shown in Figure 5-5.
8. Use a screwdriver to short the rotor of C2 to the casting. Adjust C1 for a maximum level on the Voltmeter.
9. Short C3 to the casting and adjust C2 for minimum reading on the Voltmeter.
10. **Short C4 to the casting and adjust C3 for maximum reading on the Voltmeter.**
11. **Short C5 to the casting and adjust C4 for minimum reading on the Voltmeter.**
12. **Short C6 to the casting and adjust C5 for maximum reading on the Voltmeter.**
13. **Short C7 to the casting and adjust C6 for minimum reading on the Voltmeter.**
14. **Adjust C7 for a maximum reading on the Voltmeter.**

ADJUSTMENTS

5-17. A12 FILTER ASSEMBLY CHECKS AND ADJUSTMENTS (cont'd)

15. **Disconnect the Tracking Generator, the Voltmeter and the BNC Tee Connector.**
16. Connect the equipment shown in Figure 5-4.
17. Change the Spectrum Analyzer scan mode from ZERO scan to SCAN WIDTH PER DIVISION.
18. Adjust C1 and C7 for minimum insertion loss and maximum flatness. (Insertion loss is approximately 5 dB.)
19. Adjust C2 through C6 for optimum flatness and minimum insertion loss.
20. Record the ripple, insertion loss and roll-off.

Ripple	2 dB maximum peak-to-peak	_____ dB
Insertion loss	6 dB maximum	_____ dB
Rolloff	55 dB down at 440 MHz	- d B
	55 down at 470 MHz	_____ dB

5-18. 480 MHz ACTIVE FILTER CHECKS AND ADJUSTMENTS

REFERENCE: Service Sheet 2.

DESCRIPTION: The 480 MHz bandpass filter in the A4 assembly is adjusted for maximum flatness and minimum insertion loss.

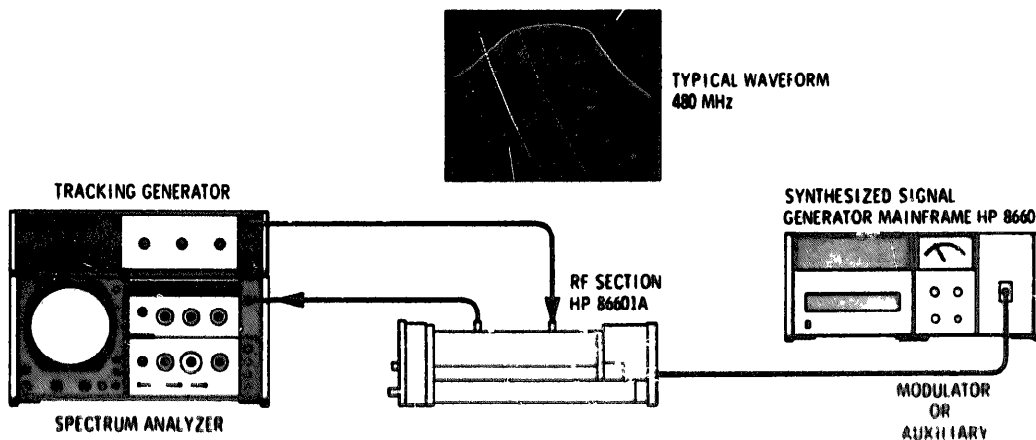


Figure 5-6. Active Filter Adjustment Setup

RECOMMENDED TEST EQUIPMENT:

Tracking Generator	HP 8444A
Spectrum Analyzer	HP 140/8554L/8552B
Electronic Counter	HP 5245M/5253B
Extender Cable	HP 11672-60001

ADJUSTMENTS

5-19. **480 MHz ACTIVE FILTER CHECKS AND ADJUSTMENTS (cont'd)**

PROCEDURE:

1. **Remove the Model 86601A from the mainframe. Remove the cover and reconnect the Model 86601A with extender cable 11672-60001.**
2. **Connect the Tracking Generator to the Spectrum Analyzer.** (Refer to the **Tracking Generator Operating and Service Manual.**)
3. **Set the Spectrum Analyzer controls as follows:** INPUT ATTENUATION - 20 dB, LOG REF LEVEL - **+10 dBm, SCAN WIDTH PER DIVISION - 2 MHz, SCAN TIME PER DIVISION - 10 MILLISECONDS and BANDWIDTH - 300 kHz.**
4. **Connect the Tracking Generator RF OUTPUT to the Electronic Counter with the Spectrum Analyzer in the ZERO scan mode.**
5. **Set the Spectrum Analyzer frequency to 480 MHz as indicated by the Electronic Counter.**
6. Set the Tracking Generator LEVEL to -14 dBm as a reference.
7. Connect the equipment as shown in Figure 5-6.
8. **Adjust A4C1, 2, 3 and 4 for maximum output and maximum flatness across the bandwidth. At 480 MHz, gain** should be greater than or equal to 17 dB. The response curve should rolloff to more than 3 dB down at 477 and 483 MHz.
9. Record the gain and rolloff.

Gain at 480 MHz _____ dB
 Rolloff at 477 MHz _____ dB
 Rolloff at 483 MHz _____ dB

SECTION VI
REPLACEABLE PARTS

6-1. INTRODUCTION

6-2. Table 6-1 provides correct stock numbers for use when ordering assemblies on an exchange basis. These factory-repaired assemblies are available on an exchange-for-credit basis at a considerable savings cost.

6-3. Table 6-2 lists the meanings of the abbreviations and reference designations used in the table of replaceable parts.

6-4. Table 6-3 lists 86601A replaceable parts in alpha-numerical order of their reference designation.

6-5. Table 6-4 contains the names and addresses that correspond to the manufacturers' code numbers.

6-6. ORDERING INFORMATION

6-7. **To order a part listed in the replaceable parts table, note the Hewlett-Packard part number and then cross-reference that part number to the National Stock Number listed in table 6-5. Then order through normal ordering channels.**

6-8. If the part number does not have a National Stock Number, then order through normal ordering channels using the Hewlett-Packard part number.

6-9. Refer to table 6-5 for part number to NSN cross-reference.

Table 6-1. Part Numbers for Assembly Exchange Orders

Assembly	New Part No.	Exchange No.
A2 Power Amplifier Assembly	86601-60018	86601-60107
A3 Feedback Amplifier	86601-60065	86601-60115
A4 Active Filter	86601-60023	86601-60110
A5 Modulator Assembly	86601-60080	86601-60117
A6 Preamplifier Assembly	86601-60017	86601-60106
A8 Attenuator Driver Assembly	86601-60006	86601-60102
A9 Reference Assembly	86601-60063	86601-60113
A10 Logic Assembly	86601-60118	86601-60119
A12 Dual Filter	86601-60022	86601-60112
A13 Programmable Attenuator	86601-60039	86601-60109
A14 Low Pass Filter	86601-60021	86601-60111
420 600 MHz Low Pass Filter	86601-60066	86601-60116

Table 6-2. Reference Designators and Abbreviations Used in Parts List

REFERENCE DESIGNATORS							
A	= assembly	F	= fuse	P	= plug	V	= vacuum tube, neon bulb, photocell, etc.
B	= motor	FL	= Filter	Q	= transistor	VL	= voltage regulator
BT	= battery	J	= jack	R	= resistor	W	= cable
C	= capacitor	K	= relay	RT	= thermistor	X	= socket
CP	= coupler	L	= inductor	S	= switch	Y	= crystal
CR	= diode	LS	= loud speaker	T	= transformer	Z	= tuned cavity, network
DL	= delay line	M	= meter	TB	= terminal board		
DS	= device signaling (lamp)	MK	= microphone	TP	= test point		
E	= misc electronic part	MP	= mechanical part	U	= integrated circuit		
ABBREVIATIONS							
A	= amperes	H	= henries	N/O	= normally open	RMO	= rack mount only
AFC	= automatic frequency control	HDW	= hardware	NOM	= nominal	RMS	= root-mean square
AMPL	= amplifier	HEX	= hexagonal	NPO	= negative positive zero (zero temperature coefficient)	RWV	= reverse working voltage
BFO	= beat frequency oscillator	HR	= hour(s)	NPN	= negative-positive-negative	S-B	= slow-blow
BE CU	= beryllium copper	Hz	= Hertz	NRFR	= not recommended for field replacement	SCR	= screw
BH	= binder head	IF	= intermediate freq	NSR	= not separately replaceable	SE	= selenium
BP	= bandpass	IMPG	= impregnated	OBD	= order by description	SECT	= section(s)
BRS	= brass	INCD	= incandescent	OH	= oval head	SEMICON	= semiconductor
BWO	= backward wave oscillator	INCL	= include(s)	OX	= oxide	SI	= silicon
CCW	= counterclockwise	INS	= insulation(ed)	PC	= peak	SL	= slide
CER	= ceramic	INT	= internal	PF	= printed circuit	SPG	= spring
CMO	= cabinet mount only	K	= kilo = 1000	PH BRZ	= phosphor bronze	SPL	= special
COEF	= coefficient	LH	= left hand	PHL	= Phillips	SST	= Stainless steel
COM	= common	LIN	= linear taper	PIV	= peak inverse voltage	SR	= split ring
COMP	= composition	LK WASH	= lock washer	PNP	= positive-negative-positive	STL	= steel
COMPL	= complete	LOG	= logarithmic taper	P/O	= part of	TA	= tantalum
CONN	= connector	LPF	= low pass filter	POLY	= polystyrene	TD	= time delay
CP	= cadmium plate	M	= milli = 10 ⁻³	PORC	= porcelain	TGL	= toggle
CRT	= cathode-ray tube	MEG	= meg = 10 ⁶	POS	= position(s)	THD	= thread
CW	= clockwise	MET FLM	= metal film	POT	= potentiometer	TI	= titanium
DEPC	= deposited carbon	MET OX	= metallic oxide	PP	= peak-to-peak	TOL	= tolerance
DR	= drive	MFR	= manufacturer	PT	= point	TRIM	= trimmer
ELECT	= electrolytic	MHz	= mega Hertz	PWV	= peak working voltage	TWT	= traveling wave tube
ENCAP	= encapsulated	MINAT	= miniature	RECT	= rectifier	μ	= micro = 10 ⁻⁶
EXT	= external	MOM	= momentary	RF	= radio frequency	VAR	= variable
F	= farads	MOS	= metalized substrate	RM	= round head or right hand	VDCW	= dc working volts
FH	= flat head	MTG	= mounting			W/	= with
FIL H	= fillister head	MY	= "mylar"			W	= watts
FXD	= fixed	N	= nano (10 ⁻⁹)			WIV	= working inverse voltage
G	= giga (10 ⁹)	N/C	= normally closed			WW	= wirewound
GE	= germanium	NE	= neon			W/O	= without
GL	= glass	NI PL	= nickel plate				
GRD	= ground(ed)						

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
A1			FRONT PANEL ASSEMBLY		
A1C1	0160-2437	6	CIFXD CER 5000 PF +80-20% 200VDCW	72982	2425-000-X5V-502P
A1C2	0160-2437		CIFXD CER 5000 PF +80-20% 200VDCW	72982	2425-000-X5V-502P
A1C3	0160-2437		CIFXD CER 5000 PF +80-20% 200VDCW	72982	2425-000-X5V-502P
A1C4	0160-2437		CIFXD CER 5000 PF +80-20% 200VDCW	72982	2425-000-X5V-502P
A1C5	0160-2437		CIFXD CER 5000 PF +80-20% 200VDCW	72982	2425-000-X5V-502P
A1C6	0160-2437		CIFXD CER 5000 PF +80-20% 200VDCW	72982	2425-000-X5V-502P
A1C7	0160-3744	2	CIFER FEED-THRU 1000 PF 200VDCW	72982	2425-000-X5U0-102Z
A1M1	1120-0540	1	METER:2-1/2", 1 MA (FOR STANDARD INSTRUMENT)	32171	82072C
A1M1	1120-0542	1	METER:2-1/2", 1MA (FOR OPTION 001)	28480	1120-0542
A1MP1	866C1-20017	1	HOUSING FRONT	2848C	866C1-20017
A1MP2	866C1-20069	1	FRAME, FRONT PANEL	28480	86601-20069
A1MP3	866C1-00034	1	PANEL:FRONT	28480	866C1-00034
A1MP3	866C1-00035	1	(FOR STANDARD INSTRUMENT ONLY) PANEL:FRONT(CPT 001)	2848C	866C1-00035
A1MP3	866C1-00036	1	MOUNT:METER	28480	86601-00036
A1MP5	866C1-20070	1	WINDOW	2848C	86601-20070
A1MP6	866C1-40018	1	SCREEN:ADJ METER	2848C	86601-40018
A1R1	21JC-3113	1	RVAR COMP 2500 OHM 10% 10 CLOG 1/4W	28480	2100-3113
A1K2	0698-3430	1	RIFXD MET FLM 21.5 OHM 1% 1/8W	2848C	0698-3430
A1S1	310C-3022	1	SWITCH:ROTARY 2 SECTION 16 POSITION	76854	TYPE LK
A2	86601-60018	1	PCWER AMPLIFIER ASSY	2848C	86601-60018
A2C1	0180-0197	21	CIFXD ELECT 2.2 UF 10% 20VDCW	56285	1500225X9020A2-DVS
A2C2	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56285	1500225X9020A2-DVS
A2C3	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56285	1500225X9020A2-DVS
A2C4	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56289	1500225X9020A2-DVS
A2C5	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56289	1500225X9020A2-DVS
A2C6	0160-2327	1	CIFXD CER 1000 PF 20% 200VDCW	96733	81048X102M
A2C7	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56289	1500225X9020A2-DVS
A2C8	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56289	1500225X9020A2-DVS
A2C9	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56285	1500225X9020A2-DVS
A2C10	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56289	1500225X9020A2-DVS
A2C11	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56285	1500225X9020A2-DVS
A2C12	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56285	1500225X9020A2-DVS
A2C13	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56285	1500225X9020A2-DVS
A2C14	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56289	1500225X9020A2-DVS
A2C15	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56289	1500225X9020A2-DVS
A2C16	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56285	1500225X9020A2-DVS
A2C17	0180-2205	2	CIFXD ELECT 0.33 UF 10% 35VDCW	56289	1500334H9035A2-DVS
A2C18	0160-3446	2	CIFXD CER 220 PF 10% 1KVDCW	56285	C0160102F221K525-COH
A2C19	0180-2205		CIFXD ELECT 0.33 UF 10% 35VDCW	5-289	1500334H9035A2-DVS
A2C20	0180-0058	4	CIFXD AL ELECT 90 UF +75-10% 25VDCW	56285	3005046025CC2-DSH
A2C21	0160-3449	2	CIFXD CER 2000 PF 10% 250VDCW	56285	C0678231F202K525-COH
A2C22	0160-3449		CIFXD CER 2000 PF 10% 250VDCW	56285	C0678231F202K525-COH
A2C23	0160-3446		CIFXD CER 220 PF 10% 1KVDCW	56285	C0160102F221K525-COH
A2C24	0160-3447	2	CIFXD CER 470 PF 10% 1000VDCW	56289	C0160102F471K525-COH
A2C25	0160-3447		CIFXD CER 470 PF 10% 1000VDCW	56289	C0160102F471K525-COH
A2C26	0160-3036	16	CIFXD CER 5000 PF +80-20% 200VDCW	28480	0160-3036
A2C27	0160-3036		CIFXD CER 5000 PF +80-20% 200VDCW	2848C	0160-3036
A2C28	0160-3036		CIFXD CER 5000 PF +80-20% 200VDCW	2848C	0160-3036
A2C29	0160-3036		CIFXD CER 5000 PF +80-20% 200VDCW	2848C	0160-3036
A2C31	1902-0361	2	DIODE:HYBRID HGT CARRIER	04710	5710030-80
A2C32	1902-0361	3	DIODE:HYBRID HGT CARRIER	2848C	1401-C535
A2C33	1902-0361		DIODE:HYBRID HGT CARRIER	2848C	1401-C535
A2C34	1902-0361	2	DIODE:HYBRID HGT CARRIER	04710	5710030-80
A2C35	1902-0361		DIODE:HYBRID HGT CARRIER	2848C	1401-C535
A2J1	1250-1901	11	CONNECTOR:RF BULKHEAD	15558	110470
A2J2	1250-1901		CONNECTOR:RF BULKHEAD	15558	110470
A2J3	1250-1901		CONNECTOR:RF BULKHEAD	15558	110470
A2L1	010C-1627	4	COIL/CHOKER 50 OHM 5% ELECTRICAL SHIELD	02142	15-1D15-2J
A2L2	010C-1627		COIL/CHOKER 50 OHM 5% ELECTRICAL SHIELD	02142	15-1D15-2J
A2L3	0160-0287	4	COIL:RF 200 OHM 5%	2848C	0160-0287
A2MP1	866C1-00034	1	BOARD ASSY:POWER AMPLIFIER	2848C	866C1-00034
A2MP2	866C1-20024	1	CONNECTOR:RF BULKHEAD	2848C	866C1-20024
A2Q1	1853-0293	3	TEST:15 AMP	00131	287583

See Introduction to this section for ordering information

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
A202	1853-0293	2	TSTR:SI PNP	60131	2N5583
A203	1854-0501		TSTR:SI NPN	C4713	MM8223
A204	1854-0501		TSTR:SI NPN	C4713	MM8023
A205	1853-0293		TSTR:SI PNP	60131	2N5583
A206	1853-0020		TSTR:SI PNP(SELECTED FROM 2N3702)	2848C	1853-C02C
A207	1854-0071	12	TSTR:SI NPN(SELECTED FROM 2N3704)	2848C	1854-C071
A208	1854-0071		TSTR:SI NPN(SELECTED FROM 2N3704)	2848C	1854-C071
A209	1853-0020		TSTR:SI PNP(SELECTED FROM 2N3702)	2848C	1853-C02C
A2010	1853-0020		TSTR:SI PNP(SELECTED FROM 2N3702)	2848C	1853-C02C
A2011	1853-0020		TSTR:SI PNP(SELECTED FROM 2N3702)	2848C	1853-002C
A2012	1854-0071	1	TSTR:SI NPN(SELECTED FROM 2N3704)	2848C	1854-C071
A2013	1853-0020		TSTR:SI PNP(SELECTED FROM 2N3702)	2848C	1853-C02C
A2R1	0757-0420		RIFXD MET FLM 750 OHM 1% 1/8W	2848C	0757-042C
A2R2	0698-0082		RIFXD MET FLM 464 OHM 1% 1/8W	2848C	0698-0082
A2R3	0764-0015		RIFXD MET FLM 560 OHM 5% 2W	2848C	0764-0015
A2R4	0698-3637	1	RIFXD MET GX 820 OHM 5% 2W	2848C	0698-3637
A2R5	0757-C402		RIFXD MET FLM 110 OHM 1% 1/8W	2848C	0757-C402
A2R6	2100-1754		R:VAR WW 50 OHM 5% TYPE V 1W	2848C	2100-1754
A2R7	0757-0316		RIFXD MET FLM 42.2 OHM 1% 1/8W	2848C	0757-0316
A2R8	0757-0294		RIFXD MET FLM 17.8 OHM 1% 1/8W	2848C	0757-0294
A2R9	0757-0294	1	RIFXD MET FLM 17.8 OHM 1% 1/8W	2848C	0757-0294
A2R10	0757-0316		RIFXD MET FLM 42.2 OHM 1% 1/8W	2848C	0757-0316
A2R11	0757-0399		RIFXD MET FLM 82.5 OHM 1% 1/8W	2848C	0757-0399
A2R12	0757-C394		RIFXD MET FLM 51.1 OHM 1% 1/8W	2848C	0757-C394
A2R13	0698-C085		RIFXD MET FLM 2.61K OHM 1% 1/8W	2848C	0698-C085
A2R14	0757-0421	1	RIFXD MET FLM 825 OHM 1% 1/8W	2848C	0757-0421
A2R15	0698-0085		RIFXD MET FLM 2.61K OHM 1% 1/8W	2848C	0698-0085
A2R16	0757-0401		RIFXD MET FLM 100 OHM 1% 1/8W	2848C	0757-0401
A2R17	0757-0401		RIFXD MET FLM 100 OHM 1% 1/8W	2848C	0757-0401
A2R18	0757-0401		RIFXD MET FLM 100 OHM 1% 1/8W	2848C	0757-0401
A2R19	0757-0438	9	RIFXD MET FLM 5.11K OHM 1% 1/8W	2848C	0757-0438
A2R20	0757-0317		RIFXD MET FLM 1.33K OHM 1% 1/8W	2848C	0757-0317
A2R21	0757-1094		RIFXD MET FLM 1.47K OHM 1% 1/8W	2848C	0757-1094
A2R22	0757-029C		RIFXD MET FLM 6.19K OHM 1% 1/8W	2848C	0757-029C
A2R23	0698-3158		RIFXD MET FLM 23.7K OHM 1% 1/8W	2848C	0698-3158
A2R24	0698-3158	1	RIFXD MET FLM 23.7K OHM 1% 1/8W	2848C	0698-3158
A2R25	0757-1094		RIFXD MET FLM 1.47K OHM 1% 1/8W	2848C	0757-1094
A2R26	0757-029C		RIFXD MET FLM 6.19K OHM 1% 1/8W	2848C	0757-029C
A2R27	0757-0465		RIFXD MET FLM 100K OHM 1% 1/8W	2848C	0757-0465
A2R28	0757-0458		RIFXD MET FLM 51.1K OHM 1% 1/8W	2848C	0757-0458
A2R29	0757-0442	8	RIFXD MET FLM 10.0K OHM 1% 1/8W	2848C	0757-0442
A2R30	0757-0317		RIFXD MET FLM 1.33K OHM 1% 1/8W	2848C	0757-0317
A2R31	0757-0401		RIFXD MET FLM 100 OHM 1% 1/8W	2848C	0757-0401
A2R32	0698-0083		RIFXD MET FLM 1.96K OHM 1% 1/8W	2848C	0698-0083
A2R33	0757-0401		RIFXD MET FLM 100 OHM 1% 1/8W	2848C	0757-0401
A2R34	2100-1755	1	R:VAR WW 100 OHM 5% TYPE V 1W	2848C	2100-1755
A2R35	0757-0438		RIFXD MET FLM 5.11K OHM 1% 1/8W	2848C	0757-0438
A2R36	0757-0438		RIFXD MET FLM 5.11K OHM 1% 1/8W	2848C	0757-0438
A2R37	0757-0438		RIFXD MET FLM 5.11K OHM 1% 1/8W	2848C	0757-0438
A2R38	0757-0438		RIFXD MET FLM 5.11K OHM 1% 1/8W	2848C	0757-0438
A3	86601-60065	1	FEED BACK AMPLIFIER ASSY	2848C	86601-60065
A3C1	0160-2149	3	CIFXD MICA 30 PF 5% 300VDCW	2848C	0160-2149
A3C2	0160-4452		CIFXD DISC CER 0.02 UF 20% 100VDCW	56289	C0238101N23M529-CUM
A3C3	0160-2204		CIFXD MICA 100PF 5%	72134	MM15F1C1J3C
A3C4	0160-0190		CIFXD MICA 200 PF 5%	72136	MM15F211J3C
A3C5	0160-0058		CIFXD AL ELECT 50 UF +75-10% 25VDCW	56289	3C0954G025CC2-DSM
A3C6	0160-0157	1	CIFXD MY 0.0047 UF 10% 200VDCW	56289	142P47292-PTS
A3C7	0170-0040		CIFXD MY 0.0047 UF 10% 200VDCW	56289	142P47392-PTS
A3C8	0180-0197		CIFXD ELECT 2.2 UF 10% 20VDCW	56289	15C0225X5C20A2-DYS
A3C9	0180-0058		CIFXD AL ELECT 50 UF +75-10% 25VDCW	56289	3C0954G025CC2-DSM
A3C10	0160-3036		CIFXD CER 5000 PF +80-20% 200VDCW	2848C	0160-3036
A3C11	0160-3036	3	CIFXD CER 5000 PF +80-20% 200VDCW	2848C	0160-3036
A3C12	0160-3036		CIFXD CER 5000 PF +80-20% 200VDCW	2848C	0160-3036
A3C13	0160-3036		CIFXD CER 5000 PF +80-20% 200VDCW	2848C	0160-3036
A3C14	0160-3036		CIFXD CER 5000 PF +80-20% 200VDCW	2848C	0160-3036
A3C15	0160-3744		C:GER FEED-THRU 1000 PF 200VDCW	72982	2425-DJC-X500-1-27
A3CR1	1902-3036	3	DIODE:BRKACDWN 3.0V 5%	04713	5217939-10
A3CR2	1902-0048		DIODE:BRKACDWN 6.0V 5%	04713	5216939-134
A3CR3	1910-0018		CONNECTOR:RF 60 W/	2848C	1910-0018
A3J1	1290-1194		CONNECTOR:RF BULKHEAD RECEPTACLE	98291	92-049-001C
A3J2	1290-1194		CONNECTOR:RF BULKHEAD RECEPTACLE	98291	92-049-001C

See introduction to this section for ordering information

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
A3L1	9140-0158	3	COIL:FXD RF 1 UH 108	99800	1025-20
A3L2	9140-0237		COIL:FXD 200 UH 58	28480	9140-0237
A3L3	9140-0237		COIL:FXD 200 UH 58	28480	9140-0237
A3L4	9140-0237		COIL:FXD 200 UH 58	28480	9140-0237
A3MP1	86601-60062		1	BOARD ASSY:FEED BACK AMPLIFIER	28480
A3MP2	86601-20066	1	COVER:FEED BACK AMPLIFIER	28480	86601-20066
A3Q1	1855-0020		TSTR:SI FET N-CHANNEL	28480	1855-0020
A3Q2	1853-0020		TSTR:SI PNP(SELECTED FROM 2N3702)	28480	1853-0020
A3Q3	1853-0020		TSTR:SI PNP(SELECTED FROM 2N3702)	28480	1853-0020
A3Q4	1854-0071		TSTR:SI NPN(SELECTED FROM 2N3704)	28480	1854-0071
A3Q5	1854-0071	1	TSTR:SI NPN(SELECTED FROM 2N3704)	28480	1854-0071
A3Q6	1855-0020		TSTR:SI FET N-CHANNEL	28480	1855-0020
A3Q7	1855-0020		TSTR:SI FET N-CHANNEL	28480	1855-0020
A3Q8	1854-0071		TSTR:SI NPN(SELECTED FROM 2N3704)	28480	1854-0071
A3Q9	1853-0020		TSTR:SI PNP(SELECTED FROM 2N3702)	28480	1853-0020
A3R1	0698-3157	1	R:FXD MET FLM 19.6K OHM 1% 1/8W	28480	0698-3157
A3R2	0757-0442		R:FXD MET FLM 10.0K OHM 1% 1/8W	28480	0757-0442
A3R3	0757-0442		R:FXD MET FLM 10.0K OHM 1% 1/8W	28480	0757-0442
A3R4	0698-0083		R:FXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A3R5	0698-0083		R:FXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A3R6	0698-0083	1	R:FXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A3R7	0757-0442		R:FXD MET FLM 10.0K OHM 1% 1/8W	28480	0757-0442
A3R8	0757-0441		R:FXD MET FLM 68.1K OHM 1% 1/8W	28480	0757-0441
A3R9	0757-0442		R:FXD MET FLM 10.0K OHM 1% 1/8W	28480	0757-0442
A3R10	0757-0280		14	R:FXD MET FLM 1K OHM 1% 1/8W	28480
A3R11	0698-0083	1	R:FXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A3R12	0757-0280		R:FXD MET FLM 1K OHM 1% 1/8W	28480	0757-0280
A3R13	0757-0438		R:FXD MET FLM 5.11K OHM 1% 1/8W	28480	0757-0438
A3R14	0698-3161		R:FXD MET FLM 38.3K OHM 1% 1/8W	28480	0698-3161
A3R15	0757-0438		R:FXD MET FLM 5.11K OHM 1% 1/8W	28480	0757-0438
A3R16	0698-3132	1	R:FXD FLM 261 OHM 1% 1/8W	28480	0698-3132
A3R17	0698-0085		R:FXD MET FLM 2.61K OHM 1% 1/8W	28480	0698-0085
A3R18	0757-0447		R:FXD MET FLM 16.2K OHM 1% 1/8W	28480	0757-0447
A3R19	0757-0401		R:FXD MET FLM 100 OHM 1% 1/8W	28480	0757-0401
A3R20	0757-0438		R:FXD MET FLM 5.11K OHM 1% 1/8W	28480	0757-0438
A3R21	0698-3159	1	R:FXD MET FLM 26.1K OHM 1% 1/8W	28480	0698-3159
A3U1	1820-0476		BOARD AMP. HI-SPEED	07203	05F7715353
A4	86601-60023	1	FILTER ASSY:ACTIVE	28480	86601-60023
A4C1	0121-0465	13	C:VAR AIR 10 PF	28480	0121-0465
A4C2	0121-0465		C:VAR AIR 10 PF	28480	0121-0465
A4C3	0121-0465		C:VAR AIR 10 PF	28480	0121-0465
A4C4	0121-0465	1	C:VAR AIR 10 PF	28480	0121-0465
A4C5	C160-3036		C:FXD CER 5000 PF +80-20% 200VDCW	28480	0160-3036
A4C6	0160-3036		C:FXD CER 5000 PF +80-20% 200VDCW	28480	0160-3036
A4J1	1250-0901		CONNECTOR:RF BULKHEAD	15558	110 /D
A4J2	1250-0901		CONNECTOR:RF BULKHEAD	15558	1104/D
A4MP1	86601-40007	1	BOXTM:ACTIVE FILTER DIEL.	28480	86601-40007
A4MP2	86601-20037		INSERT:ACTIVE FILTER ASSY	28480	86601-20037
A4MP3	86601-20035		HOUSING:ACTIVE FILTER ASSY	28480	86601-20035
A4MP4	86601-20026		STRIPLINE	28480	86601-20026
A4MP5	86601-00009		COVER:ACTIVE FILTER ASSY	28480	86601-00009
A4A1	86601-60011	1	BOARD ASSY:INPUT AMPLIFIER	28480	86601-60011
A4A1C1	0160-3078	10	C:FXD CER 1000 PF 20% 100VDCW	28480	0160-3078
A4A1C2	0121-0447		C:VAR CER 1.0-2.5 PF 63VDCW	28480	0121-0447
A4A1C3	0160-3078		C:FXD CER 1000 PF 20% 100VDCW	28480	0160-3078
A4A1C4	0160-3078		C:FXD CER 1000 PF 20% 100VDCW	28480	0160-3078
A4A1C5	0160-3078		C:FXD CER 1000 PF 20% 100VDCW	28480	0160-3078
A4A1C6	0121-0447	4	C:VAR CER 1.0-2.5 PF 63VDCW	28480	0121-0447
A4A1C7	0160-3078		C:FXD CER 1000 PF 20% 100VDCW	28480	0160-3078
A4A1C8	0160-2247		COIL:FXD 20 0.1uH 108	28480	0160-2247
A4A1C9	1854-0345		T:TR:SI NPN	00131	245175
A4A1C10	1854-0345		T:TR:SI NPN	00131	245175
A4A1R1	0698-3079	8	R:FXD MET FLM 19.6 OHM 1% 1/8W	28480	0698-3079
A4A1R2	0698-3151		R:FXD MET FLM 2.67K OHM 1% 1/8W	28480	0698-3151
A4A1R3	0757-0439		R:FXD MET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A4A1R4	0698-3040		R:FXD MET FLM 19.6 OHM 1% 1/8W	28480	0698-3040
A4A1R5	0757-0439		R:FXD MET FLM 6.81K OHM 1% 1/8W	28480	0757-0439

See introduction to this section for ordering information.

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
A4A1R6 A4A1R7 A4A1R8 A4A1R9 A4A1R10	0698-3151 0698-3440 0698-3443 0757-0294 0698-3443	3	R:FXD MET FLN 2.87K OHM 1% 1/8W R:FXD MET FLN 196 OHM 1% 1/8W R:FXD MET FLN 287 OHM 1% 1/8W R:FXD MET FLN 17.9 OHM 1% 1/8W R:FXD MET FLN 287 OHM 1% 1/8W	2848C 2848C 2848C 2848C 2848C	0698-3151 0698-3440 0698-3443 0757-0294 0698-3443
A4A2	86601-60012	1	BOARD ASSY:OUTPUT AMPLIFIER	28480	86601-60012
A4A2C1 A4A2C2 A4A2C3 A4A2C4 A4A2C5	0160-3878 0160-3878 0121-0447 0160-3878 0160-3878		C:FXD CER 1000 PF 20% 100VDCW C:FXD CER 1000 PF 20% 100VDCW C:VAR CER 1.5-2.5 PF 63VDCW C:FXD CER 1000 PF 20% 100VDCW C:FXD CER 1000 PF 20% 100VDCW	80031 80031 2848C 80031 80031	CV2059X7R102M CV2059X7R102M 0121-0447 CV2059X7R102M CV2059X7R102M
A4A2C6 A4A2C7 A4A2L1 A4A2Q1 A4A2Q2	0121-0447 0160-3878 9100-2247 1854-0345 1854-0345		C:VAR CER 1.5-2.5 PF 63VDCW C:FXD CER 1000 PF 20% 100VDCW COIL:FXD RF 0.10 UH 10% TSTR:SI NPN TSTR:SI NPN	2848C 80031 28480 80131 80131	0121-0447 CV2059X7R102M 9100-2247 2N5179 2N5179
A4A2R1 A4A2R2 A4A2R3 A4A2R4 A4A2R5	0698-3429 0698-3151 0757-0439 0698-3440 0757-0439		R:FXD MET FLN 19.6 OHM 1% 1/8W R:FXD MET FLN 2.87K OHM 1% 1/8W R:FXD MET FLN 6.81K OHM 1% 1/8W R:FXD MET FLN 196 OHM 1% 1/8W R:FXD MET FLN 6.81K OHM 1% 1/8W	28480 28480 28480 28480 28480	0698-3429 0698-3151 0757-0439 0698-3440 0757-0439
A4A2R6 A4A2R7	0698-3151 0698-3440		R:FXD MET FLN 2.87K OHM 1% 1/8W R:FXD MET FLN 196 OHM 1% 1/8W	28480 28480	0698-3151 0698-3440
A5	86601-60080	1	MODULATOR ASSY	2848C	86601-60080
A5C1 A5C2 A5C3	0160-3036 0160-3036 0160-3036		C:FXD CER 5000 PF +80-20% 200VDCW C:FXD CER 5000 PF +80-20% 200VDCW C:FXD CER 5000 PF +80-20% 200VDCW	2848C 2848C 28480	0160-3036 0160-3036 0160-3036
A5J1 A5J2 A5J3 A5J4 A5MP1	1250-1194 1250-1194 1250-1194 1250-1194 86601-20065	1	CONNECTOR:RF BULKHEAD RECEPTACLE CONNECTOR:RF BULKHEAD RECEPTACLE CONNECTOR:RF BULKHEAD RECEPTACLE CONNECTOR:RF BULKHEAD RECEPTACLE DIVIDER:MODULATOR	98291 98291 98291 98291 2848C	52-045-4610 52-045-4610 52-045-4610 52-045-4610 86601-20065
A5MP2 A5MP3	86601-20067 86601-20072	1 1	CABLE:MODULATOR COVER:MODULATOR ASSY	2848C 2848C	86601-20067 86601-20072
A5A1	86601-60078	1	BOARD ASSY:MODULATOR	28480	86601-60078
ASA1C1 ASA1C2 ASA1C3 ASA1C4 ASA1C5	0160-3878 0121-0447 0160-3878 0160-3878 0121-0447		C:FXD CER 1000 PF 20% 100VDCW C:VAR CER 1.5-2.5 PF 63VDCW C:FXD CER 1000 PF 20% 100VDCW C:FXD CER 1000 PF 20% 100VDCW C:VAR CER 1.5-2.5 PF 63VDCW	80031 2848C 80031 80031 2848C	CV2059X7R102M 0121-0447 CV2059X7R102M CV2059X7R102M 0121-0447
ASA1C6 ASA1C7 ASA1C8 ASA1C9 ASA1C10	0160-3878 0160-2208 0160-3878 0160-3444 0160-3456	2 1 1 4	C:FXD CER 1000 PF 20% 100VDCW C:FXD MICA 330 PF 5% 300VDCW C:FXD CER 1000 PF 20% 100VDCW C:FXD CER 100 PF 10% 250VDCW C:FXD CER 1000 PF 10% 250VDCW	80031 2848C 80031 96289 96289	CV2059X7R102M 0160-2208 CV2059X7R102M C157P251F101K522-COM C067P251F102K522-COM
ASA1E1 ASA1E1 ASA1E1 ASA1E1 ASA1E1	0940-2070 0490-1013 08660-80005 08660-80005 9100-2247	2 1 4 1 1	MIXER:500 MHZ RELAY:REED 90J OHM 10% 5V INDUCTOR INDUCTOR COIL:FXD RF 0.10 UH 10%	2848C 18635 28480 2848C 2848C	0940-2070 R2840-1 08660-80005 08660-80005 9100-2247
ASA1E4 ASA1Q1 ASA1Q2 ASA1R1 ASA1R2	9140-0158 1854-0345 1854-0345 0698-3429 0757-0439		COIL:FXD RF 1 UH 10% TSTR:SI NPN TSTR:SI NPN R:FXD MET FLN 19.6 OHM 1% 1/8W R:FXD MET FLN 6.81K OHM 1% 1/8W	9900C 80131 80131 28480 2848C	1025-20 2N5179 2N5179 0698-3429 0757-0439
ASA1R3 ASA1R4 ASA1R5 ASA1R6 ASA1R7	0698-3151 0698-3440 0757-0294 0698-3151 0698-3440		R:FXD MET FLN 2.87K OHM 1% 1/8W R:FXD MET FLN 196 OHM 1% 1/8W R:FXD MET FLN 6.81K OHM 1% 1/8W R:FXD MET FLN 2.87K OHM 1% 1/8W R:FXD MET FLN 196 OHM 1% 1/8W	2848C 2848C 2848C 2848C 2848C	0698-3151 0698-3440 0757-0294 0698-3151 0698-3440
ASA1R8 ASA1R9 ASA1R10	0757-0280 0757-0280 0757-1000	1	R:FXD MET FLN 1% OHM 1% 1/8W R:FXD MET FLN 1% OHM 1% 1/8W R:FXD MET FLN 91.1 OHM 1% 1/8W	2848C 2848C 2848C	0757-0280 0757-0280 0757-1000

See introduction to this section for ordering information

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
A5A2	86601-60060	1	BOARD ASSY:MODULATOR II	28480	86601-60060
A5A2C1	0160-3878		C:FXD CER 100C PF 20% 100VDCW	80031	CV2059X7R102M
A5A2C2	0121-0447		C:VAR CER 1.5-2.5 PF 63VDCW	28480	0121-0447
A5A2C3	0160-3878		C:FXD CER 1000 PF 20% 100VDCW	80031	CV2059X7R102M
A5A2C4	0121-0447		C:VAR CER 1.5-2.5 PF 63VDCW	28480	0121-0447
A5A2C5	0160-3878		C:FXD CER 1000 PF 20% 100VDCW	80031	CV2059X7R102M
A5A2C6	0160-3878		C:FXD CER 1000 PF 20% 100VDCW	80031	CV2059X7R102M
A5A2C7	0160-3878		C:FXD CER 1000 PF 20% 100VDCW	80031	CV2059X7R102M
A5A2C8	0160-2208		C:FXD MICA 330 PF 5% 300VDCW	28480	0160-2208
A5A2E1	0960-2070		MIXER:500 MHZ	28480	0560-2070
A5A2L1	08660-80005		INDUCTOR	28480	08660-80005
A5A2L2	08660-80005		INDUCTOR	28480	08660-80005
A5A2L3	9100-2247		COIL:FXD RF 0.10 UH 10% COIL:FXD RF 1 UH 10%	28480	9100-2247
A5A2L4	9140-0158		COIL:FXD RF 1 UH 10%	99800	1025-20
A5A2Q1	1854-0345		TSTR:SI NPN	80131	2N5175
A5A2Q2	1854-0345		TSTR:SI NPN	80131	2N5175
A5A2R1	0757-0439		R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A5A2R2	0698-3151		R:FXD NET FLM 2.87K OHM 1% 1/8W	28480	0698-3151
A5A2R3	0698-3440		R:FXD NET FLM 196 OHM 1% 1/8W	28480	0698-3440
A5A2R4	0757-0439		R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A5A2R5	0698-3151		R:FXD NET FLM 2.87K OHM 1% 1/8W	28480	0698-3151
A5A2R6	0698-3440		R:FXD NET FLM 196 OHM 1% 1/8W	28480	0698-3440
A5A2R7	0757-0280		R:FXD NET FLM 1K OHM 1% 1/8W	28480	0757-0280
A5A2R8	0757-0280		R:FXD NET FLM 1K OHM 1% 1/8W	28480	0757-0280
A6	86601-60017	1	PRE-AMPLIFIER ASSY	28480	86601-60017
A6C1	0160-2058		C:FXD AL ELECT 50 UF +75-10% 25VDCW	56289	30D506G025CC2-DSM
A6C2	0160-2306		C:FXD MICA 27 PF 5%	28480	0160-2306
A6C3	0160-2306		C:FXD MICA 27 PF 5%	28480	0160-2306
A6C4	0160-0197		C:FXD ELECT 2.2 UF 10% 20VDCW	56289	1500225X9020A2-OVS
A6C5	0160-2150		C:FXD MICA 33 PF 5%	28480	0160-2150
A6C6	0160-3456		C:FXD CER 1000 PF 10% 250VDCW	56289	C067F251F102K522-COM
A6C7	0160-3456		C:FXD CER 1000 PF 10% 250VDCW	56289	C067F251F102K522-COM
A6C8	0160-2055		C:FXD CER 0.01 UF +80-20% 100VDCW	56289	C023F101F103J522-COM
A6C9	0160-0197		C:FXD ELECT 2.2 UF 10% 20VDCW	56289	1500225X9020A2-OVS
A6C10	0160-0197		C:FXD ELECT 2.2 UF 10% 20VDCW	56289	1500225X9020A2-OVS
A6C11	0160-0197		C:FXD ELECT 2.2 UF 10% 20VDCW	56289	1500225X9020A2-OVS
A6C12	0160-3456		C:FXD CER 1000 PF 10% 250VDCW	56289	C067F251F102K522-COM
A6C13	0160-0197		C:FXD ELECT 2.2 UF 10% 20VDCW	56289	1500225X9020A2-OVS
A6C14	0160-3036		C:FXD CER 5000 PF +80-20% 200VDCW	28480	0160-3036
A6C15	0160-3036		C:FXD CER 5000 PF +80-20% 200VDCW	28480	0160-3036
A6CR1	1902-0048		DIODE:BREAKDOWN 6.81V 5% DIODE:BREAKDOWN 6.81V 5%	04713	SZ10030-134
A6CR2	1902-0048		DIODE:BREAKDOWN 6.81V 5% DIODE:BREAKDOWN 6.81V 5%	04713	SZ10030-134
A6J1	1250-0901		CONNECTOR:RF BULKHEAD	15550	110-70
A6J2	1250-0901		CONNECTOR:RF BULKHEAD	15550	1104/0
A6L1	9100-1627		CGIL/CHOKO 39 UH 5%	82142	15-1319-2J
A6L2	86601-80004	2	CGIL	28480	06601-80004
A6L3	9100-2248	1	CGIL/CHOKO 0.12 UH 10%	82142	09-4416-2K
A6L4	86601-80004	1	CGIL	28480	06601-80004
A6MP1	86601-20023	1	COVER:PRE-AMPLIFIER ASSY	28480	06601-20023
A6MP2	86601-60002	1	BOARD ASSY:PRE-AMPLIFIER	28480	86601-60002
A6Q1	1854-0345		TSTR:SI NPN	80131	2N5175
A6Q2	1854-0345		TSTR:SI NPN	80131	2N5175
A6Q3	1854-0345		TSTR:SI NPN	80131	2N5175
A6Q4	1854-0345		TSTR:SI NPN	80131	2N5175
A6R1	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R2	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R3	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R4	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R5	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R6	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R7	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R8	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R9	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R10	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R11	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R12	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R13	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R14	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R15	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R16	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R17	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R18	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R19	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R20	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R21	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R22	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R23	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R24	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439
A6R25	0757-0439	1	R:FXD NET FLM 6.81K OHM 1% 1/8W	28480	0757-0439

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
A7	86601-60009	1	BOARD ASSY:INTEGR	2848C	86601-60009
ATP1	1251-2857	2	CONNECTOR STRIP:14 MALE CONTACT	02660	221-1515
ATXA7	1251-2857		CONNECTOR STRIP:14 MALE CONTACT	0266C	221-1515
ATXA8	1251-1626	1	CONNECTOR:PC (2 X 12) 24 CONTACT	71785	252-12-30-300
ATXA9	1251-2834	1	CONNECTOR:PC EDGE (2 X 10) 20 CONTACT	71785	252-10-30-300
ATXA10	1251-1388	1	CONNECTOR:PC (2 X 15) 30 CONTACT	71785	252-15-30-008
A8	86601-60006	1	BOARD ASSY:ATTENUATOR DRIVER FOR OPTION 001, OMIT A8	2848C	86601-60006
ABCR1	1902-3002	4	DIODE BREAKDOWN:2.37V 5%	28480	1502-3002
ABCR2	1902-3002		DIODE BREAKDOWN:2.37V 5%	28480	1902-3002
ABCR3	1902-3002		DIODE BREAKDOWN:2.37V 5%	28480	1502-3002
ABCR4	1902-3002		DIODE BREAKDOWN:2.37V 5%	2848C	1902-3002
ABCR5	1901-0025	9	DIODE:SILICON 100MA/1V	07263	FD 2387
ABCR6	1901-0025		DIODE:SILICON 100MA/1V	07263	FD 2387
ABCR7	1901-0025		DIODE:SILICON 100MA/1V	07263	FD 2387
ABCR8	1901-0025		DIODE:SILICON 100MA/1V	07263	FD 2387
ABCR9	1901-0025		DIODE:SILICON 100MA/1V	07263	FD 2387
ABCR10	1901-0025		DIODE:SILICON 100MA/1V	07263	FD 2387
ABCR11	1901-0025		DIODE:SILICON 100MA/1V	07263	FD 2387
ABCR12	1901-0025		DIODE:SILICON 100MA/1V	07263	FD 2387
A:Q1	1853-0213	4	TSTR:SI PNP	80131	2N4236
A:Q2	1854-0361	4	TSTR:SI NPN	80131	2N4235
A:Q3	1853-0213		TSTR:SI PNP	80131	2N4236
A:Q4	1854-0361		TSTR:SI NPN	80131	2N4235
A:Q5	1854-0071		TSTR:SI NPN(SELECTED FROM 2N3704)	28480	1854-0071
A:Q6	1853-0020		TSTR:SI PNP(SELECTED FROM 2N3702)	2848C	1853-0020
A:Q7	1854-0071		TSTR:SI NPN(SELECTED FROM 2N3704)	28480	1854-0071
A:Q8	1853-0020		TSTR:SI PNP(SELECTED FROM 2N3702)	28480	1853-0020
A:Q9	1853-0213		TSTR:SI PNP	80131	2N4236
A:Q10	1854-0361		TSTR:SI NPN	80131	2N4235
A:Q11	1853-0213		TSTR:SI PNP	80131	2N4236
A:Q12	1854-0361		TSTR:SI NPN	80131	2N4235
A:Q13	1854-0071		TSTR:SI NPN(SELECTED FROM 2N3704)	28480	1854-0071
A:Q14	1853-0020		TSTR:SI PNP(SELECTED FROM 2N3702)	28480	1853-0020
A:Q15	1854-0071		TSTR:SI NPN(SELECTED FROM 2N3704)	28480	1854-0071
A:Q16	1853-0020		TSTR:SI PNP(SELECTED FROM 2N3702)	28480	1853-0020
AB:1	0757-0280		RIFXD MET FLN 1K OHM 1% 1/8W	28480	0757-0280
AB:2	0757-0280		RIFXD MET FLN 1K OHM 1% 1/8W	28480	0757-0280
AB:3	0757-0280		RIFXD MET FLN 1K OHM 1% 1/8W	28480	0757-0280
AB:4	0757-0280		RIFXD MET FLN 1K OHM 1% 1/8W	28480	0757-0280
AB:5	0757-0159	8	RIFXD MET FLN 1000 OHM 1% 1/2W	28480	0757-0159
AB:6	0698-3440		RIFXD MET FLN 1% OHM 1% 1/8W	28480	0698-3440
AB:7	0757-0159		RIFXD MET FLN 1000 OHM 1% 1/2W	28480	0757-0159
AB:8	0757-0159		RIFXD MET FLN 1000 OHM 1% 1/2W	28480	0757-0159
AB:9	0698-3440		RIFXD MET FLN 1% OHM 1% 1/8W	28480	0698-3440
AB:10	0757-0159		RIFXD MET FLN 1000 OHM 1% 1/2W	28480	0757-0159
AB:11	0757-0159		RIFXD MET FLN 1000 OHM 1% 1/2W	28480	0757-0159
AB:12	0698-3440		RIFXD MET FLN 1% OHM 1% 1/8W	28480	0698-3440
AB:13	0757-0159		RIFXD MET FLN 1000 OHM 1% 1/2W	28480	0757-0159
AB:14	0757-0159		RIFXD MET FLN 1000 OHM 1% 1/2W	28480	0757-0159
AB:15	0757-0401		RIFXD MET FLN 100 OHM 1% 1/8W	28480	0757-0401
AB:16	0757-0159		RIFXD MET FLN 1000 OHM 1% 1/2W	28480	0757-0159
AB:17	0698-0082		RIFXD MET FLN 464 OHM 1% 1/8W	28480	0698-0082
AB:18	0698-0082		RIFXD MET FLN 464 OHM 1% 1/8W	28480	0698-0082
AB:19	0698-0082		RIFXD MET FLN 464 OHM 1% 1/8W	28480	0698-0082
AB:20	0698-0082		RIFXD MET FLN 464 OHM 1% 1/8W	28480	0698-0082
AB:21	0698-0082		RIFXD MET FLN 464 OHM 1% 1/8W	28480	0698-0082
AB:22	0698-0082		RIFXD MET FLN 464 OHM 1% 1/8W	28480	0698-0082
AB:23	0698-0082		RIFXD MET FLN 464 OHM 1% 1/8W	28480	0698-0082
AB:24	0698-0082		RIFXD MET FLN 464 OHM 1% 1/8W	28480	0698-0082
A9	86601-60003	1	BOARD ASSY:REFERENCE	28480	86601-60003
A9E1	0160-2226	1	CIFXD MECA 2200 PF 5% 100VDC	2848C	0160-2226
A9E1E1	1902-0041		DIODE:GERMANYUM 9.11V 5%	04713	5210910-18

See introduction to this section for ordering information

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
A9CR2	1901-0225	6	DIODE: SILICON 100MA/1V	07263	FD 2387
A9K1	0490-0916		RELAY: REED 1 FORM A 0.5 AMP	15636	RA30231051
A9K2	0490-0916		RELAY: REED 1 FORM A 0.5 AMP	15636	RA30231051
A9K3	0490-0916		RELAY: REED 1 FORM A 0.5 AMP	15636	RA30231051
A9K4	0490-0916		RELAY: REED 1 FORM A 0.5 AMP	15636	RA30231051
A9K5	0490-0916	5	RELAY: REED 1 FORM A 0.5 AMP	15636	RA30231051
A9K6	0490-0916		RELAY: REED 1 FORM A 0.5 AMP	15636	RA30231051
A9Q1	1854-0071		TSTR: SI NPN (SELECTED FROM 2N3704)	28480	1854-0071
A9Q2	1853-0015		TSTR: SI PNP	80131	2N3640
A9Q3	1853-0015		TSTR: SI PNP	80131	2N3640
A9Q4	1853-0322	4	TSTR: SI PNP	80131	2N2946A
A9Q5	1853-0015		TSTR: SI PNP	80131	2N3640
A9Q6	1853-0322		TSTR: SI PNP	80131	2N2946A
A9Q7	1853-0015		TSTR: SI PNP	80131	2N3640
A9Q8	1853-0322		TSTR: SI PNP	80131	2N2946A
A9Q9	1853-0015	2	TSTR: SI PNP	80131	2N3640
A9Q10	1854-0071		TSTR: SI NPN (SELECTED FROM 2N3704)	28480	1854-0071
A9Q11	1853-0322		TSTR: SI PNP	80131	2N2946A
A9R1	0757-0418		RIFXD MET FLM 619 OHM 1% 1/8W	28480	0757-0418
A9R2	2100-2413		RIVAR FLM 200 OHM 10% LIN 1/2W	28480	2100-2413
A9R3	0757-0418	1	RIFXD MET FLM 619 OHM 1% 1/8W	28480	0757-0418
A9R4	0698-3443		RIFXD MET FLM 287 OHM 1% 1/8W	28480	0698-3443
A9R5	0757-0442		RIFXD MET FLM 10.0K OHM 1% 1/8W	28480	0757-0442
A9R6	0757-0442		RIFXD MET FLM 10.0K OHM 1% 1/8W	28480	0757-0442
A9R7	0698-3446		RIFXD MET FLM 303 OHM 1% 1/8W	28480	0698-3446
A9R8	0757-0280	1	RIFXD MET FLM 1K OHM 1% 1/8W	28480	0757-0280
A9R9	0698-0083		RIFXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A9R10	0698-0083		RIFXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A9R11	0698-0083		RIFXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A9R12	0698-0083		RIFXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A9R13	2100-2633	2	RIVAR GERMET 1K OHM 10% LIN 1/2W	28480	2100-2633
A9R14	0757-0280		RIFXD MET FLM 1K OHM 1% 1/8W	28480	0757-0280
A9R15	0757-0442		RIFXD MET FLM 10.0K OHM 1% 1/8W	28480	0757-0442
A9R16	0698-0083		RIFXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A9R17	0698-0083		RIFXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A9R18	0698-0083	1	RIFXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A9R19	0698-0083		RIFXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A9R20	0698-0083		RIFXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A9R21	0698-4482		RIFXD FLM 17.4K OHM 1% 1/8W	28480	0698-4482
A9R22	0698-3498		RIFXD MET FLM 8.66K OHM 1% 1/8W	28480	0698-3498
A9R23	0698-3154	1	RIFXD MET FLM 4.22K OHM 1% 1/8W	28480	0698-3154
A9R24	0698-4430		RIFXD FLM 1.91K OHM 1% 1/8W	28480	0698-4430
A9R25	0698-4406		RIFXD FLM 119 OHM 1% 1/8W	28480	0698-4406
A9R26	0698-4406		RIFXD FLM 119 OHM 1% 1/8W	28480	0698-4406
A9R27	0698-3486		RIFXD FLM 232 OHM 1% 1/8W	28480	0698-3486
A9R28	0698-3486	2	RIFXD FLM 232 OHM 1% 1/8W	28480	0698-3486
A9R29	0698-3510		RIFXD MET FLM 453 OHM 1% 1/8W	28480	0698-3510
A9R30	0698-3510		RIFXD MET FLM 453 OHM 1% 1/8W	28480	0698-3510
A9R31	0698-3495		RIFXD MET FLM 806 OHM 1% 1/8W	28480	0698-3495
A9R32	2100-2633		RIVAR GERMET 1K OHM 10% LIN 1/2W	28480	2100-2633
A9R33	0698-3495	1	RIFXD MET FLM 806 OHM 1% 1/8W	28480	0698-3495
A9R34	2100-2632		RIVAR FLM 100 OHM 10% LIN 1/2W	28480	2100-2632
A9R35	0698-0083		RIFXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A9R36	0698-3453		RIFXD MET FLM 196K OHM 1% 1/8W	28480	0698-3453
A9R37	0698-3150		RIFXD MET FLM 2.37K OHM 1% 1/8W	28480	0698-3150
A9U1	1020-0201	1	INTEGRATED CIRCUIT: OPERATIONAL AMPL	04713	MC1439C
A10	86601-00000	1	PGA-D ASSY: LOGIC	28480	86601-00000
A10C1	0180-0270	1	CIRCUIT BOARD 22 OF 108 (10VDC)	01295	367600A
A10L1	1020-0277		CIRCUIT BOARD 20 OF 108	01295	367600A
A10U1	1020-0277		CIRCUIT BOARD 20 OF 108	01295	367600A
A10U2	1020-0277		CIRCUIT BOARD 20 OF 108	01295	367600A
A10U3	1020-0277	1	CIRCUIT BOARD 20 OF 108	01295	367600A
A10U4	1020-0277		CIRCUIT BOARD 20 OF 108	01295	367600A
A10U5	1020-0277		CIRCUIT BOARD 20 OF 108	01295	367600A
A10U6	1020-0277		CIRCUIT BOARD 20 OF 108	01295	367600A
A10U7	1020-0277	1	CIRCUIT BOARD 20 OF 108	01295	367600A
A11	86601-00000	1	WIRING BOARD: STRAP	28480	86601-00000

See Introduction to this section for ordering information.

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
A11MP1	1251-1313	13	CONNECTOR: F & P FEMALE CONNECTOR	6244C	220-502
A11MP2	1251-2858	1	CONNECTOR: BODY: 15-OPEN POSITIONS	7444B	7444B
A11MP3	1251-3087	10	CONNECTOR: F & P CONNECTOR 016 FEMALE	8131C	1CG-09C85
A11M1	86601-60041	1	CONNECTOR FACE: 66-PIN	2848C	5040-C343
			SEE W1	2848C	86601-60041
A11M7	86601-60037	2	SEE W3	2848C	86601-60037
A11M8	86601-60038	2	SEE W6	2848C	86601-60038
A11M11	86601-60040	2	SEE W11	2848C	86601-60040
A11M17	86601-60049	2	SEE W17	2848C	86601-60049
A11M18	86601-60086	2	SEE W18	2848C	86601-60086
A12	86601-60022	1	FILTER ASSY: DUAL	2848C	86601-60022
A12J1	1250-0901		CONNECTOR: RF BULKHEAD	1555B	11C4/D
A12J2	1250-0901		CONNECTOR: PF BULKHEAD	1555B	11C4/D
A12J3	1250-0901		CONNECTOR: RF BULKHEAD	1555B	11C4/D
A12J4	1250-0901		CONNECTOR: RF BULKHEAD	1555B	11C4/D
A12MP1	86601-30004	1	COVER: DUAL FILTER	2848C	86601-30004
A12MP2	86601-00025	1	GASKET	2848C	86601-00025
A12MP3	86601-20027	1	STRIPLINE-455	2848C	86601-20027
A12MP4	86601-20028	1	STRIPLINE-500	2848C	86601-20028
A12MP5	86601-20030	1	INSERT-455	2848C	86601-20030
A12MP6	86601-20031	1	INSERT-500	2848C	86601-20031
A12MP7	86601-20034	1	HCUSING: DUAL FILTER	2848C	86601-20034
A12MP8	86601-40003	2	BOTTOM-455 DIELECT	2848C	86601-40003
A12M8	86601-40005	2	BOTTOM-500 DIELECT	2848C	86601-40005
A12A1	0121-0465		BAND PASS FILTER: 500 MHZ	2848C	0121-0465
A12A1C1	0121-0465		C:VAR AIR 10 PF	2848C	0121-0465
A12A1C2	0121-0465		C:VAR AIR 10 PF	2848C	0121-0465
A12A2	0121-0465		BAND PASS FILTER: 450-460 MHZ	2848C	0121-0465
A12A2C1	0121-0465		C:VAR AIR 10 PF	2848C	0121-0465
A12A2C2	0121-0465		C:VAR AIR 10 PF	2848C	0121-0465
A12A2C3	0121-0465		C:VAR AIR 10 PF	2848C	0121-0465
A12A2C4	0121-0465		C:VAR AIR 10 PF	2848C	0121-0465
A12A2C5	0121-0465		C:VAR AIR 10 PF	2848C	0121-0465
A12A2C6	0121-0465		C:VAR AIR 10 PF	2848C	0121-0465
A12A2C7	0121-0465		C:VAR AIR 10 PF	2848C	0121-0465
A13	86601-60039	1	ATTENUATOR ASSY: S SECTION FOR OPTION 001, OMIT A13.	2848C	86601-60039
A14	86601-60021	1	FILTER ASSY: LOW PASS	2848C	86601-60021
A14C1	0160-2150		C:FXD MICA 33 PF 58	2848C	0160-2150
A14C2	0160-2257	1	C:FXD CER 10 PF 58 300VDCW	72982	3C1-0C0-C0HC-100J
A14C3	0160-2308	1	C:FXD MICA 36 PF 58	2848C	C160-2308
A14C4	0160-2200	1	C:FXD MICA 83 PF 58	72136	RD015E4J0J3C
A14C5	0160-2199		C:FXD MICA 30 PF 58 300VDCW	2848C	C160-2199
A14C6	0160-2199		C:FXD MICA 30 PF 58 300VDCW	2848C	C160-2199
A14C7	0160-2265	1	C:FXD CER 22 PF 58 300VDCW	72982	3C1-NPG-22PF
A14L1	86601-80001	1	COIL: FXD 47	2848C	86601-80001
A14L2	86601-80002	1	COIL: 12 T	2848C	86601-80002
A14L3	86601-80003	1	COIL: 12-1/2 T	2848C	86601-80003
A14MP1	86601-60010	1	BOARD ASSY: LOW PASS FILTER	2848C	86601-60010
A14MP2	7100-1042	1	CONNECTOR: RECTANGULAR 0.954" X 2.331"	02673	HU-3794-CA-CRS-HYD
A14MP3	10514-0005	1	BRACKET: 155L	2848C	10514-0005
A14J1	1250-1021	2	CONNECTOR: RF 50 OHM SNAP ON TYPE	98291	51-043-4610
A14J2	1250-1021	2	CONNECTOR: RF 50 OHM SNAP ON TYPE	98291	51-043-4610
A14MP4	86601-00027	1	CAN: LP FILTER	2848C	86601-00027
A15	10514A-004/H58	1	MIXER: DOUBLE BALANCED	2848C	10514A-004/H58
A16	10514A-OPT 004	2	MIXER DOUBLE BALANCED	2848C	10514A-OPT 004

See Introduction to this section for ordering information

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
A17	10514A-004		MIXER-DOUBLE BALANCED	28480	10514A-004
A18	86601-60091	1	WIRING HARNESS:MAIN	28480	86601-60091
A18MP1	1200-0063	17	LUG:CRIMP	28480	1200-0063
A18MP2	1251-2262	2	CONNECTOR:PC12 X 10120 CONTACTS	76530	251-10-30-400
A18MP3	1251-3087		CONTACT:R & P CONNECTOR #16 FEMALE	81312	100-05085
A18MP4	5020-C176	17	INSULATOR FOR SNAP-ON PINS	28480	5020-0176
A19	86601-60089	2	CABLE ASSY GRAY/YEL	28480	86601-60089
A19W4	86601-60030	1	SEE W4	28480	86601-60030
A19W8	86601-60069	2	SEE W8	28480	86601-60069
A19W9	86601-60068	2	SEE W9	28480	86601-60068
A19W10	86601-60071	2	SEE W10	28480	86601-60071
A19W13	86601-60032	2	SEE W13	28480	86601-60032
A19W19	86601-60070	2	SEE W19	28480	86601-60070
W1	86601-60041		CABLE ASSY:WHITE/GREEN	28480	86601-60041
W2	86601-60035	1	CABLE ASSY:GRAY	28480	86601-60035
W3	86601-60037		CABLE ASSY:WHITE/RED	28480	86601-60037
W4	86601-60089		CABLE ASSY GRAY/YEL	28480	86601-60089
W5	86601-60029	1	CABLE ASSY:GRAY/ORANGE	28480	86601-60029
W6	86601-60038		CABLE ASSY:WHITE/ORANGE	28480	86601-60038
W7	86601-60034	1	CABLE ASSY:GRAY	28480	86601-60034
W8	86601-60069		CABLE ASSY:GRAY/WHI E	28480	86601-60069
W9	86601-60068		CABLE ASSY:GRAY/BLACK	28480	86601-60068
W10	86601-60071		CABLE ASSY:GRAY/GREEN	28480	86601-60071
W11	86601-60040		CABLE ASSY:WHITE/YELLOW	28480	86601-60040
W12	86601-60036	1	CABLE ASSY:GRAY	28480	86601-60036
W13	86601-60032		CABLE ASSY:GRAY/BLUE	28480	86601-60032
W14	86601-60027	1	CABLE ASSY:GRAY/RED	28480	86601-60027
W15	86601-60026	1	CABLE ASSY:GRAY/BROWN	28480	86601-60026
W16	86601-60059	1	CABLE ASSY:ATTENUATOR, GRAY (FOR OPTION 001)	28480	86601-60059
W16	86601-60028	1	CABLE ASSY:ATTENUATOR, GRAY FOR OPTION 001 OMIT 86601-60028	28480	86601-60028
W17	86601-60049		CABLE ASSY:GRAY/ORANGE	28480	86601-60049
W18	86601-60086		CABLE ASSY:WHITE/GREEN	28480	86601-60086
W19	86601-60070		CABLE ASSY:GRAY/VIOLET	28480	86601-60070
KA7-1	1251-2500	1	CONNECTOR:PC EDGE12 X 6112 CONTACT	71785	251-06-30-400
KA7-2	1251-2262	1	CONNECTOR:PC12 X 10120 CONTACTS	76530	251-10-30-400
			MISCELLANEOUS		
	0370-1089	1	KNOB:RND JADE GRAY FOR 0.125" DIA SHAFT	28480	0370-1089
	0370-2108	1	KNOB:BAR W/SKIRT, JADE GRAY	28480	0370-2108
	1250-0914	1	BODY:RF CONNECTOR FOR OPTION 001 ONLY	67460	131-150
	1750-0915	1	CONTACT:RF CONNECTOR FOR OPTION 001 ONLY	02660	131-149
	7120-0004	1	NAMEPLATE:SERIAL	28480	7120-0004
	7124-1688	1	LABEL:ID(MODEL/OPTION)	28480	7124-1688
	5040-0306	1	INSULATOR FOR OPTION 001 ONLY	28480	5040-0306
	08555-20093	1	CENTER CONDUCTOR FOR OPTION 001 ONLY	28480	08555-20093
	08559-20094	1	BODY:BULKHEAD FOR OPTION 001 ONLY	28480	08559-20094
	08761-2027	1	INSULATOR FOR OPTION 001 ONLY	28480	08761-2027
	86601-00001	1	PANEL:FRONT	28480	86601-00001
			FOR STANDARD INSTRUMENT ONLY		
	86601-00002	1	MOUNT:METER	28480	86601-00002
	86601-00006	1	BRACKET:RIBBER	28480	86601-00006
	86601-00013	1	LATCH	28480	86601-00013
	86601-00014	1	BRACKET:ATTENUATOR	28480	86601-00014
			FOR STANDARD INSTRUMENT ONLY		
	86601-00028	1	PANEL:FRONT	28480	86601-00028
			FOR OPTION 001 ONLY		
	86601-00029	1	CABLE:ROUTER	28480	86601-00029
	86601-00030	1	CIRCUIT BOARD ASSY	28480	86601-00030

See Introduction to this section for ordering information

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
	86601-20013	2	EXTRUSION:SHIELD	2848C	86601-20013
	86601-20014	1	EXTRUSION:END PLATE	2848C	86601-20014
	86601-20015	2	EXTRUSION:DIVIDER	2848C	86601-20015
	86601-20016	1	FRAME:FRONT PANEL	28480	86601-20016
	86601-20018	1	PANEL:REAR	2848C	86601-20018
	86601-20019	1	STUD LATCH	2848C	86601-20019
	86601-20020	1	WASHER:LATCH	2848C	86601-20020
	86601-20051	1	WINDOW	28480	86601-20051
	86601-40017	1	SCREW:METER ADJUST	2848C	86601-40017

See Introduction to this section for ordering information

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
A3	86601-60019	1	FEED-BACK AMPLIFIER ASSY	28480	86601-60019
A3C1	G180-0058	2	C:FXD AL ELECT 50 UF +75-10% 25VDCM	56285	3005066025CC2-DSM
A3C2	0180-0058		C:FXD AL ELECT 50 UF +75-10% 25VDCM	56285	3005066025CC2-DSM
A3C3	0160-2204	1	C:FXD MICA 100PF 5% 72136		RDML5F101J3C
A3C4	0140-0198	2	C:FXD MICA 200 PF 5% 72136		RDML5F201J3C
A3C5	0160-2199	1	C:FXD MICA 30 PF 5% 300VDCM	28480	0160-2159
A3C6	0160-3452	1	C:FXD DISC CER 0.02 UF 20% 100VDCM	56285	C0238101H203MS25-COM
A3C7	0180-1733	1	C:FXD ELECT 0.22 UF 10% 35VDCM	28480	0180-1735
A3C8	0180-0116	1	C:FXD ELECT 6.8 UF 10% 35VDCM	56285	1500465X903582-OVS
A3C9	0160-0158	1	C:FXD MY 0.0056 UF 10% 200VDCM	56285	152PS6252-PTS
A3C10	0160-3063	5	C:FXD MICA 390 PF 5% 300VDCM	00853	RDML9F391J35
A3C11	0160-3063		C:FXD MICA 390 PF 5% 300VDCM	00853	RDML9F391J35
A3C12	0160-3063		C:FXD MICA 390 PF 5% 300VDCM	00853	RDML9F391J35
A3C13	0160-3063		C:FXD MICA 390 PF 5% 300VDCM	00853	RDML9F391J35
A3C14	0160-3063		C:FXD MICA 390 PF 5% 300VDCM	00853	RDML9F391J35
A3C15	0160-3744	1	C:CER FEED-THRU 1000 PF 200VDCM	72982	2425-C00-X5U0-102Z
A3CR1	1902-0041	2	DIODE: BREAKDOWN 5.11V 5% 04713		5210935-58
A3CR2	1902-3036	1	DIODE: BREAKDOWN 3.16V 5% 04713		5210935-36
A3J1	1250-0901	5	CONNECTOR:RF BULKHEAD	15558	1104/D
A3J2	1250-0901		CONNECTOR:RF BULKHEAD	15558	1104/D
A3L1	9140-1058	1	COIL/CHOKE 1 UH	28480	9140-1058
A3L2	9140-0237	3	COIL:FXD 200 UH 5% 28480		9140-0237
A3L3	9140-0237		COIL:FXD 200 UH 5% 28480		9140-0237
A3L4	9140-0237		COIL:FXD 200 UH 5% 28480		9140-0237
A3L5	9100-1667	1	COIL/CHOKE 3900 UH 5% 82142		24-1313-20J
A3MP1	86601-00025	1	GASKET	28480	86601-00025
A3MP2	86601-60004	1	BOARD ASSY:FEED-BACK AMPLIFIER	28480	86601-60004
A3Q1	1855-0020	3	TSTR:SI FET N-CHANNEL	28480	1855-0020
A3Q2	1853-0020	3	TSTR:SI NPNISELECTED FROM 2N3702)	28480	1853-0020
A3Q3	1853-0020		TSTR:SI NPNISELECTED FROM 2N3702)	28480	1853-0020
A3Q4	1854-0071	5	TSTR:SI NPNISELECTED FROM 2N3704)	28480	1854-0071
A3Q5	1854-0071		TSTR:SI NPNISELECTED FROM 2N3704)	28480	1854-0071
A3Q6	1855-0020		TSTR:SI FET N-CHANNEL	28480	1855-0020
A3Q7	1855-0020		TSTR:SI FET N-CHANNEL	28480	1855-0020
A3Q8	1854-0071		TSTR:SI NPNISELECTED FROM 2N3704)	28480	1854-0071
A3Q9	1853-0020		TSTR:SI NPNISELECTED FROM 2N3702)	28480	1853-0020
A3R1	0698-3150	1	R:FXD MET FLM 2.37K OHM 1% 1/8W	28480	0698-3150
A3R2	0698-0083	11	R:FXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A3R3	0698-3157	2	R:FXD MET FLM 19.6K OHM 1% 1/8W	28480	0698-3157
A3R4	0757-0442	6	R:FXD MET FLM 10.0K OHM 1% 1/8W	28480	0757-0442
A3R5	0757-0442		R:FXD MET FLM 10.0K OHM 1% 1/8W	28480	0757-0442
A3R6	0757-0442		R:FXD MET FLM 10.0K OHM 1% 1/8W	28480	0757-0442
A3R7	0698-3153	3	R:FXD MET FLM 3.83K OHM 1% 1/8W	28480	0698-3153
A3R8	0698-3159	1	R:FXD MET FLM 26.1K OHM 1% 1/8W	28480	0698-3159
A3R9	0698-0083		R:FXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083
A3R10	0757-0280	4	R:FXD MET FLM 1K OHM 1% 1/8W	28480	0757-0280
A3R11	0757-0280		R:FXD MET FLM 1K OHM 1% 1/8W	28480	0757-0280
A3R12	0757-0438	2	R:FXD MET FLM 5.11K OHM 1% 1/8W	28480	0757-0438
A3R13	0698-3153		R:FXD MET FLM 3.83K OHM 1% 1/8W	28480	0698-3153
A3R14	0757-0438		R:FXD MET FLM 5.11K OHM 1% 1/8W	28480	0757-0438
A3R15	0757-0401	2	R:FXD MET FLM 100 OHM 1% 1/8W	28480	0757-0401
A3R16	0698-0085	1	R:FXD MET FLM 2.61K OHM 1% 1/8W	28480	0698-0085
A3R17	0698-3151	5	R:FXD MET FLM 2.87K OHM 1% 1/8W	28480	0698-3151
A3R18	0698-3157		R:FXD MET FLM 19.6K OHM 1% 1/8W	28480	0698-3157
A3R19	0757-0401		R:FXD MET FLM 100 OHM 1% 1/8W	28480	0757-0401
A3R20	0757-0447	1	R:FXD MET FLM 16.2K OHM 1% 1/8W	28480	0757-0447
A3R21	0698-3153		R:FXD MET FLM 3.83K OHM 1% 1/8W	28480	0698-3153
A3U1	1820-0476	1	IC:OP. AMP. HI-SPEED	07268	49F7715303
A5	86601-60016	1	MODULATOR ASSY	28480	86601-60016
A5C1	0160-3036	1	C:FXD CER 5000 PF 400-20% 200VDCM	28480	0160-3036
A5J1	1250-0901		CONNECTOR:RF BULKHEAD	15558	1104/D
A5J2	1250-0901		CONNECTOR:RF BULKHEAD	15558	1104/D
A5J3	1250-0901		CONNECTOR:RF BULKHEAD	15558	1104/D
A5MP1	86601-20022	1	CONNECTOR:RF BULKHEAD	28480	86601-20022
A5A1	86601-60001	1	BOARD ASSY:MODULATOR	28480	86601-60001
A5A1G1	0160-3436	7	C:FXD CER 1000 PF 10% 200VDCM	56285	0047251F102K100-COM
A5A1G2	0160-2208	1	C:FXD MICA 500 PF 5% 300VDCM	28480	0160-2208

See Introduction to this section for ordering information

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number	
45A1C3	0160-2236	2	C:FXD CER 1.0 PF 500VDCM	72982	3C1-000-CCX0-109C	
45A1C4	0160-3456	5	C:FXD CER 1000 PF 10% 250VDCM	56285	C067F251F102K522-CDM	
45A1C5	0160-2327		C:FXD CER 1000 PF 20% 100VDCM	96733	81C48X102M	
45A1C6	0160-3456		C:FXD CER 1000 PF 10% 250VDCM	56285	C067F251F102K522-CDM	
45A1C7	0160-2236		C:FXD CER 1.0 PF 500VDCM	72982	3C1-000-CCX0-109C	
45A1C8	0160-3456		C:FXD CER 1000 PF 10% 250VDCM	56285	C067F251F102K522-CDM	
45A1C9	0160-2327	1	C:FXD CER 1000 PF 20% 100VDCM	96733	81C48X102M	
45A1C10	0160-2327		C:FXD CER 1000 PF 20% 100VDCM	96733	81C48X102M	
45A1C11	0160-2238		C:FXD CER 1.5 PF 500VDCM	72982	3C1-000-CCX0-159C	
45A1C12	0160-3456		C:FXD CER 1000 PF 10% 250VDCM	56285	C067F251F102K522-CDM	
45A1C13	0160-2327		C:FXD CER 1000 PF 20% 100VDCM	96733	81048X102M	
45A1C14	0160-3456		C:FXD CER 1000 PF 10% 250VDCM	56285	C067F251F102K522-CDM	
45A1C15	0160-2327	1	C:FXD CER 1.27-1-0.25 PF 500VDCM	72982	3C1-000-CCX0-129C	
45A1C16	0160-3456		C:FXD CER 1000 PF 10% 250VDCM	56285	C067F251F102K522-CDM	
45A1C17	0160-2327		C:FXD CER 1000 PF 20% 100VDCM	96733	81C48X102M	
45A1E1	0960-2070		1	MIXER:500 MHZ	28480	0960-2070
45A1L1	9100-2247		1	COIL:FXD RF 0.10 UH 10%	28480	9100-2247
45A1L2	9140-0158	1	COIL:FXD RF 1 UH 10%	59800	1025-20	
45A1Q1	1854-0345	4	TSTR:SI NPN	80131	2N5175	
45A1Q2	1854-0345		TSTR:SI NPN	80131	2N5175	
45A1Q3	1854-0345	4	TSTR:SI NPN	80131	2N5179	
45A1Q4	1854-0345		TSTR:SI NPN	80131	2N5175	
45A1R1	0757-0439		R:FXD MET FLM 6.81K OHM 1% 1/8W	28480	0757-0439	
45A1R2	0698-3151		R:FXD MET FLM 2.87K OHM 1% 1/8W	28480	0698-3151	
45A1R3	0698-7195		R:FXD MET FLM 19.6 OHM 2% 1/8W	28480	0698-7195	
45A1R4	0698-3440	4	R:FXD MET FLM 196 OHM 1% 1/8W	28480	0698-3440	
45A1R5	0757-0439		R:FXD MET FLM 6.81K OHM 1% 1/8W	28480	0757-0439	
45A1R6	0698-3151		R:FXD MET FLM 2.87K OHM 1% 1/8W	28480	0698-3151	
45A1R7	0698-3440		R:FXD MET FLM 196 OHM 1% 1/8W	28480	0698-3440	
45A1R8	0757-0439		R:FXD MET FLM 6.81K OHM 1% 1/8W	28480	0757-0439	
45A1R9	0698-3151	2	R:FXD MET FLM 2.87K OHM 1% 1/8W	28480	0698-3151	
45A1R10	0698-3440		R:FXD MET FLM 196 OHM 1% 1/8W	28480	0698-3440	
45A1R11	0757-0439		R:FXD MET FLM 6.81K OHM 1% 1/8W	28480	0757-0439	
45A1R12	0698-3151		R:FXD MET FLM 2.87K OHM 1% 1/8W	28480	0698-3151	
45A1R13	0698-3440		R:FXD MET FLM 196 OHM 1% 1/8W	28480	0698-3440	
45A1R14	0698-3438	2	R:FXD MET FLM 147 OHM 1% 1/8W	28480	0698-3438	
45A1R15	0698-3435		R:FXD MET FLM 38.3 OHM 1% 1/8W	28480	0698-3435	
45A1R16	0698-3438		R:FXD MET FLM 147 OHM 1% 1/8W	28480	0698-3438	
45A2	86601-60020	1	FILTER:LOW PASS 600 MHZ	28480	86601-60020	
A9	86601-60005	1	BOARD ASSY:REFERENCE	28480	86601-60005	
A9C1	0160-2226	1	C:FXD MICA 2200 PF 5% 300VDCM	28480	0160-2226	
A9C2	1702-0041		U100E:BREAKDOWN 5.11V 5%	04713	5Z10935-98	
A9K1	1901-0025		DICDE:SiLICON 100MA/1V	07263	FD 2387	
A9K2	0490-0916		RELAY:REED 1 FORM A 0.5 AMP	15636	RA30231051	
A9K3	0490-0916		RELAY:REED 1 FORM A 0.5 AMP	15636	RA30231051	
A9K4	0490-0916		RELAY:REED 1 FORM A 0.5 AMP	15636	RA30231051	
A9K5	0490-0916	RELAY:REED 1 FORM A 0.5 AMP	15636	RA30231051		
A9K6	0490-0916	RELAY:REED 1 FORM A 0.5 AMP	15636	RA30231051		
A9Q1	1854-0071	5	TSTR:SI NPN(SELECTED FROM 2N3704)	28480	1854-0071	
A9Q2	1853-0015		TSTR:SI PNP	80131	2N3640	
A9Q3	1853-0015		TSTR:SI PNP	80131	2N3640	
A9Q4	1853-0322		TSTR:SI PNP	80131	2N2946A	
A9Q5	1853-0015		TSTR:SI PNP	80131	2N3640	
A9Q6	1853-0322	1	TSTR:SI PNP	80131	2N2946A	
A9Q7	1853-0015		TSTR:SI PNP	80131	2N3640	
A9Q8	1853-0322		TSTR:SI PNP	80131	2N2946A	
A9Q9	1853-0015		TSTR:SI PNP	80131	2N3640	
A9Q10	1854-0071		TSTR:SI NPN(SELECTED FROM 2N3734)	28480	1854-0071	
A9Q11	1853-0322	2	TSTR:SI PNP	80131	2N2946A	
A9R1	2100-2637		R:VAR CERMET 1K OHM 10% LIM 1/2W	28480	2100-2633	
A9R2	0757-0410		R:FXD MET FLM 619 OHM 1% 1/8W	28480	0757-0410	
A9R3	2100-2633		R:VAR CERMET 1K OHM 10% LIM 1/2W	28480	2100-2633	
A9R4	0757-0442	1	R:FXD MET FLM 10.0K OHM 1% 1/8W	28480	0757-0442	
A9R5	0757-0442	2	R:FXD MET FLM 10.0K OHM 1% 1/8W	28480	0757-0442	
A9R6	0698-0083		R:FXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083	
A9R7	0698-0083		R:FXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083	
A9R8	0698-4406		R:FXD FLM 115 OHM 1% 1/8W	28480	0698-4406	
A9R9	0698-0083		R:FXD MET FLM 1.96K OHM 1% 1/8W	28480	0698-0083	

See introduction to this section for ordering information

Table 6-3. Replaceable Parts

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
A9R10	C658-4482	1	R:FXD FLM 17.4K OHM 1% 1/8W	2848C	0658-4482
A9R11	0658-4436		R:FXD FLP 115 OHM 1% 1/8W	2848C	0658-4436
A9R12	C698-0083		R:FXD MET FLM 1.96K OHM 1% 1/8W	2848C	0698-0083
A9R13	C698-3486	2	R:FXD FLM 232 OHM 1% 1/8W	2848C	0658-3486
A9R14	0757-C280		R:FXD MET FLM 1K OHM 1% 1/8W	2848C	0757-C280
A9R15	0698-6083		R:FXD MET FLM 1.96K OHM 1% 1/8W	2848C	0698-6083
A9R16	0698-3498	1	R:FXD MET FLM 8.66K OHM 1% 1/8W	2848C	0658-3498
A9R17	C698-3486		R:FXD FLP 232 OHM 1% 1/8W	2848C	0658-3486
A9R18	C698-C083		R:FXD MET FLP 1.96K OHM 1% 1/8W	2848C	0698-C083
A9R19	C698-3510	2	R:FXD MET FLP 453 OHM 1% 1/8W	2848C	0698-3510
A9R20	C698-C083		R:FXD MET FLM 1.96K OHM 1% 1/8W	2848C	0698-C083
A9R21	C698-3154	1	R:FXD MET FLM 4.22K OHM 1% 1/8W	2848C	0698-3154
A9R22	0698-3510		R:FXD MET FLM 453 OHM 1% 1/8W	2848C	0698-3510
A9R23	0698-C083		R:FXD MET FLM 1.96K OHM 1% 1/8W	2848C	0698-C083
A9R24	C698-3495	2	R:FXD MET FLM 866 OHM 1% 1/8W	2848C	0658-3495
A9R25	C698-C083		R:FXD MET FLM 1.96K OHM 1% 1/8W	2848C	0698-C083
A9R26	0698-4436	1	R:FXD FLM 1.91K OHM 1% 1/8W	2848C	0658-4436
A9R27	0698-3495		R:FXD MET FLM 866 OHM 1% 1/8W	2848C	0658-3495
A9R28	0757-C280		R:FXD MET FLM 1K OHM 1% 1/8W	2848C	0757-C280
A9R29	0757-0442		R:FXD MET FLM 10.0K OHM 1% 1/8W	2848C	0757-0442
A9R30	210C-2522	1	R:VAR CERMET 10K OHM 10% LIN 1/2W	2848C	210C-2522
A9R31	C698-3453	1	R:FXD MET FLM 196K OHM 1% 1/8W	2848C	0698-3453
A9R32	0698-3446	1	R:FXD MET FLM 383 OHM 1% 1/8W	2848C	0698-3446
A9U1	182C-0201	1	INTEGRATED CIRCUIT:OPERATIONAL AMPL	04713	MC1435G

Table 6-4. Manufacturer's Code List

MFR NO.	MANUFACTURER NAME	ADDRESS	ZIP CODE
01121	ALLEN BRADLEY CO.	MILWAUKEE, WIS.	53204
01295	TEXAS INSTRUMENTS INC. SEMICONDUCTOR COMPONENTS DIV.	DALLAS, TEX.	75231
02114	FERROXCUBE CORP.	SAUGERTIES, N.Y.	12477
02600	AMPHENOL CORP.	BROADVIEW, ILL.	60153
02875	MUDSIH TOOL & DIE CO.	NEWARK, N.J.	07105
04713	MOTOROLA SEMICONDUCTOR PROD. INC.	PHOENIX, ARIZ.	85008
07263	FAIRCHILD CAMERA & INST. CORP. SEMICONDUCTOR DIV.	MOUNTAIN VIEW, CALIF.	94040
15558	MICON ELECTRONICS INC.	GARDEN CITY LONG IS., N.Y.	11530
15636	ELEC-TROL INC.	NORTHRIDGE, CALIF.	91325
18324	SIGNETICS CORP.	SUNNYVALE, CALIF.	94086
2848C	HEWLETT-PACKARD CO. CORPORATE HQ	YOUR NEAREST HP OFFICE	
56289	SPRAGUE ELECTRIC CO.	N. ADAMS, MASS.	01247
71785	CINCH MFG. CO. DIV TRW INC.	ELK GROVE VILLAGE, ILL.	
72136	ELECTRO MOTIVE MFG. CO. INC.	WILLIMANTIC, CONN.	06226
72928	GUDEMANN DIV. GULTON IND. INC.	CHICAGO, ILL.	60610
72982	ERIE TECHNOLOGICAL PROD. INC.	ERIE, PA.	16512
74868	AMPHENOL CORP. RF DIV.	DANBURY, CONN.	06810
76530	CINCH MONADNOCK HILLS DIV. TRW INC.	CITY OF INDUSTRY, CALIF.	91746
76854	OAK MFG. CO. DIV. OAK ELECTRO/NETICS CORP.	CRYSTAL LAKE, ILL.	60014
80031	MERCO DIV. SESSIONS CLUCK CO.	MORRISTOWN, N.J.	07960
80131	ELECTRONIC INDUSTRIES ASSOCIATION	WASHINGTON D.C.	20506
81312	WINCHESTER ELECTRONICS DIV. LITTON IND. INC.	PAKVILLE, CONN.	06779
82142	AIRCO SPEER ELECT. COMP.	DU BOIS, PA.	15801
96733	SAN FERNANDO ELECT. MFG. CO.	SAN FERNANDO, CALIF.	91341
98291	SELECTAD CORP.	NAMARONEL, N.Y.	10544
99830	DELEVAN ELECTRONICS CORP.	E. AURORA, N.Y.	14052

See introduction to this section for ordering information

TABLE 6-5
PART NUMBER-NATIONAL STOCK NUMBER
CROSS REFERENCE INDEX

PART NUMBER	FSCM	NATIONAL STOCK NUMBER	PART NUMBER	FSCM	NATIONAL STOCK NUMBER
8E042X102M	96733	5910-00-244-7171	0180-0116	28480	5910-00-809-4701
CV2059X7R102M	80031	5910-01-022-6482	0180-0197	28480	5910-00-850-5355
HC1439G	04713	5962-00-252-0225	0180-0228	28480	5910-00-719-9907
HC4001P	04713	5962-00-455-1814	0180-1735	28480	5910-00-430-6016
RA30231051	15636	5945-00-233-1542	0683-0565	28480	5905-00-931-1066
RDM15E430J3C	72136	5910-00-195-4107	0698-0082	28480	5905-00-974-6075
RDM15F101J3C	72136	5910-00-463-5949	0698-0083	28480	5905-00-407-0052
R2846-1	15636	5945-00-448-6876	0698-0085	28480	5905-00-998-1814
SN7400N	01295	5962-00-865-4625	0698-3132	28480	5905-00-828-0388
SN7474N	01295	5962-00-106-4287	0698-3150	28480	5905-00-481-1357
SZ10939-134	04713	5961-00-912-3099	0698-3151	28480	5905-00-246-8634
SZ10939-38	04713	5961-00-350-2205	0698-3153	28480	5905-00-974-6081
0160-0198	28480	5910-00-914-2605	0698-3154	28480	5905-00-891-4215
0160-0157	28480	5910-00-961-9591	0698-3157	28480	5905-00-433-6904
0160-0158	28480	5910-00-497-7598	0698-3158	28480	5905-00-858-8927
0160-2055	28480	5910-00-211-1611	0698-3159	28480	5905-00-407-0053
0160-2199	28480	5910-00-244-7164	0698-3161	28480	5905-00-974-6082
0160-2200	28480	5910-00-195-4107	0698-3429	28480	5905-00-407-0075
0160-2204	28480	5910-00-463-5949	0698-3430	28480	5905-00-420-7136
0160-2208	28480	5910-00-430-5685	0698-3438	28480	5905-0-974-6080
0160-2226	28480	5910-00-885-6540	0698-3440	28480	5905-00-828-0377
0160-2236	28480	5910-00-444-6724	0698-3443	28480	5905-00-194-0341
0160-2265	28480	5910-00-444-6725	0698-3446	28480	5905-00-974-6083
0160-2306	28480	5910-00-883-6281	0698-3453	28480	5905-00-078-1548
0160-2327	28480	5910-00-244-7171	0698-3498	28480	5905-00-478-2244
0160-2437	28480	5910-00-431-3956	0698-3510	28480	5905-00-407-0107
0160-3036	28480	5940-00-138-1326	0698-7195	28480	5905-00-161-8921
0160-3447	28480	5910-00-913-0802	0698-7229	28480	5905-01-009-7560
0160-3456	28480	5910-01-014-2874	0757-0159	28480	5905-00-830-6677
0160-3876	28480	5910-00-348-2617	0757-0180	28480	5905-00-972-4907
0170-0040	28480	5910-00-829-0245	0757-0274	28480	5905-00-858-9105
0180-0058	28480	5910-00-027-7069	0757-0280	28480	5905-00-853-8190

TABLE 6-5
PART NUMBER-NATIONAL STOCK NUMBER
CROSS REFERENCE INDEX

PART NUMBER	FSCM	NATIONAL STOCK NUMBER	PART NUMBER	FSCM	NATIONAL STOCK NUMBER
0757-0290	28480	5905-00-858-8826	131-149	02660	5999-00-479-8176
0757-0294	28480	5905-00-974-5709	1820-0054	28480	5962-00-138-5248
0757-0316	28480	5905-00-981-7475	1820-0077	28480	5962-00-138-5250
0757-0317	28480	5905-00-244-7189	1820-0201	28480	5962-00-252-0225
0757-0346	28480	5905-00-998-1906	1853-0015	28480	5961-00-927-0845
0757-0394	28480	5905-00-412-4036	1853-0020	28480	5961-00-904-2540
0757-0399	28480	5905-00-929-7774	1853-0213	28480	5961-00-937-1409
0757-0401	28480	5905-00-981-7529	1854-0071	28480	5961-00-137-4608
0757-0402	28480	5905-00-405-8091	1854-0247	28480	5961-00-464-4049
0757-0405	28480	5905-00-493-0738	1854-0345	28480	5961-00-401-0507
0757-0417	28480	5905-00-858-9417	1854-0361	28480	5961-00-400-5973
0757-0418	28480	5905-00-412-4037	1854-0404	28480	5961-00-408-9807
0757-0421	28480	5905-00-891-4219	1855-0020	28480	5961-00-105-8867
0757-0438	28480	5905-00-929-2529	1901-0025	28480	5961-00-978-7468
0757-0439	28480	5905-00-990-0303	1901-0535	28480	5961-00-451-8685
0757-0442	28480	5905-00-998-1792	1902-0041	28480	5961-00-858-7372
0757-0447	28480	5905-00-981-7530	1902-0048	28480	5961-00-912-3099
0757-0458	28480	5905-00-494-4628	1902-3036	28480	5961-00-350-2205
0757-0461	28480	5905-00-089-7577	1910-0016	28480	5961-00-954-9182
0757-0465	28480	5905-00-904-4412	2N3640	80131	5961-00-927-0845
0757-1000	28480	5905-00-057-8480	2N4236	80131	5961-00-937-1409
0757-1094	28480	5905-00-917-0580	2N4239	80131	5961-00-400-5973
08555-20093	28480	5999-00-08-8444	2N5179	80131	5961-00-401-0507
08660-80005	28480	5950-00-443-9518	2100-1754	28480	5905-00-407-0077
1025-20	29800	5950-00-059-5920	2100-1755	28480	5905-00-407-0078
1200-0063	28480	5990-00-937-4420	2100-1759	28480	5905-00-221-7472
1205-0011	28480	5990-00-789-3794	2100-2413	28480	5905-00-138-5086
1250-0901	28480	5935-00-477-1147	2100-2522	28480	5905-00-476-5797
1250-0914	28480	5935-00-434-3040	2100-2632	28480	5905-00-476-5718
1251-2034	28480	5935-00-267-2973	2100-2633	28480	5905-00-476-5796
1251-2262	28480	5935-00-026-0952	2100-3113	28480	5905-00-470-3420
1251-3087	28480	5999-01-079-9981	251-06-30-400	71785	5905-00-405-7709

TABLE 6-5
PART NUMBER-NATIONAL STOCK NUMBER
CROSS REFERENCE INDEX

PART NUMBER	FSCM	NATIONAL STOCK NUMBER	PART NUMBER	FSCM	NATIONAL STOCK NUMBER
252-10-30-300	71785	5935-00-267-2973			
252-12-30-300	71785	5935-00-448-2236			
252-15-30-008	71785	5935-00-138-5209			
5020-0176	28480	5970-00-531-7134			
5040-0306	28480	5970-00-470-7622			
9100-1627	28480	5950-00-475-4996			
9100-2247	28480	5950-00-405-3735			
9140-0158	28480	5950-00-059-5920			
9140-0237	28480	5950-00-431-3216			
9170-0029	28480	5950-00-406-6419			

SECTION VII
MANUAL CHANGES

7-1. INTRODUCTION

changes listed opposite your instrument serial number. Perform these changes in the sequence listed.

7-2. This section contains information for adapting this manual to instruments for which the content does not apply directly.

7-4. Refer to paragraph 7-8 for manual changes pertaining to later aerial numbered instruments.

7-3. To adapt this manual to your instrument, refer to Table 7-1 and make all of the manual

Table 7-1. Manual changes by Serial Number

Serial Prefix or Number	Make Manual Changes
1317A	A
1307A	A, B
1250A	A - C
1249A	A - D
1223A	A - E
1214A	A - F
1201A	A - G
1150A	A - H
1110A	A - I

7-5. MANUAL CHANGE INSTRUCTIONS

7-6. **Unless otherwise noted, make manual changes in the alphabetical order in which they appear until the serial prefix of your instrument is reached.**

7-7. Table 7-3 provides a cross reference of assemblies to changes.

CHANGE A

Page 8-19, Figure 8-26 (A10 assembly)

Change part number to 86601-60008 and exchange part number to 86601-60104 Refer to Figure 7-2 for a partial schematic. Component part numbers and reference designators do not change

CHANGE B

Page 8-17, Figure 8-24 and Table 6-3 (A9 assembly)

Delete A9R37. Replace with printed circuit trace.

CHANGE C

Table 6-3

Change A3J1 and A3J2 to: 1250-0901 CONNECTOR RF BULKHEAD 15558 1104 D

CHANGE C (Cont'd)

Table 6-3 (Cont'd)

Change A5J1 and A5J2 to: 1250-0901 CONNECTOR: RF BULKHEAD 15558 1104/D

Delete: 86601-00051, BRACKET: MIXER 28480 86601-00051.

86601-20080, GUIDE: PLUG-IN 28480 86601-20080.

86601-00052, COVER: HALF 28480 86601-00052.

Add: 86601-00096, BRACKET: MIXER 28480 86601-00096

86601-00029, COVER, OUTER 28480 86601-00029.

CHANGE D

Table 6-3

Change A1M1 part number to 1120-1561 (Option 001 1120-1563)

Page 8-17, Figure 8-24 and Table 6-3 (A3 assembly)

Change A3R4 to 0757-0442 R:FXD MET F:M 10.0 K OHM 1% 1/8 W.

Page 8-17, Figure 8-24 and Table 6-3 (A9 assembly)

Change A9R32 to 2100-2522 R:VARCERMET 10K OHM 10% LIN 1/2W.

CHANGE E

Page 8-13, Figure 8-17 (A5 assembly)

Move inductive bead A5A1Z1 from the Base of A5A1Q1 to the Base of A5A1Q2.

CHANGE F

Page 8-13, Figure 8-17, Table 6-1 and Table 6-3 (A5 assembly)

Change part number to 86601-60064 and exchange part number to 36601-60114.

Delete: A5J4, A5C3, A5A1C10, ASA1R10, A5A1K1.

Relabel the input to A5J1 CNTRL, change the wire color code to 80 and make the input symbol 4A.

Connect the lead from A5J1 to A1A5R9.

NOTE

If your instrument has serial prefix 110A or 1150A do not make these changes in your manual.

CHANGE G

Table 6-3

Change A1M1 part number to 1120-1545 (Option 001 1120-1553).

Change 86601-00034 to 86601-00001.

86601-00036 to 86601-00002.

86601-00035 to 86601-00028.

86601-20069 to 86601-20016.

86601-20070 to 36601-20051.

36601-40018 to 86601-40017.

CHANGE H

Page 8-13, Figure 8-17 and Table 6-1 (A5 assembly)

Change part number to 36601-60016 and exchange part number to 86601-60105.

Refer to Figure 7-3 for schematic, Figure 7-4 for component locations and Table 7-2 for replaceable parts.

CHANGE H (Cont'd)

Page 8-17, Figure 8-24 and Table 6-1 (A9 assembly)

Change part number to 86601-60005 and exchange part number to 86601-60102.
 Refer to Figure 7-5 for schematic, Figure 7-6 for component locations and Table 7-2 for replaceable Parts.

Page 8-17, Figure 8-24 and Table 6-1 (A3 assembly)

Change part number to 86601-60019 and exchange part number to 86601-60108.
 Refer to Figure 7-7 for schematic, Figure 7-8 for component locations and Table 702 for replaceable parts.

Page 8-13, Figure 8-17 and Table 6-1

Delete the A20 assembly 86601-60066.

CHANGE I

Page 8-13, Figure 8-17 and Table 6-3 (A4 assembly)

Change A4A1 and A4A2 components as follows:
 C1 and C4 to 24 pF 0160-2266 R2 and R6 to 3830 ohms 0698-3153
 C2 to .001 uF 0160-3456 R4 and R7 to 215 ohms 0698-3441
 C5 and C7 to 1000 pF 0160-2327 Q1 and Q2 to 1854-0431
 Delete the inductive bead, Z1, part number 9170-0029 from the base lead of A4A2Q2.

Page 5-2, Paragraph 5-14

Substitute the following procedure.

RF OUTPUT METER CALIBRATION

REFERENCE: Service Sheets 3 and 4.

DESCRIPTION: The rf output meter reading is adjusted at +3 and -7 dBm to ensure tracking across the range of the **VERNIER** control.

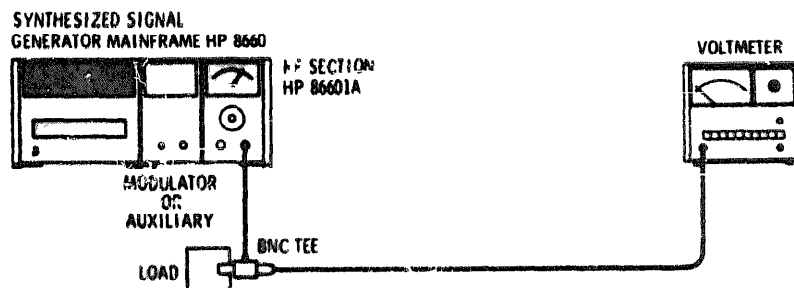


Figure 7-1. RF Output meter Calibration Setup

RECOMMENDED TEST EQUIPMENT:

Broadband Sampling Voltmeter	HP 3406A
BNC Tee Connector	UG274B/L/
50 Ohm Load	HP 1250-0, (C)
Extender Cable	HP 11672-6-001

CHANGE I (Cont'd)

RF OUTPUT METER CALIBRATION (cont'd)

PROCEDURE:

1. **Clean the Model 86601A meter face with** anti-static solution.
(Recommended: "STATNUL" manufactured by Weston Instruments Inc., Newark, NJ.)
2. **Connect the** BNC Tee connector to the 86601A OUTPUT, the 50 ohm load and the Broadband **Sampling Voltmeter** as shown in Figure 5-1.
3. Set the OUTPUT RANGE switch to +10 dBm and the VERNIER full clockwise.
4. Set the mainframe center frequency to 50 MHz.
5. **Set the REF ADJ control (A9R2)** for a +13.5 dBm reading on the Broadband Sampling Voltmeter
6. Adjust the VERNIER control counterclockwise to obtain a reading of +3 dBm on the Broadband Sampling Voltmeter.
7. Set the MTR ADJ Control (A9R32) for a reading on the Model 86601A output meter of +13 dBm
8. Adjust the VERNIER control counterclockwise for a reading on the Model 86601A output meter -7 dBm.
9. Set the DET control (A2R34) for a +3 dBm reading on the Broadband Sampling Voltmeter.
10. Repeat steps 5 through 9 until no further adjustment is necessary.

Table 7-2. Assembly-Change Cross Reference Index

Assembly	Change								
	A	B	C	D	E	F	G	H	I
A1				X			X		
A3			X	X				X	
A4									X
A5			X		X	F		X	
A9	X	X		X				X	
A10								X	

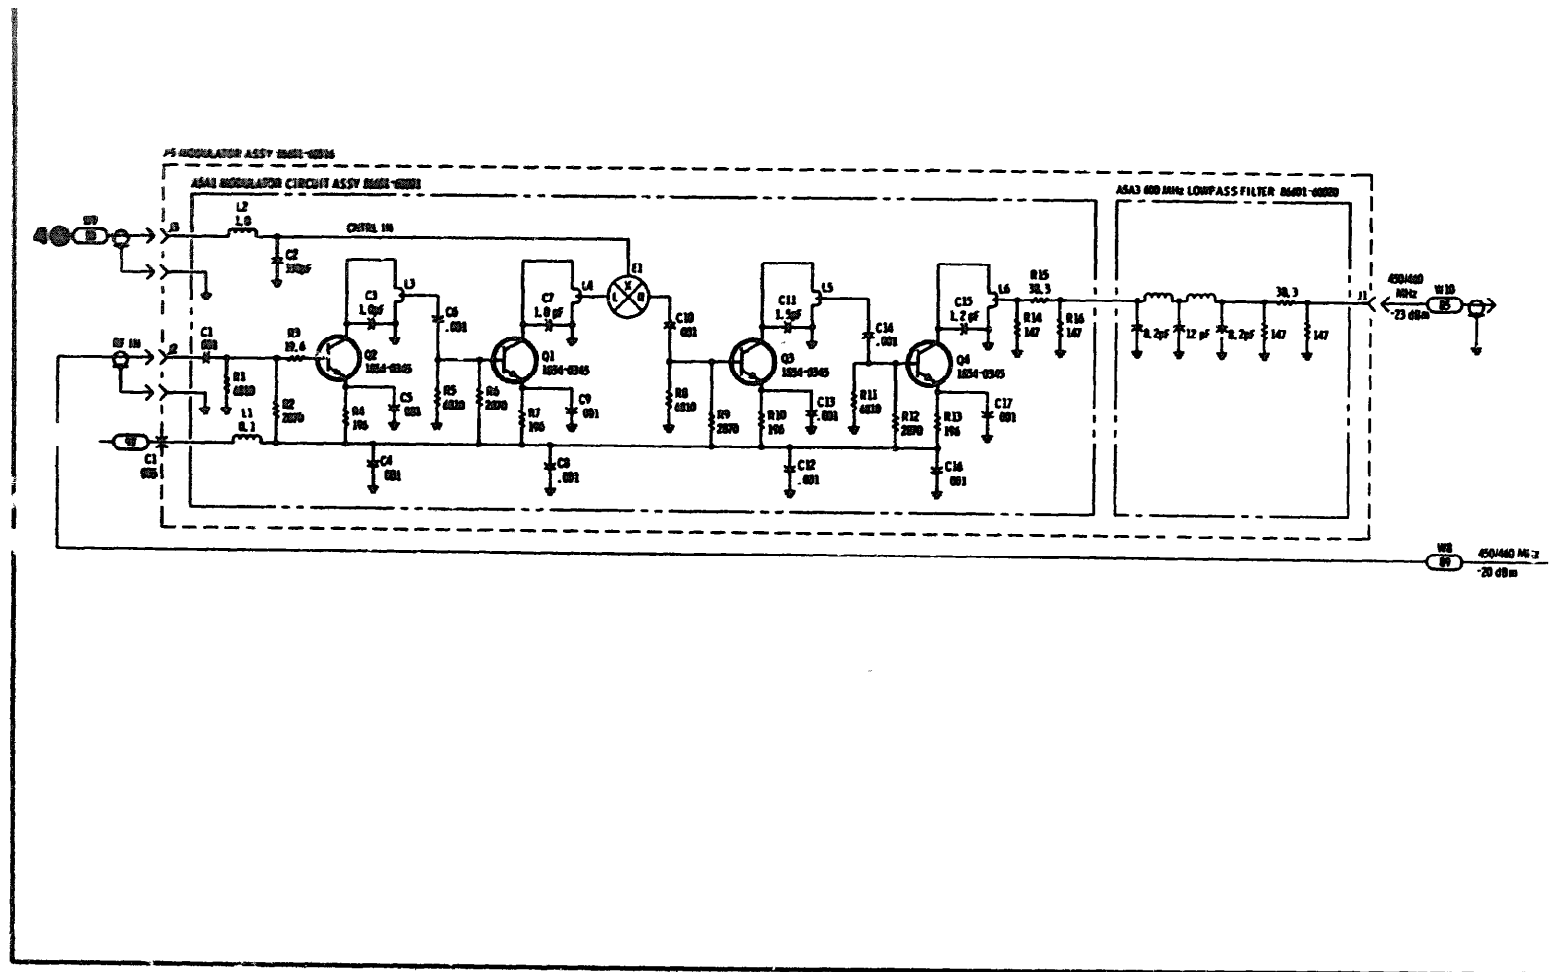


Figure 7-3. A5 Modulator Assembly 86601-60001

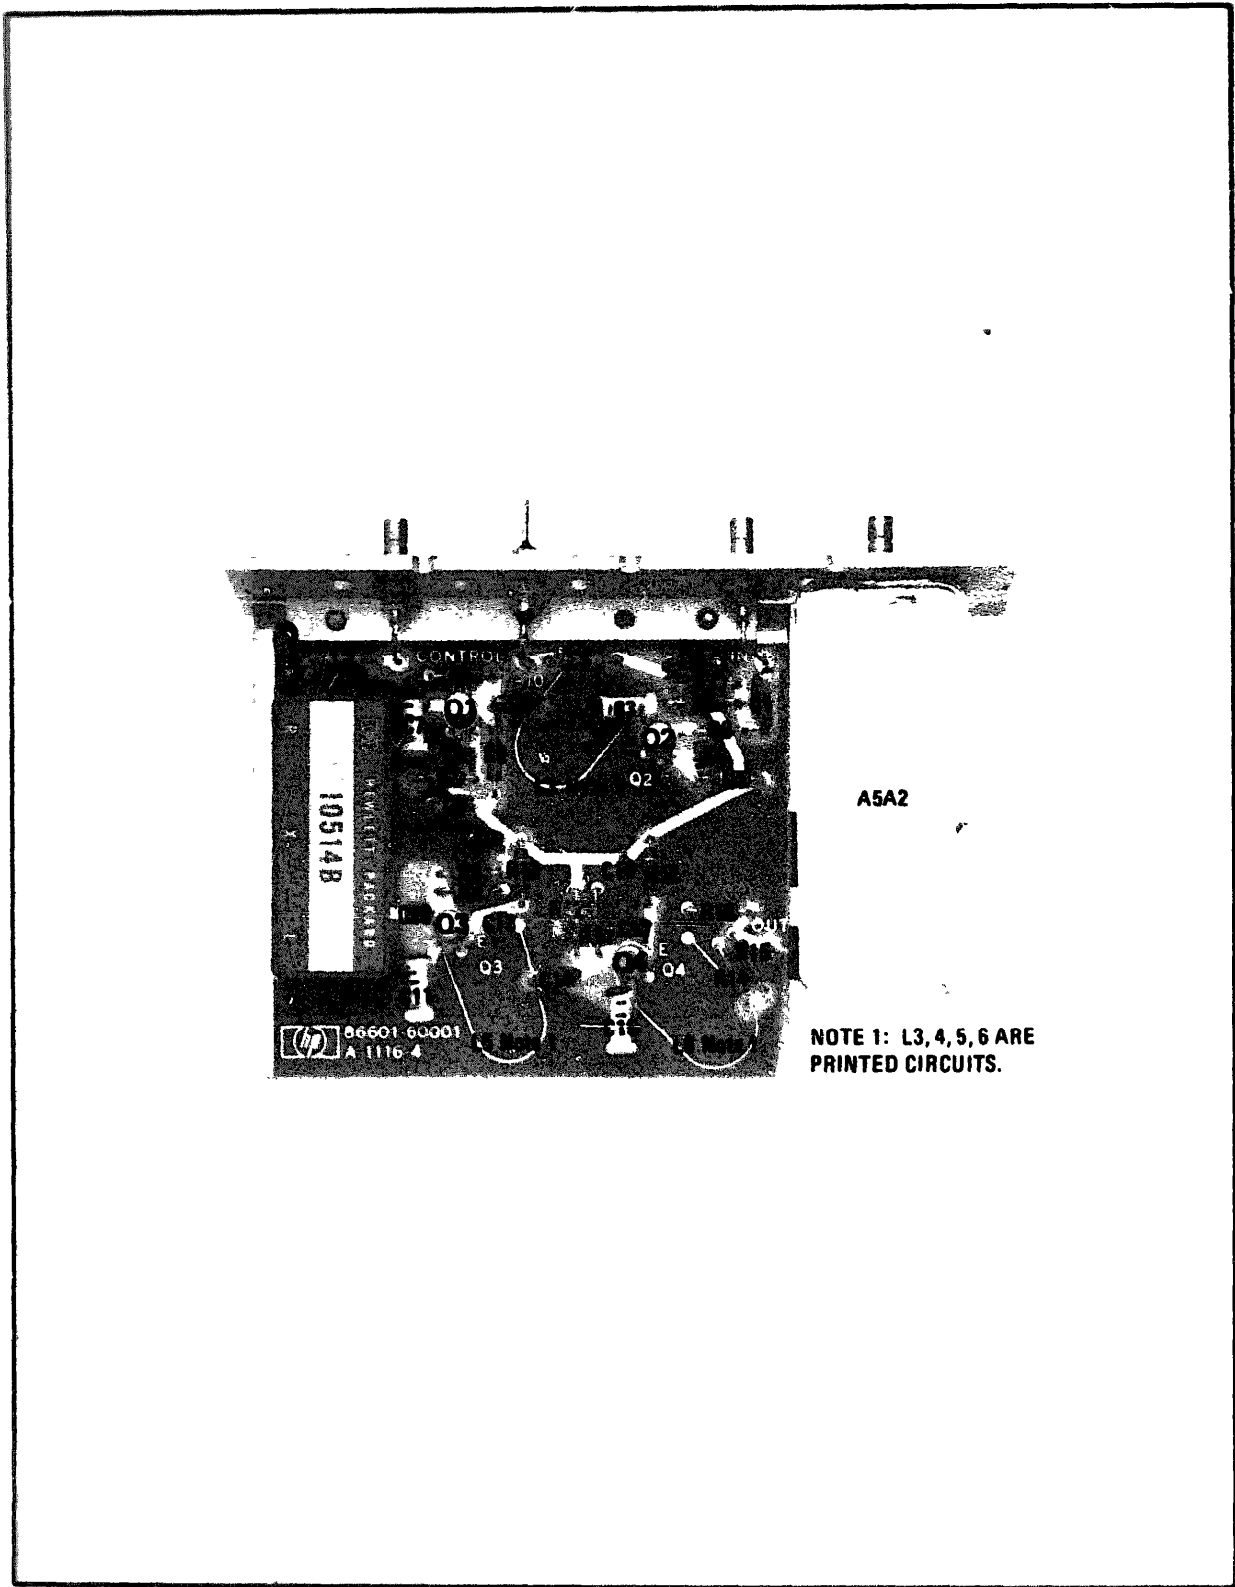


Figure 7-4. Modulator Assembly Component Locations

Model 86601A

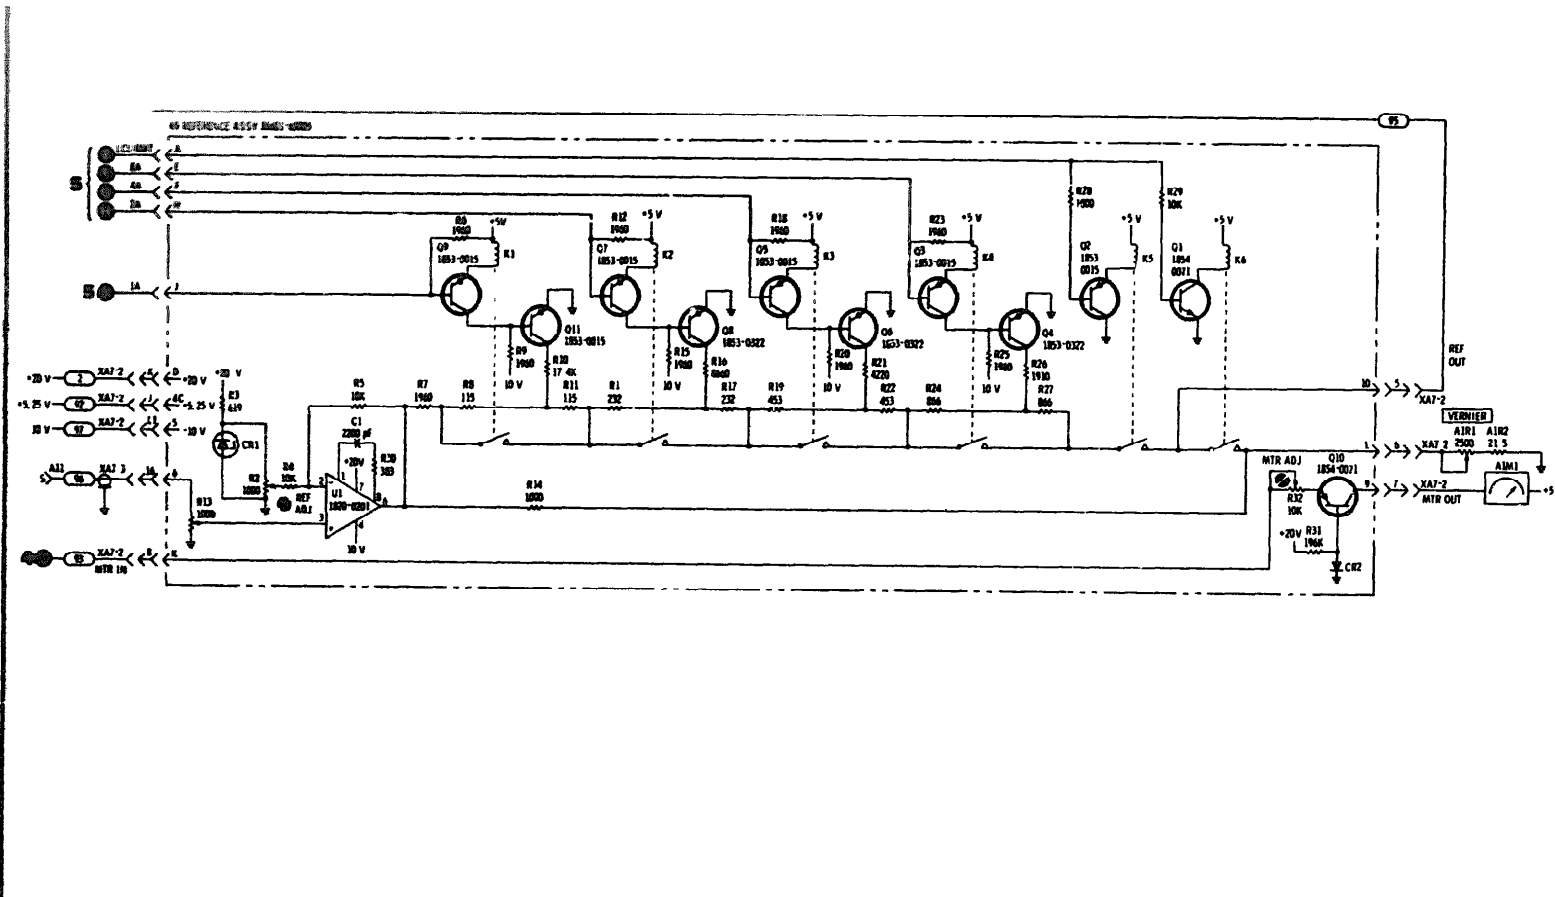


Figure 7-5. Reference Assembly

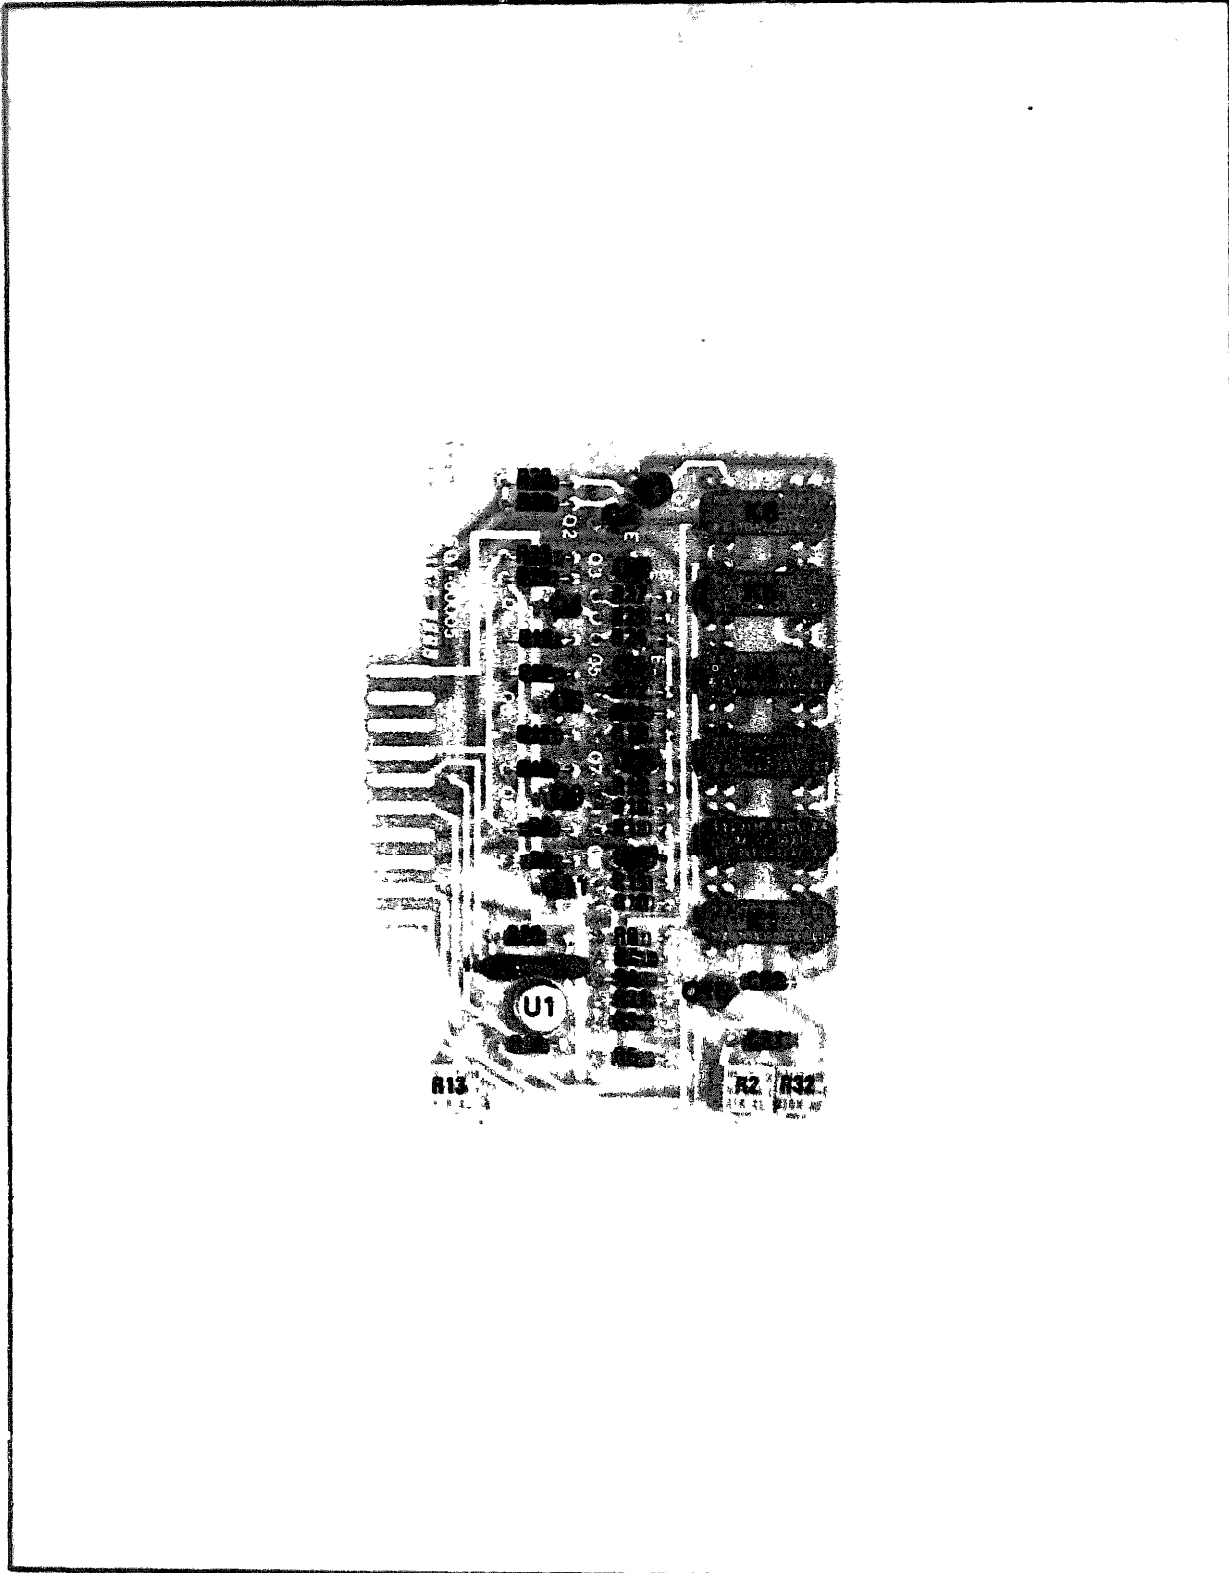


Figure 7-6. Reference Assembly Component Location

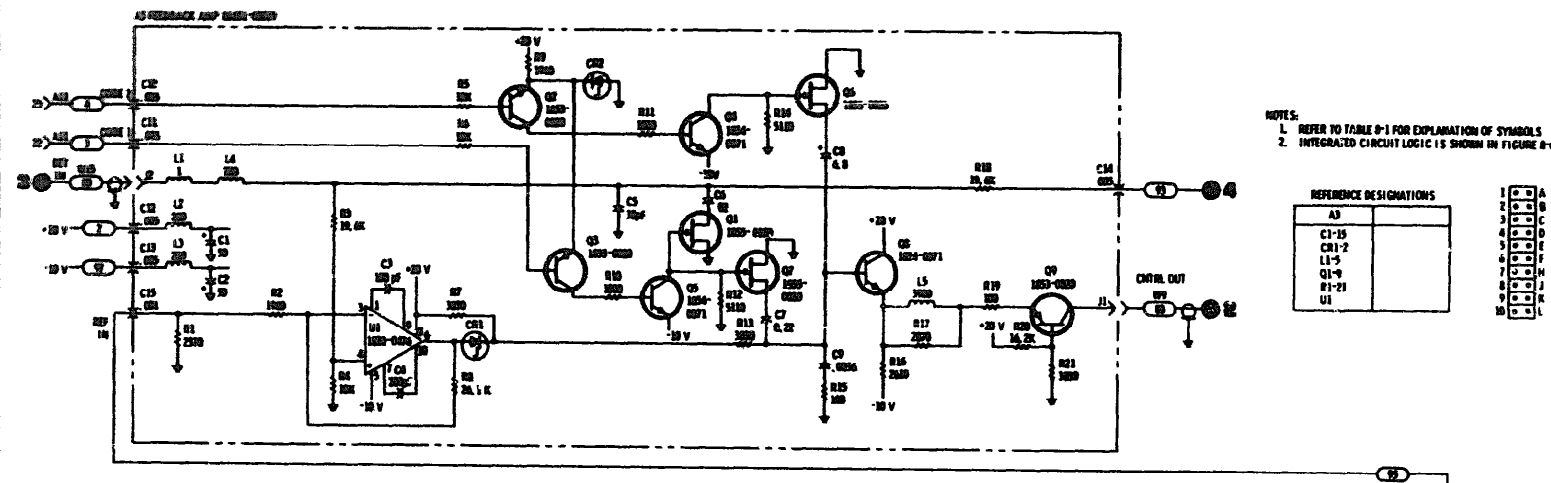


Figure 7-7. Feedback Amplifier

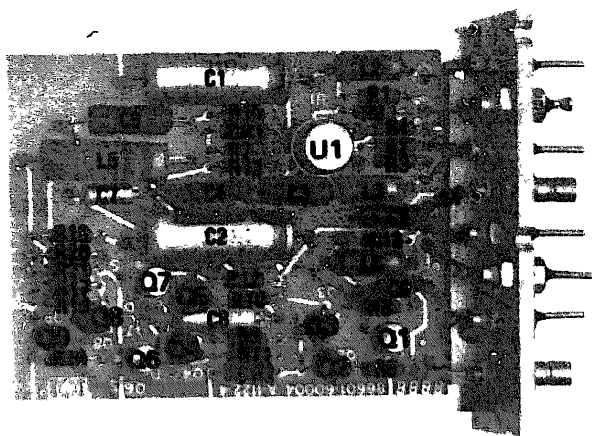


Figure 7-8. Feedback Amplifier Component Locations

Manual Changes

7-8. The manual changes given **below are for correcting errors and for adapting** the manual to instruments containing **improvements made after the printing of the** manual. Make all ERRATA corrections first and **then make all appropriate serial** number related changes indicated in the table.

Serial Prefix or Number	Make Manual Changes	Serial Prefix or Number	Make Manual Changes
1443A	1	▶ 1623A	1 through 5
1508A	1, 2		
1520A	1, 2, 3		
1524A	1 through 4		
1551A	1 through 5		
1616A	1 through 6		

▶ **NEW ITEM**

ERRATA

Page 1-2, Table 1-1:

- Change the heading "Spurious **Signals**" to "**Spurious Signals (CW and AM only)**".
- Change the heading "Signal-to-Phase Noise Ratio" to "**Signal-to-Phase Noise Ratio (CW and AM only)**".
- Change the heading "Residual **FM**" to "**Residual FM (CW and AM only)**".

Page 4-6, paragraph 4-15:

Change the first sentence of the SPECIFICATION to "**All non-harmonically related spurious signals (in the CW and AM modes) are at least 80 dB below the selected output signal.**"

Page, paragraph 4-16:

Add the following to the SPECIFICATION sentence "**in the CW and AM modes only**".

Page 4-10, paragraph 4-18:

Add the following to the SPECIFICATION sentence "in the CW and AM modes only"

Page 4-13, Figure 4-11:

Change the Variable-Phase Generator's output to the sine-wave output connector (one connector to the left of the output shown).

Page 6-3, Table 6-3:

Change A1M1 HP Part Numbers to 1120-0540 (EXCEPT OPTION 001) and 1120-0542 (OPTION 001 ONLY)

Page 6-5 and 6-6, Table 6-3:

Change the A4 and A5 parts list as shown in the table in this supplement.

Page 6-8, Table 6-3:

Add A20, 86601-60066, 600 MHz Low Pass Filter Assembly

CHANGE 1

Page 6-8:

Replace the parts list for the A8 assembly with the new portion of Table 6-3 found in this supplement.

Page 8-21:

**Replace Figure 8-27 with the new component location diagram found in this supplement.
Replace Figure 8-28 with the new schematic found in this supplement.**

CHANGE 2

Change A1M1 HP Part Number 1120-0540 (EXCEPT OPTION 001) to 1120-0543 (EXCEPT OPTION 001).

CHANGE 3

Page 6-5, Table 6-3:

Change A4A1C1, A4A1C4, A4A2C1, and A4A2C4 to 0160-3875, CAPACITOR FXD 22 pF $\pm 5\%$ 200 SVDC CER, 28480, 0160-3875.

Add to A4A1 miscellaneous, 1200-0172, 2, INSULATOR XSTR TO-18, 28480, 1200-0172.

Add to A4A2 miscellaneous, 1200-0172, 2, INSULATOR XSTR TO-18, 28480, 1200-0172.

Page 6-6, Table 6-3:

Change A5A1C1, A5A1C4, A5A2C1, and A5A2C5 to 0160-3875, CAPACITOR FXD 22 pF $\pm 5\%$ 200 WVDC CER, 28480, 0160-3875.

Delete A5A1Z1

Add to A5A1 miscellaneous, 1200-0172, 2, INSULATOR XSTR TO-18, 28480, 1200-0172.

Add to A5A2 miscellaneous, 1200-0172, 2, INSULATOR XSTR TO-18, 28480, 1200-0172.

Page 6-8, Table 6-3:

Change A8R5, R6, R16, R16, R25 and R26 to 0683-0335, RESISTOR 3.3 5% .25W FC TC--400/+500, 01121, CB33G5.

Page 8-13, Figure 8-13 (Service Sheet 2):

Change the value of the following capacitors to 22 pF: A4A1C1, A4A1C4, A4A2C1, A4A2C4, A5A1C1, A5A1C4, A5A2C1, and A5A2C5.

Page 8-21, Figure 8-28:

Change the value of A8R5, R6, R15, R16, R25, and R26 to 3.3 ohms.

NOTE

Refer to Change 1 of this supplement.

CHANGE 4

Page 6-1, Table 6-1:

Change the A13 Programmable Attenuator to A13 Attenuator.

Change the New Part No. of the A13 Attenuator to 86603-60043.

Page 6-9, Table 6-3 and page 8-21, Figure 8-28:

Change the HP Part Number of A13 to 86603-60043. The Exchange Part No. is unchanged.

Table 6-3. Replaceable Parts (P/O Errata; Page 1 of 2)

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
A4	86601-60023	1	FILTER ASSEMBLY, ACTIVE	28480	86601-60023
	86601-00009	1	COVER, ACTIVE FILTER ASSY	28480	86601-00009
	86601-20026	1	STRIPLINE	28480	86601-20026
	86601-20035	1	HOUSING, ACTIVE FILTER ASSY	28480	86601-20035
	86601-20037	1	INSERT, ACTIVE FILTER ASSY	28480	86601-20037
	86601-40007	2	BOTTOM, ACTIVE FILTER DIE.	28480	86601-40007
A4C1	0121-0465	4	C:VAR AIR 10 PF	28480	0121-0465
A4C2	0121-0465		C:VAR AIR 10 PF	28480	0121-0465
A4C3	0121-0465		C:VAR AIR 10 PF	28480	0121-0465
A4C4	0121-0465		C:VAR AIR 10 PF	28480	0121-0465
A4C5	0160-3036		CAPACITOR-FXD 5000PF +80-20E 200MVDC CER	28480	0160-3036
A4C6	0160-3036	5	CAPACITOR-FXD 5000PF +80-20E 200MVDC CER	28480	0160-3036
A4J1	1250-0901	2	CONNECTOR-RF SMB M SGL MOLE FR	2K497	700166
A4J2	1250-0901		CONNECTOR-RF SMB M SGL MOLE FR	2K497	700166
A4A1	86601-60011	1	BOARD ASSEMBLY, INPUT AMPLIFIER	28480	86601-60011
A4A1C1	0160-3878	20	CAPACITOR-FXD 1000PF +-20E 100MVDC CER	28480	0160-3878
A4A1C2	0160-3878		CAPACITOR-FXD 1000PF +-20E 100MVDC CER	28480	0160-3878
A4A1C3	0121-0447		CAPACITOR: VAR; TRMR; CER; 1.5/2.5PF	00865	75-TRIKO-03 1.5-2.5
A4A1C4	0160-3878		CAPACITOR-FXD 1000PF +-20E 100MVDC CER	28480	0160-3878
A4A1C5	0160-3878		CAPACITOR-FXD 1000PF +-20E 100MVDC CER	28480	0160-3878
A4A1C6	0121-0447	4	CAPACITOR: VAR; TRMR; CER; 1.5/2.5PF	00865	75-TRIKO-03 1.5-2.5
A4A1C7	0160-3878		CAPACITOR-FXD 1000PF +-20E 100MVDC CER	28480	0160-3878
A4A1L1	9100-2247	4	COIL-FXD WOLDED RF CHCKE 100MH 10E	24226	10/100
A4A1L2	08660-80005		INDUCTOR	28480	08660-80005
A4A1L3	08660-80005		INDUCTOR	28480	08660-80005
A4A1Q1	1854-0345	2	TRANSISTOR NPN 2N5179 SI TO-18 PD=200MW	04713	2N5179
A4A1Q2	1854-0345		TRANSISTOR NPN 2N5179 SI TO-18 PD=200MW	04713	2N5179
A4A1R1	0498-3429	3	RESISTOR 19.6 1% .125W F TC=0+-100	03088	PM55-1/8-TO-196-F
A4A1R2	0498-3151		RESISTOR 2.87K 1% .125W F TC=0+-100	16299	C4-1/8-TO-2871-F
A4A1R3	0737-0439		RESISTOR 6.81K 1% .125W F TC=0+-100	24546	C4-1/8-TO-6811-F
A4A1R4	0498-3440		RESISTOR 194 1% .125W F TC=0+-100	16299	C4-1/8-TO-194-F
A4A1R5	0737-0439		RESISTOR 6.81K 1% .125W F TC=0+-100	24546	C4-1/8-TO-6811-F
A4A1R6	0498-3151		RESISTOR 2.87K 1% .125W F TC=0+-100	16299	C4-1/8-TO-2871-F
A4A1R7	0498-3440	2	RESISTOR 194 1% .125W F TC=0+-100	16299	C4-1/8-TO-194-F
A4A1R8	0498-3443		RESISTOR 287 1% .125W F TC=0+-100	16299	C4-1/8-TO-287-F
A4A1R9	0737-0294	1	RESISTOR 17.0 1% .125W F TC=0+-100	19701	MFAC1/8-TO-170-F
A4A1R10	0498-3443	1	RESISTOR 287 1% .125W F TC=0+-100	16299	C4-1/8-TO-287-F
A4A2	86601-60012	1	BOARD ASSEMBLY, OUTPUT AMPLIFIER	28480	86601-60012
A4A2C1	0160-3878	20	CAPACITOR-FXD 1000PF +-20E 100MVDC CER	28480	0160-3878
A4A2C2	0160-3878		CAPACITOR-FXD 1000PF +-20E 100MVDC CER	28480	0160-3878
A4A2C3	0121-0447		CAPACITOR: VAR; TRMR; CER; 1.5/2.5PF	00865	75-TRIKO-03 1.5-2.5
A4A2C4	0160-3878		CAPACITOR-FXD 1000PF +-20E 100MVDC CER	28480	0160-3878
A4A2C5	0160-3878		CAPACITOR-FXD 1000PF +-20E 100MVDC CER	28480	0160-3878
A4A2C6	0121-0447	4	CAPACITOR: VAR; TRMR; CER; 1.5/2.5PF	00865	75-TRIKO-03 1.5-2.5
A4A2C7	0160-3878		CAPACITOR-FXD 1000PF +-20E 100MVDC CER	28480	0160-3878
A4A2L1	9100-2247	4	COIL-FXD WOLDED RF CHCKE 100MH 10E	24226	10/100
A4A2L2	08660-80005		INDUCTOR	28480	08660-80005
A4A2L3	08660-80005		INDUCTOR	28480	08660-80005
A4A2Q1	1854-0345	2	TRANSISTOR NPN 2N5179 SI TO-18 PD=200MW	04713	2N5179
A4A2Q2	1854-0345		TRANSISTOR NPN 2N5179 SI TO-18 PD=200MW	04713	2N5179
A4A2R1	0498-3429	3	RESISTOR 19.6 1% .125W F TC=0+-100	03088	PM55-1/8-TO-196-F
A4A2R2	0498-3151		RESISTOR 2.87K 1% .125W F TC=0+-100	16299	C4-1/8-TO-2871-F
A4A2R3	0737-0439		RESISTOR 6.81K 1% .125W F TC=0+-100	24546	C4-1/8-TO-6811-F
A4A2R4	0498-3440		RESISTOR 194 1% .125W F TC=0+-100	16299	C4-1/8-TO-194-F
A4A2R5	0737-0439		RESISTOR 6.81K 1% .125W F TC=0+-100	24546	C4-1/8-TO-6811-F
A4A2R6	0498-3151		RESISTOR 2.87K 1% .125W F TC=0+-100	16299	C4-1/8-TO-2871-F
A4A2R7	0498-3440	2	RESISTOR 194 1% .125W F TC=0+-100	16299	C4-1/8-TO-194-F
A4A2R8	0737-0294		RESISTOR 17.0 1% .125W F TC=0+-100	19701	MFAC1/8-TO-170-F
A4A2R9	0498-3443	1	RESISTOR 287 1% .125W F TC=0+-100	16299	C4-1/8-TO-287-F
A4A2R10	0498-3151	4	RESISTOR 2.87K 1% .125W F TC=0+-100	16299	C4-1/8-TO-2871-F
A4A2R11	0737-0294		RESISTOR 17.0 1% .125W F TC=0+-100	19701	MFAC1/8-TO-170-F
A4	86601-60000	1	MODULATOR ASSEMBLY	28480	86601-60000
	86601-20065	1	SHIELD, MODULATOR	28480	86601-20065
	86601-20072	1	COVER, MODULATOR ASSEMBLY	28480	86601-20072
A4E1	0160-3036	4	CAPACITOR-FXD 5000PF +80-20E 200MVDC CER	28480	0160-3036
A4E2	0160-3036		CAPACITOR-FXD 5000PF +80-20E 200MVDC CER	28480	0160-3036
A4E3	0160-3036		CAPACITOR-FXD 5000PF +80-20E 200MVDC CER	28480	0160-3036
A4E4	1250-1104	4	CONNECTOR-PP 54 510 M SGL MOLE FR	70001	50-045-0410
A4E5	1250-1104		CONNECTOR-PP 54 510 M SGL MOLE FR	70001	50-045-0410
A4E6	1250-1104		CONNECTOR-PP 54 510 M SGL MOLE FR	70001	50-045-0410
A4E7	1250-1104		CONNECTOR-PP 54 510 M SGL MOLE FR	70001	50-045-0410

Table 6-3. Replaceable Parts (P/O Errata; Page 2 of 2)

Reference Designation	MP Part Number	Qty	Description	Mfr Code	Mfr Part Number
ASA1	86601-60078	1	BOARD ASSEMBLY, MODULATOR	28480	86601-60078
ASA1C1	0160-3878		CAPACITOR-FRD 1000PF +-20% 100WVDC CER	28480	0160-3878
ASA1C2	0121-0447		CAPACITOR: VAR: TRMR; CER: 1.5/2.5PF	00865	75-TRMR-03 1.5-2.5
ASA1C3	0160-3878		CAPACITOR-FRD 1000PF +-20% 100WVDC CER	28480	0160-3878
ASA1C4	0160-3878		CAPACITOR-FRD 1000PF +-20% 100WVDC CER	28480	0160-3878
ASA1C5	0121-0447		CAPACITOR: VAR: TRMR; CER: 1.5/2.5PF	00865	75-TRMR-03 1.5-2.5
ASA1C6	0160-3878		CAPACITOR-FRD 1000PF +-20% 100WVDC CER	28480	0160-3878
ASA1C7	0160-2208	2	CAPACITOR-FRD 330PF +-5% 300WVDC MICA	28480	0160-2208
ASA1C8	0160-3878	2	CAPACITOR-FRD 1000PF +-20% 100WVDC CER	28480	0160-3878
ASA1C9	0160-3456	1	CAPACITOR-FRD 1000PF +-10% 100WVDC CER	28480	0160-3456
ASA1C10	0160-3456	1	CAPACITOR-FRD 1000PF +-10% 100WVDC CER	28480	0160-3456
ASA1E1	105148	2	MIXER, 500 MHZ	28480	105148
ASA1K1	0490-1013	1	RELAY; REED; IC .25A 2JW COM1; 5V CNIL	28480	0490-1013
ASA1L1	08660-80005		INDUCTOR	28480	08660-80005
ASA1L2	08660-80005		INDUCTOR	28480	08660-80005
ASA1L3	9180-2247		COIL-FRD MOLDED RF CHOKE 100MH 10% COIL-FRD MOLDED RF CHOKE 1UH 10%	24226	10/100 10/101
ASA1L4	9140-0198	2	COIL-FRD MOLDED RF CHOKE 1UH 10%	24226	10/101
ASA1Q1	1854-0345		TRANSISTOR NPN 2N5179 SI TO-72 PD=200MW	04713	2N5179
ASA1Q2	1854-0345		TRANSISTOR NPN 2N5179 SI TO-72 PD=200MW	04713	2N5179
ASA1R1	0698-3429		RESISTOR 19.6 1% .125W F TC=0+-100	03868	FRES5-1/8-TO-196R-F
ASA1R2	0757-0439		RESISTOR 6.81K 1% .125W F TC=0+-100	24546	C4-1/8-TO-6811-F
ASA1R3	0698-3429		RESISTOR 2.87K 1% .125W F TC=0+-100	16299	C4-1/8-TO-2871-F
ASA1R4	0698-3440		RESISTOR 19.6 1% .125W F TC=0+-100	16299	C4-1/8-TO-196R-F
ASA1R5	0757-0439		RESISTOR 6.81K 1% .125W F TC=0+-100	24546	C4-1/8-TO-6811-F
ASA1R6	0698-3151		RESISTOR 2.87K 1% .125W F TC=0+-100	16299	C4-1/8-TO-2871-F
ASA1R7	0698-3430		RESISTOR 19.6 1% .125W F TC=0+-100	16299	C4-1/8-TO-196R-F
ASA1R8	0757-0230		RESISTOR 1K 1% .125W F TC=0+-100	24546	C4-1/8-TO-1001-F
ASA1R9	0757-0230		RESISTOR 1K 1% .125W F TC=0+-100	24546	C4-1/8-TO-1001-F
ASA1R10	0757-1970	1	RESISTOR 91.1 1% .5W F TC=0+-100	19701	HF7C1/2-TO-9111-F
ASA1Z1	9170-0029		CURE, MAC, SHIELDING BEAD, .178 OD .047	02114	56-590-65A2/4A
ASA2	86601-60060	1	BOARD ASSEMBLY, MODULATOR II	28480	86601-60060
ASA2C1	0160-3878		CAPACITOR-FRD 1000PF +-20% 100WVDC CER	28480	0160-3878
ASA2C2	0121-0447		CAPACITOR: VAR: TRMR; CER: 1.5/2.5PF	00865	75-TRMR-03 1.5-2.5
ASA2C3	0160-3878		CAPACITOR-FRD 1000PF +-20% 100WVDC CER	28480	0160-3878
ASA2C4	0121-0447		CAPACITOR: VAR: TRMR; CER: 1.5/2.5PF	00865	75-TRMR-03 1.5-2.5
ASA2C5	0160-3878		CAPACITOR-FRD 1000PF +-20% 100WVDC CER	28480	0160-3878
ASA2C6	0160-3878		CAPACITOR-FRD 1000PF +-20% 100WVDC CER	28480	0160-3878
ASA2C7	0160-3456		CAPACITOR-FRD 1000PF +-10% 100WVDC CER	28480	0160-3456
ASA2C8	0160-2208		CAPACITOR-FRD 330PF +-5% 300WVDC MICA	28480	0160-2208
ASA2C9	0160-3878		CAPACITOR-FRD 1000PF +-20% 100WVDC CER	28480	0160-3878
ASA2E1	105148		MIXER, 500 MHZ	28480	105148
ASA2L1	08660-80005		INDUCTOR	28480	08660-80005
ASA2L2	08660-80005		INDUCTOR	28480	08660-80005
ASA2L3	9180-2247		COIL-FRD MOLDED RF CHOKE 100MH 10% COIL-FRD MOLDED RF CHOKE 1UH 10%	24226	10/100 10/101
ASA2L4	9140-0198		COIL-FRD MOLDED RF CHOKE 1UH 10%	24226	10/101
ASA2Q1	1854-0345		TRANSISTOR NPN 2N5179 SI TO-72 PD=200MW	04713	2N5179
ASA2Q2	1854-0345		TRANSISTOR NPN 2N5179 SI TO-72 PD=200MW	04713	2N5179
ASA2R1	0757-0439		RESISTOR 6.81K 1% .125W F TC=0+-100	24546	C4-1/8-TO-6811-F
ASA2R2	0698-3151		RESISTOR 2.87K 1% .125W F TC=0+-100	16299	C4-1/8-TO-2871-F
ASA2R3	0698-3440		RESISTOR 19.6 1% .125W F TC=0+-100	16299	C4-1/8-TO-196R-F
ASA2R4	0757-0439		RESISTOR 6.81K 1% .125W F TC=0+-100	24546	C4-1/8-TO-6811-F
ASA2R5	0698-3151		RESISTOR 2.87K 1% .125W F TC=0+-100	16299	C4-1/8-TO-2871-F
ASA2R6	0698-3440		RESISTOR 19.6 1% .125W F TC=0+-100	16299	C4-1/8-TO-196R-F
ASA2R7	0757-0230		RESISTOR 1K 1% .125W F TC=0+-100	24546	C4-1/8-TO-1001-F
ASA2R8	0757-0230		RESISTOR 1K 1% .125W F TC=0+-100	24546	C4-1/8-TO-1001-F
ASA2Z1	86601-20067	1	CABLE, MODULATOR	28480	86601-20067

Table 6-3. Replaceable Parts (P/O Change 1)

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
AS	06602-07040	1	ATTENUATOR 701/70N ASSY	20480	06602-07040
ABCR1	1901-0025	8	DIODE-GERM PRP 100V 200MA	20480	1901-0025
ABCR2	1901-0025		DIODE-GERM PRP 100V 200MA	20480	1901-0025
ABCR3	1901-0025		DIODE-GERM PRP 100V 200MA	20480	1901-0025
ABCR4	1901-0025		DIODE-GERM PRP 100V 200MA	20480	1901-0025
ABCR5	1901-0025		DIODE-GERM PRP 100V 200MA	20480	1901-0025
ABCR6	1901-0025	8	DIODE-GERM PRP 100V 200MA	20480	1901-0025
ABCR7	1901-0025		DIODE-GERM PRP 100V 200MA	20480	1901-0025
ABCR8	1901-0025		DIODE-GERM PRP 100V 200MA	20480	1901-0025
ABQ1	1853-0213	4	TRANSISTOR PNP 2N4236 SI CHIP PD=1	04713	2N4236
ABQ2	1854-0361		TRANSISTOR NPN 2N4239 SI PD=800MW	04713	2N4239
ABQ3	1853-0020		TRANSISTOR PNP SI CHIP PD=300MW	20480	1853-0020
ABQ4	1854-0071		TRANSISTOR NPN SI PD=300MW FT=200MHZ	20480	1854-0071
ABQ5	1854-0404		TRANSISTOR NPN SI TO-18 PD=300MW	20480	1854-0404
ABQ6	1853-0020	4	TRANSISTOR PNP SI CHIP PD=300MW	20480	1853-0020
ABQ7	1853-0213		TRANSISTOR PNP 2N4236 SI CHIP PD=1W	04713	2N4236
ABQ8	1854-0361		TRANSISTOR NPN 2N4239 SI PD=800MW	04713	2N4239
ABQ9	1853-0020		TRANSISTOR PNP SI CHIP PD=300MW	20480	1853-0020
ABQ10	1854-0071		TRANSISTOR NPN SI PD=300MW FT=200MHZ	20480	1854-0071
ABQ11	1854-0404	4	TRANSISTOR NPN SI TO-18 PD=300MW	20480	1854-0404
ABQ12	1853-0020		TRANSISTOR PNP SI CHIP PD=300MW	20480	1853-0020
ABQ13	1853-0213		TRANSISTOR PNP 2N4236 SI CHIP PD=1W	04713	2N4236
ABQ14	1854-0361		TRANSISTOR NPN 2N4239 SI PD=800MW	04713	2N4239
ABQ15	1853-0020		TRANSISTOR PNP SI CHIP PD=300MW	20480	1853-0020
ABQ16	1854-0071	4	TRANSISTOR NPN SI PD=300MW FT=200MHZ	20480	1854-0071
ABQ17	1854-0404		TRANSISTOR NPN SI TO-18 PD=300MW	20480	1854-0404
ABQ18	1853-0020		TRANSISTOR PNP SI CHIP PD=300MW	20480	1853-0020
ABQ19	1853-0213		TRANSISTOR PNP 2N4236 SI CHIP PD=1W	04713	2N4236
ABQ20	1854-0361		TRANSISTOR NPN 2N4239 SI PD=800MW	04713	2N4239
ABQ21	1853-0020	4	TRANSISTOR PNP SI CHIP PD=300MW	20480	1853-0020
ABQ22	1854-0071		TRANSISTOR NPN SI PD=300MW FT=200MHZ	20480	1854-0071
ABQ23	1854-0404		TRANSISTOR NPN SI TO-18 PD=300MW	20480	1854-0404
ABQ24	1853-0020		TRANSISTOR PNP SI CHIP PD=300MW	20480	1853-0020
ABR1	0757-0290		8	RESISTOR 1K 1% .125W F TUBULAR	24546
ABR2	0757-0159	RESISTOR 1K 1% .5W F TUBULAR		19701	MF7C1/2-T0-100-F
ABR3	0757-0159	RESISTOR 1K 1% .5W F TUBULAR		19701	MF7C1/2-T0-100-F
ABR4	0698-3440	RESISTOR 196 OHM 1% .125W F TUBULAR		16299	C4-1/8-T0-196-F
ABR5	0811-2915	RESISTOR 1.5 OHM 5% .5W PW TUBULAR		91637	PS1/2-T2-195-J
ABR6	0811-2915	4	RESISTOR 1.5 OHM 5% .5W PW TUBULAR	91637	PS1/2-T2-195-J
ABR7	0757-0290		RESISTOR 1K 1% .125W F TUBULAR	24546	C4-1/8-T0-1001-F
ABR8	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR9	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR10	0698-3440		RESISTOR 196 OHM 1% .125W F TUBULAR	16299	C4-1/8-T0-196-F
ABR11	0757-0290	4	RESISTOR 1K 1% .125W F TUBULAR	24546	C4-1/8-T0-1001-F
ABR12	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR13	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR14	0698-3440		RESISTOR 196 OHM 1% .125W F TUBULAR	16299	C4-1/8-T0-196-F
ABR15	0811-2915		RESISTOR 1.5 OHM 5% .5W PW TUBULAR	91637	PS1/2-T2-195-J
ABR16	0811-2915	4	RESISTOR 1.5 OHM 5% .5W PW TUBULAR	91637	PS1/2-T2-195-J
ABR17	0757-0290		RESISTOR 1K 1% .125W F TUBULAR	24546	C4-1/8-T0-1001-F
ABR18	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR19	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR20	0698-3440		RESISTOR 196 OHM 1% .125W F TUBULAR	16299	C4-1/8-T0-196-F
ABR21	0757-0290	4	RESISTOR 1K 1% .125W F TUBULAR	24546	C4-1/8-T0-1001-F
ABR22	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR23	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR24	0698-3440		RESISTOR 196 OHM 1% .125W F TUBULAR	16299	C4-1/8-T0-196-F
ABR25	0811-2915		RESISTOR 1.5 OHM 5% .5W PW TUBULAR	91637	PS1/2-T2-195-J
ABR26	0811-2915	4	RESISTOR 1.5 OHM 5% .5W PW TUBULAR	91637	PS1/2-T2-195-J
ABR27	0757-0290		RESISTOR 1K 1% .125W F TUBULAR	24546	C4-1/8-T0-1001-F
ABR28	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR29	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR30	0698-3440		RESISTOR 196 OHM 1% .125W F TUBULAR	16299	C4-1/8-T0-196-F
ABR31	0757-0290	4	RESISTOR 1K 1% .125W F TUBULAR	24546	C4-1/8-T0-1001-F
ABR32	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR33	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR34	0698-3440		RESISTOR 196 OHM 1% .125W F TUBULAR	16299	C4-1/8-T0-196-F
ABR35	0811-2915		RESISTOR 1.5 OHM 5% .5W PW TUBULAR	91637	PS1/2-T2-195-J
ABR36	0811-2915	4	RESISTOR 1.5 OHM 5% .5W PW TUBULAR	91637	PS1/2-T2-195-J
ABR37	0757-0290		RESISTOR 1K 1% .125W F TUBULAR	24546	C4-1/8-T0-1001-F
ABR38	0757-0159		RESISTOR 1K 1% .5W F TUBULAR	19701	MF7C1/2-T0-100-F
ABR39	0698-3440		RESISTOR 196 OHM 1% .125W F TUBULAR	16299	C4-1/8-T0-196-F
ABR40	0811-2915		RESISTOR 1.5 OHM 5% .5W PW TUBULAR	91637	PS1/2-T2-195-J
ABV1	1902-3002	8	DIODE-ZNR 2.37V SE 00-7 PD=.4W TC=	04713	52 10930-2
ABV2	1902-3002		DIODE-ZNR 2.37V SE 00-7 PD=.4W TC=	04713	52 10930-2
ABV3	1902-3002		DIODE-ZNR 2.37V SE 00-7 PD=.4W TC=	04713	52 10930-2
ABV4	1902-3002		DIODE-ZNR 2.37V SE 00-7 PD=.4W TC=	04713	52 10930-2

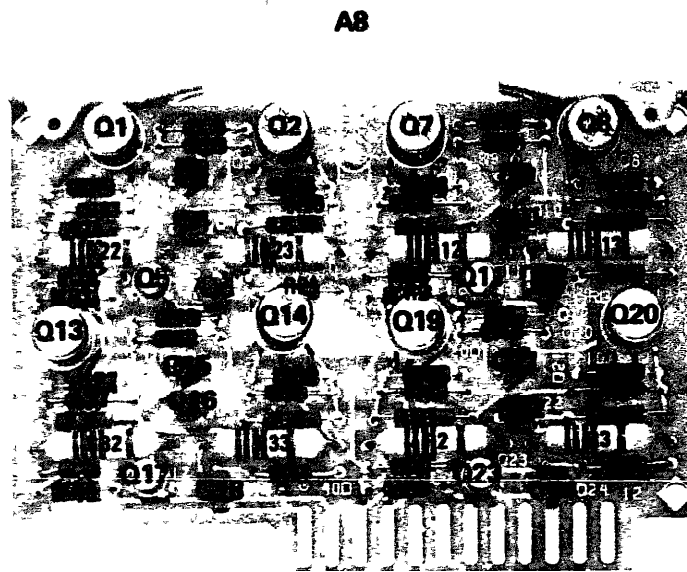


Figure 8-27. Attenuator Driver Component Locations (P/O Change 1)

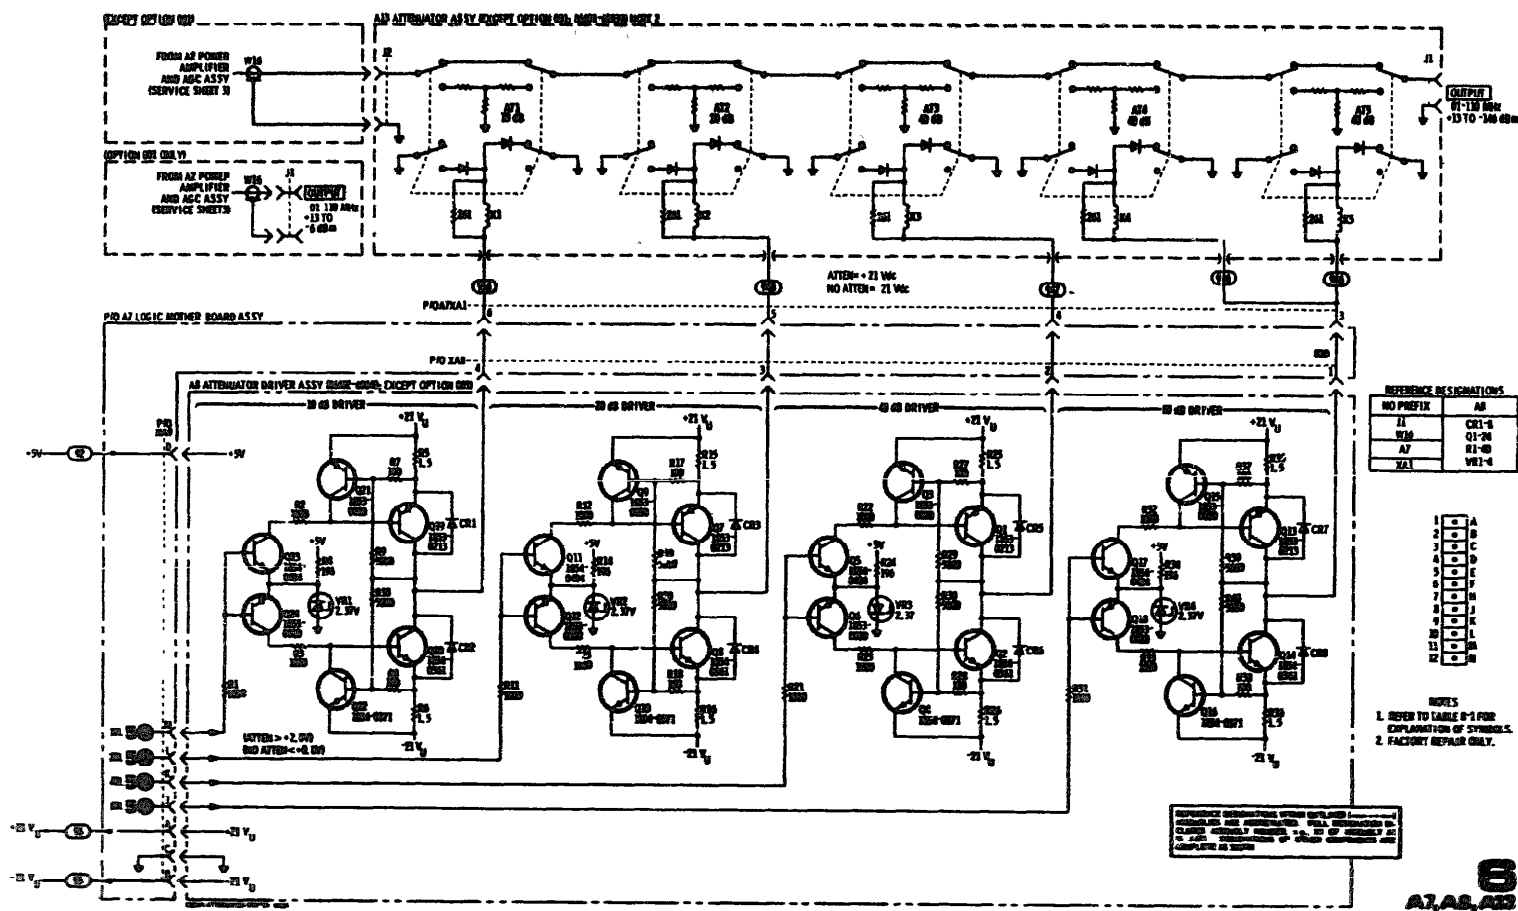


Figure 8-28. Attenuator Driver Assembly (P/O Change 1)

CHANGE 5

Page 6-8, Table 6-3 and page 8-21, Figure 8-28 (Service Sheet 6):

Delete ~~A8R9~~, ~~R10~~, ~~R19~~, ~~R20~~, ~~R29~~, R30, R39 and R40.

► CHANGE 8

Page 5-1:

Add the following paragraph:

FACTORY SELECTED COMPONENTS

Factory selected components are identified on the schematics and parts list by an asterisk which follows the reference designator. The normal value of the components are shown. The manual change sheets will provide updated information pertaining to the selected components. Tabel 5-1 lists the reference designator, the criterion used for selecting a particular value, the normal value range, and the service sheet where the component part is shown.

Page 5-1:

Add the following table:

Factory Selected Components

Reference Designator	Selected For	Normal Value Range	Service Sheet
A2R39	Minimum AM distortion at 90% AM depth with VERNIER control set for meter reading of -6 dB and OUTPUT RANGE switch set to +10 dBm.	400Ω to ∞	3
A5A1R1, A5A1R6, A5A2R1, A5A2R2, A5A2R6, A5A2R7, A5A2R8, and A5A2R12	Gain of ≥ 41 dB with +0.5 Vdc on the control input; < 1 dB with +0.1 Vdc on the control line. Change the resistors as indicated in the Modulator Assembly Adjustments.	68.1Ω or omitted 68.1Ω or 511Ω 68.1Ω or omitted 0 or 26.1Ω 68.1Ω or 511Ω 68.1Ω or 511Ω 68.1Ω or omitted	2

Page 5-10:

Add the following adjustment procedure.

5-19. MODULATOR ASSEMBLY ADJUSTMENT

REFERENCE: Service Sheet 2.

DESCRIPTION: The fixed dynamic range of the modulator is set so the gain extremes extend beyond specified limits. The gain extremes are set by selecting resistors with a specific control voltage input to the modulators.

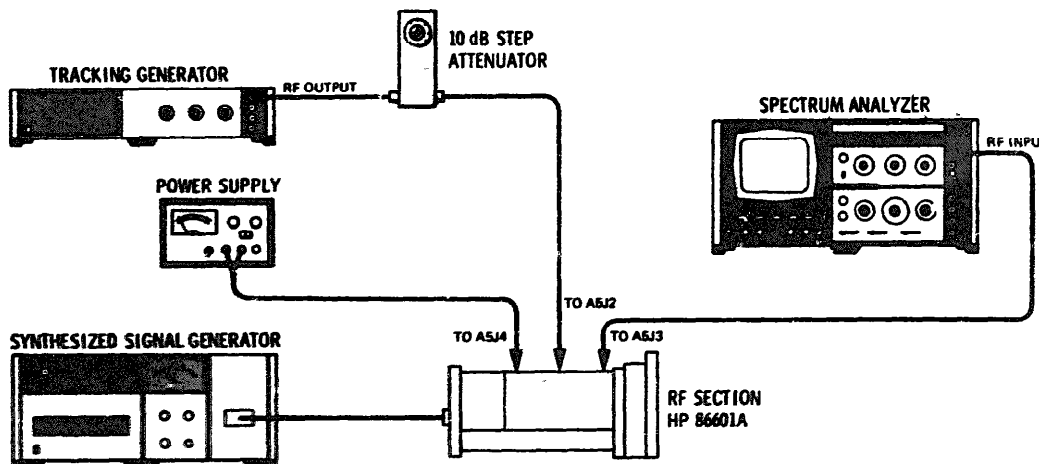


Figure 5-7. Modulator Assembly Adjustment Test Setup.

EQUIPMENT:	Tracking Generator	HP 8444A
	Spectrum Analyzer	HP 140T/8554L/8552B
	Electronic Counter	HP 5245M/5253B
	Extender Cable	HP 11672-60001
	10 dB Step Attenuator	HP 355D
	Power Supply	HP 6214A

- PROCEDURE:**
- 1 . Remove the Model 86601A from the mainframe. Remove the cover and reconnect the Model 86601A with extender cable 11672-60001.
 - 2 . Connect the Tracking Generator to the Spectrum Analyzer. (Refer to the Tracking Generator Operating and Service Manual.)
 - 3 . Set the Spectrum Analyzer controls as follows: INPUT ATTENUATION 20 dB, LOG REF LEVEL +10 dBm, SCAN WIDTH PER DIVISION 2 MHz, SCAN TIME PER DIVISION 10 MILLISECONDS and BANDWIDTH 300 kHz.
 - 4 . Connect the Tracking Generator RF OUTPUT to the Electronic Counter with the Spectrum Analyzer in the ZERO scan mode.
 - 5 . Set the Spectrum Analyzer frequency to 455 MHz as indicated by the Electronic Counter.
 - 6 . Set the 10 dB step attenuator for 10 dB attenuation. Adjust the Tracking Generator LEVEL to a reference of -24 dBm as indicated on the analyzer display.

CHANGE 6 (Cont'd)

7. Set the power supply voltage to +5.0 Vdc.
8. **Connect** the equipment as shown in Figure 5-7.
9. **Verify that the output is greater than or equal to +18 dBm. If the output is correct, proceed to step 10. Otherwise, change the following resistors in the order shown until the output is at least +18 dBm.**

Reference Designator	Change To
A5A1R1 A5A2R12	remove 511Ω
A5A2R1 A5A2R6	remove 511Ω
A5A1R6 A5A2R7	511Ω remove
A5A2R2 A5A2R8	0Ω (wire) 0Ω (wire)

10. Set the power supply voltage to +0.10 Vdc. Verify that the output is less than or equal to -23 dBm. If the output is correct, the adjustment is complete. Otherwise, change the following resistors in the order shown until the output is the less than or equal to -23 dBm. If any resistors are changed, return to step 7 and recheck the levels in step 9.

Reference Designator	Change To
A5A2R1 A5A2R6	68.1Ω 68.1Ω
A5A2R12 A5A2R1	68.1Ω 68.1Ω
A5A1R6 A5A2R7	68.1Ω 68.1Ω
A5A2R2 A5A2R8	26.1Ω 26.1Ω

Page 6-4, Table 6.2

ADD ABOVE, 1/16-INCH RESISTOR 68 1Ω 1% 120V 7 TC-60000
 ADD 32 WIREWOUND, 1/16-INCH, 1% RESISTOR 26 1Ω 1% 120V 7 TC-60000
 ADD 32 WIREWOUND, 1/16-INCH, 1% RESISTOR 68 1Ω 1% 120V 7 TC-60000

Model 86601A

Manual Changes

CHANGE 6 (Cont'd)

Page 6-5 and 6-6, Table 6-3:

Change the parts list for the A5 Assembly as shown in the table.

Page 8-13, Figure 8-17 (Service Sheet 2):

Change the diagram as shown in the partial schematic.

Page 8-15, Figure 8-20 (Service Sheet 3):

Add A2R39*, 619 ohms, in parallel with A2CR5.

Table 6-3. Replaceable Part (P/O Change 6; 2 of 2)

Reference Designation	HP Part Number	Qty	Description	Mfr Code	Mfr Part Number
RECEIVER	0000-0000	1	RECEIVER ASSEMBLY	2000	CD-100-00-0000-0
RECEIVER	0000-0000		RECEIVER ASSEMBLY	2000	CD-100-00-0000-0
RECEIVER	0000-0000		RECEIVER ASSEMBLY	2000	CD-100-00-0000-0
RECEIVER	0000-0000		RECEIVER ASSEMBLY	2000	CD-100-00-0000-0
RECEIVER	0000-0000		RECEIVER ASSEMBLY	2000	CD-100-00-0000-0
RECEIVER	0000-0000		RECEIVER ASSEMBLY	2000	CD-100-00-0000-0
RECEIVER	0000-0000		RECEIVER ASSEMBLY	2000	CD-100-00-0000-0
RECEIVER	0000-0000		RECEIVER ASSEMBLY	2000	CD-100-00-0000-0

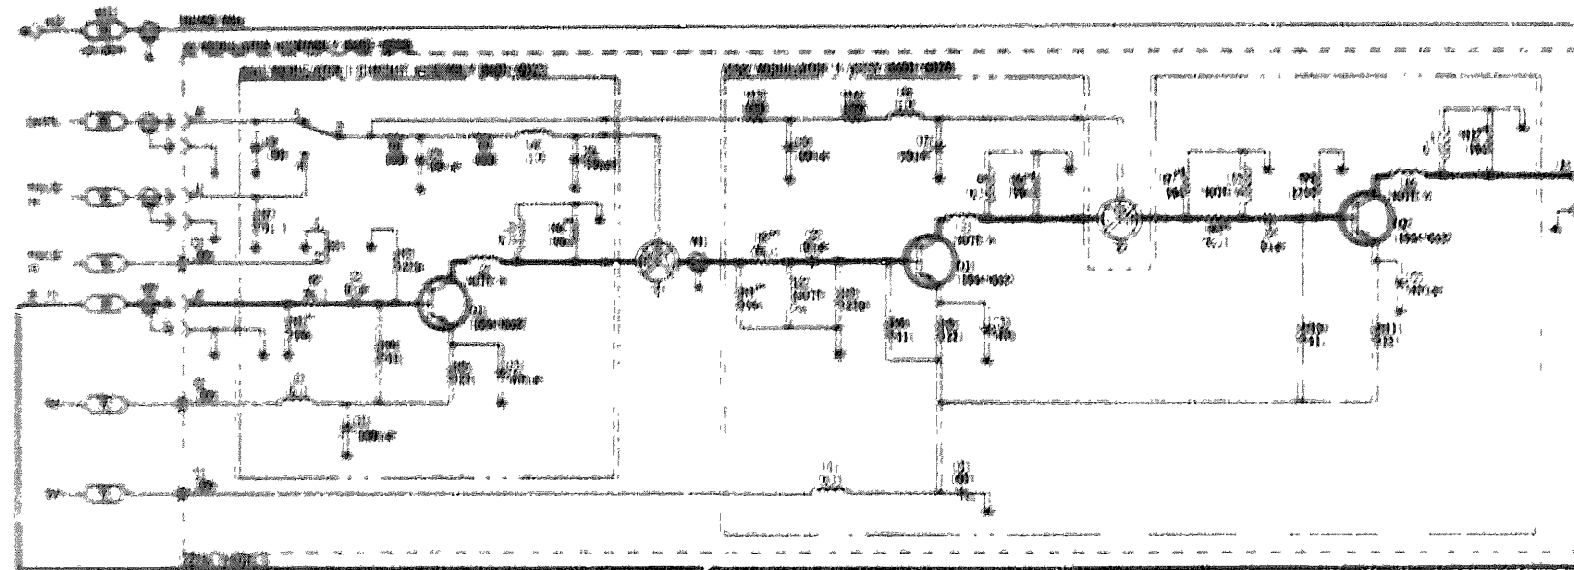


Figure 6-3. *Pitron Micron and Modulator Submodule (partial alternate parts) Change 6.*

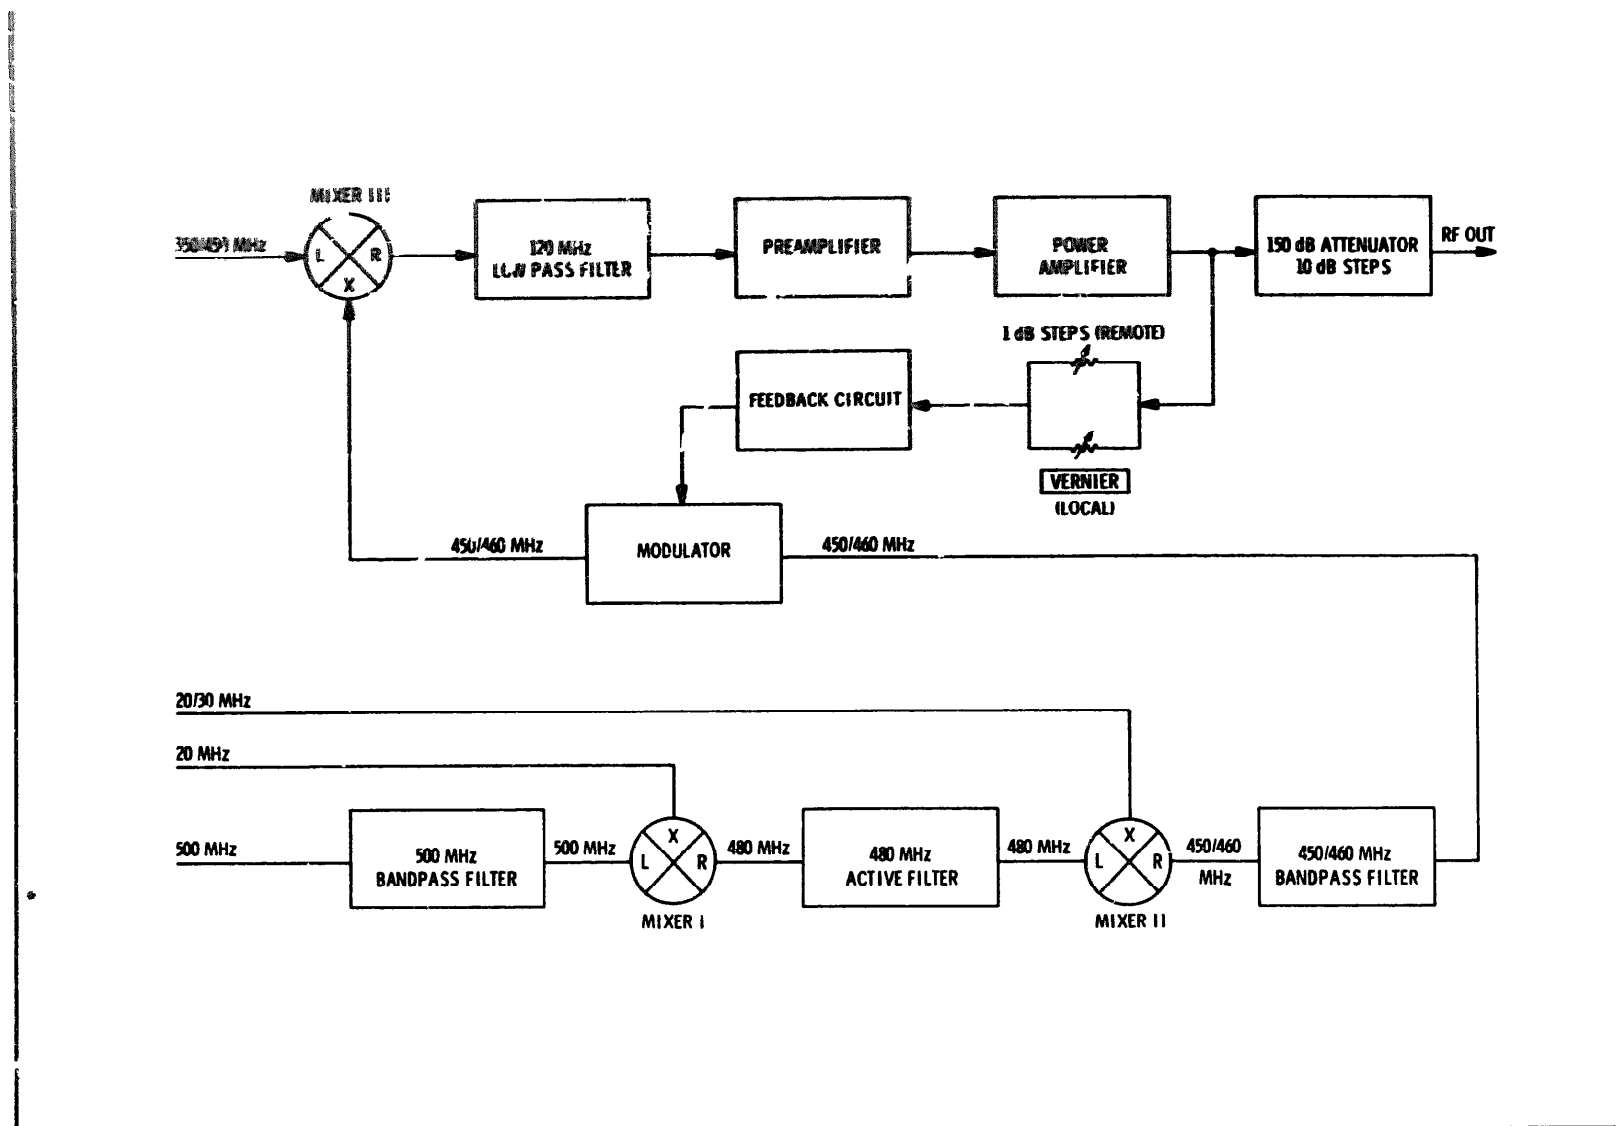


Figure 8-1. Model 86601A Simplified Block Diagram

SECTION VIII

SERVICE

8-1. INTRODUCTION

8-2. This section provides instructions for testing, troubleshooting and repairing the Hewlett-Packard Model 86601A RF Section. Information throughout this section is based on the assumption that the Model 86601A is interconnected with a Model 8660 Synthesized Signal Generator that is functioning properly.

8-3. PRINCIPLES OF OPERATION

8-4. Figure 8-1, Simplified Block Diagram, and the following discussion illustrate the basic principles of the Model 86601A. More detailed information about principles of operation of the Model 86601A may be found in the text for Service Sheet 1. In addition, detailed information to the circuit level is provided on the individual service sheets.

8-5. The Model 86601A RF Section has no internal oscillators. The output frequency is developed by mixing and filtering the precise digitally controlled rf inputs from the mainframe. The inputs from the mainframe are:

- a. A 500 MHz signal from the reference section.
- b. A 20 MHz signal from the reference section which is coupled through the Modulation Section.

NOTE

In the FM mode the 20 MHz signal is generated in the **Modulation Section**.

- c. **A signal between 20.000001 and 30.00000 MHz (1 Hz resolution) from the SL1 Loop.**

NOTE

In option 004 mainframes this signal is between 20.0001 and 30.0000 MHz (100 Hz resolution).

- d. **A signal between 350 and 450 MHz (10 MHz steps) from the RF Loop.**

8-6. There are three mixers in the Model 86601A. Mixer I mixes the 500 MHz and the 20 MHz inputs to produce a 480 MHz output. The 480 MHz signal is amplified and filtered and then coupled to Mixer

II where it is mixed with the 20 to 30 MHz signal from the mainframe SL1 Loop to provide a 450 to 460 MHz output. The output of Mixer II is filtered and amplified, and in the AM mode, modulated before it is coupled to Mixer III. In Mixer III the 450 to 460 MHz signal is mixed with the 350 to 450 MHz signal to produce the final output frequency which is between .01 and 100.999999 MHz (.01 to 109.99999 MHz when option 004 mainframe is used).

8-7. The output of Mixer III is coupled through two 120 MHz low pass filters and a pre-amplifier to the power amplifier.

8-8. The power amplifier assembly contains an Automatic Gain Control circuit which controls a feedback amplifier in the leveling loop. Code 1 and Code 2 inputs from the mainframe DCU operate an electronic band switch to aid in leveling the rf output across the output range.

8-9. Three attenuators are used to control the output level of the Model 86601A. These attenuators function as follows:

- a. In the local mode a 150 dB programmable attenuator, OUTPUT RANGE, controls the output level from +10 dBm to -140 dBm in 10 dB steps. A VERNIER control adds the capability of setting the output level to +13 dBm and to other points between the 10 dB steps.

- b. In the remote mode the 150 dB **programmable attenuator is remotely controlled and the front panel controls (OUTPUT RANGE and VERNIER) are inoperative.** A 1 dB per step **programmable attenuator in the Model 86601A is remotely programmed to set the output level between the 10 dB steps of the 150 dB attenuator.**

8-10.0 RECOMMENDED TEST EQUIPMENT

8-11. Test equipment and accessories required to maintain the Model 86601A are listed in the Maintenance Allocation Chart. Substitute test equipments are listed in Table 1-2.

8-12. TROUBLESHOOTING

8-13. Troubleshooting procedures are divided into two maintenance levels in this manual.

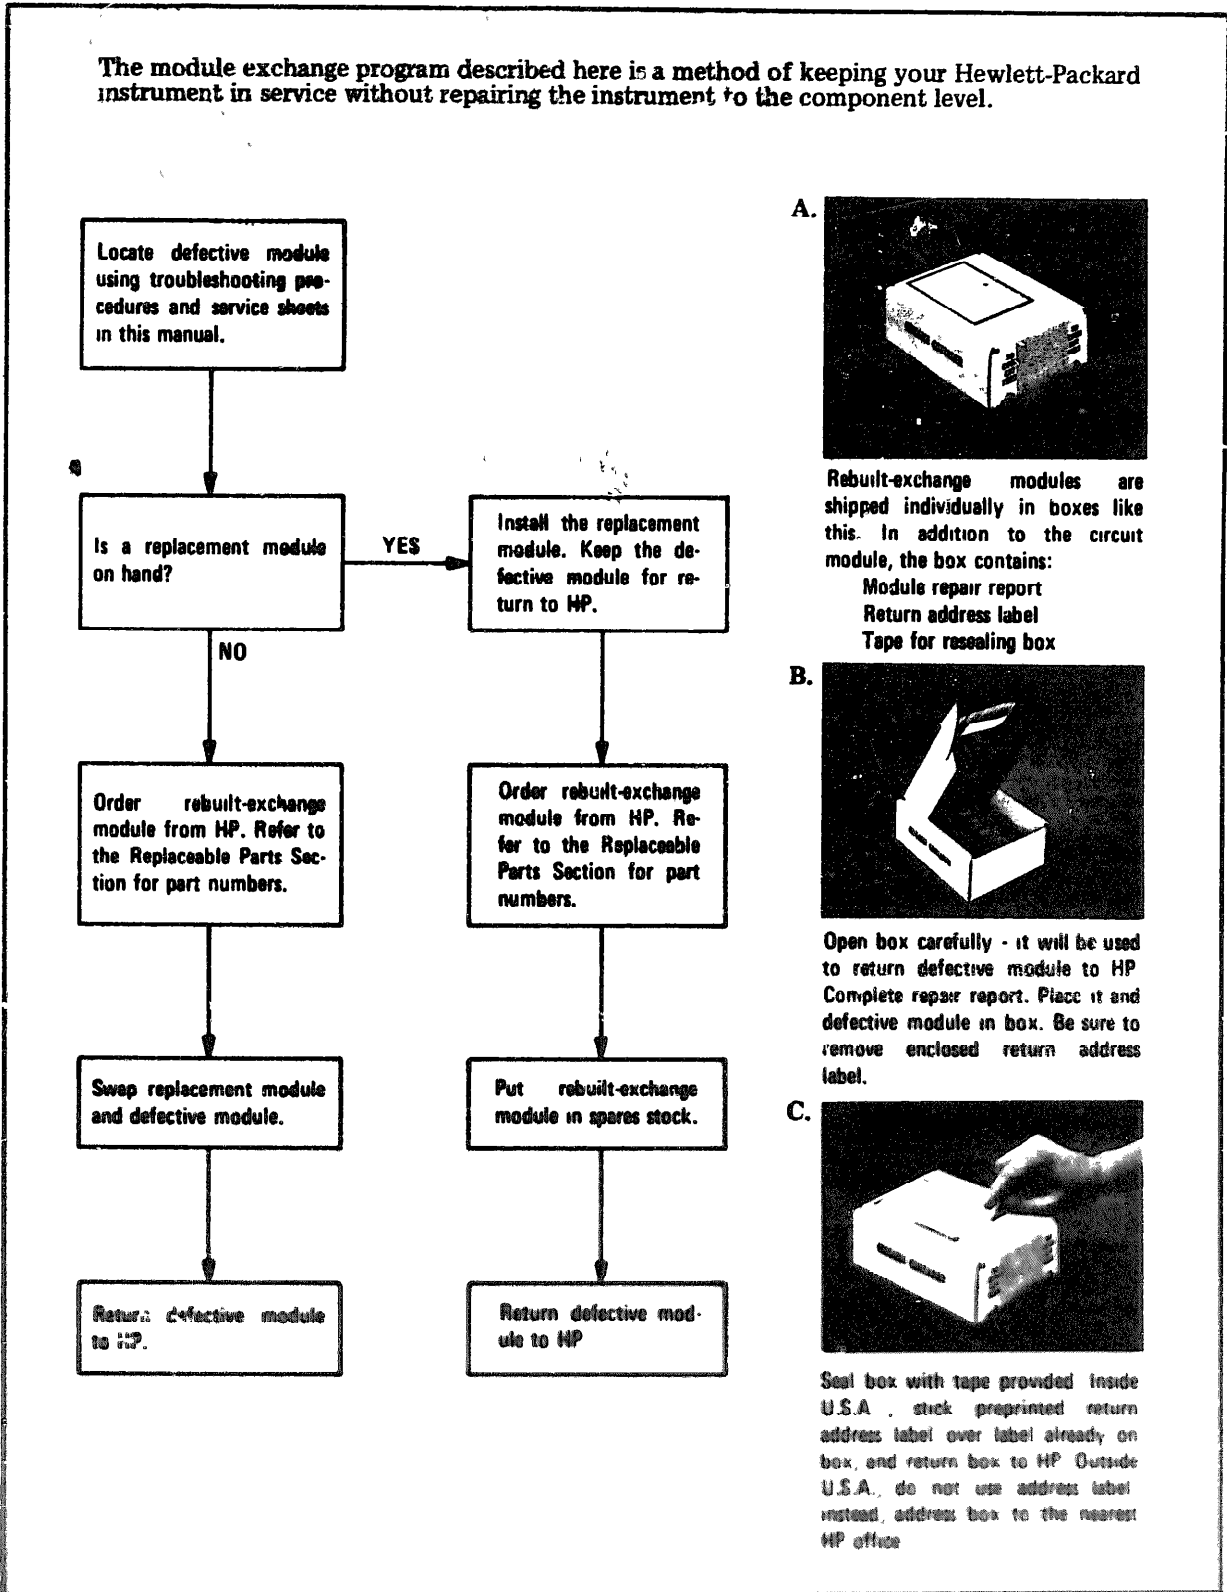


Figure 8-2. Diagram of Module Exchange Program

SECTION VIII

SERVICE

8-1. INTRODUCTION

8-2. This section provides instructions for testing, troubleshooting and repairing the Hewlett-Packard Model 86601A RF Section. Information throughout this section is based on the assumption that the Model 86601A is interconnected with a Model 8660 Synthesized Signal Generator that is functioning properly.

8-3. PRINCIPLES OF OPERATION

8-4. Figure 8-1, Simplified Block Diagram, and the following discussion illustrate the basic principles of the Model 86601A. More detailed information about principles of operation of the Model 86601A may be found in the text for Service Sheet 1. In addition, detailed information to the circuit level is provided on the individual service sheets.

8-5. The Model 86601A RF Section has no internal oscillators. The output frequency is developed by mixing and filtering the precise digitally controlled rf inputs from the mainframe. The inputs from the mainframe are:

a. A 500 MHz signal from the reference section.

b. A 20 MHz signal from the reference section which is coupled through the Modulation Section.

NOTE

In the FM mode the 20 MHz signal is generated in the Modulation Section.

c. A signal between 20.000001 and 30.00000 MHz (1 Hz resolution) from the SL1 Loop.

NOTE

In option 004 mainframes this signal is between 20.0001 and 30.0000 MHz (100 Hz resolution)

d. A signal between 350 and 450 MHz (10 MHz steps) from the RF Loop.

8-6. There are three mixers in the Model 86601A. Mixer I mixes the 300 MHz and the 20 MHz inputs to produce a 480 MHz output. The 480 MHz signal is amplified and filtered and then coupled to Mixer

II where it is mixed with the 20 to 30 MHz signal from the mainframe SL1 Loop to provide a 450 to 460 MHz output. The output of Mixer II is filtered and amplified, and in the AM mode, modulated before it is coupled to Mixer III. In Mixer III the 450 to 460 MHz signal is mixed with the 350 to 450 MHz signal to produce the final output frequency which is between .01 and 109.999999 MHz (01 to 109.9999 MHz when option 004 mainframe is used).

8-7. The output of Mixer III is coupled through two 120 MHz low pass filters and a pre-amplifier to the power amplifier.

8-8. The power amplifier assembly contains an Automatic Gain Control circuit which controls a feedback amplifier in the leveling loop. Code 1 and Code 2 inputs from the mainframe DCU operate an electronic band switch to aid in leveling the rf output across the output range.

8-9. Three attenuators are used to control the output level of the Model 86601A. These attenuators function as follows:

a. In the local mode a 150 dB programmable attenuator, OUTPUT RANGE, controls the output level from +10 dBm to -140 dBm in 10 dB steps. A VERNIER control adds the capability of setting the output level to +13 dBm and to other points between the 10 dB steps.

b. In the remote mode the 150 dB programmable attenuator is remotely controlled and the front panel controls (OUTPUT RANGE and VERNIER) are inoperative. A 1 dB per step programmable attenuator in the Model 86601A is remotely programmed to set the output level between the 10 dB steps of the 150 dB attenuator

8-10. RECOMMENDED TEST EQUIPMENT

8-11. Test equipment and accessories required to maintain the Model 86601A are listed in the Maintenance Allocation Chart. Substitute test equipments are listed in Table 1-2.

8-12. TROUBLESHOOTING

8-13. Troubleshooting procedures are divided into two maintenance levels in this manual.

8-14. The first maintenance level is designed to utilize the Hewlett-Packard Module Exchange Program. A troubleshooting tree enables a relatively inexperienced technician to isolate the cause of a malfunction to a circuit board or assembly. A factory-repaired replacement for the defective circuit board or assembly may be ordered through the nearest HP Sales and Service office using the special part numbers listed in Table 6-1. Refer to paragraph 8-18 and to figure 8-2 for additional information relative to the Module Exchange Program.

8-15. The second maintenance level involves repairing the instrument to the component level. The troubleshooting tree, in addition to aiding in the detection of faulty circuit boards or assemblies, also refers the technician to the appropriate service sheets to be used if repairs are to be accomplished to the component level. Circuit descriptions and test procedures for this maintenance level are located on the page facing the schematic diagram of the circuit to be repaired.

8-16. If the cause of a malfunction is found and remedied in any circuit containing adjustable components, the applicable adjustment procedure in Section V of this manual should be performed.

8-17. REPAIR

8-18. **Module Exchange.** This instrument, because of its modular design, may be repaired by simply replacing a defective module. Modular design is a method of construction that groups individual circuits on a replaceable assembly. Modular design, coupled with a factory-repaired module exchange program, eliminates the need to repair to the component level. Factory-repaired modules are available on an exchange-for-credit basis that reduces module cost substantially below the cost of a new module.

8-19. This manual provides a procedure which enables the technician to quickly isolate the cause of a malfunction to a defective module.

8-20. Exchange modules should be ordered by the exchange numbers shown in Table 6-1 from the nearest HP Sales and Service office.

8-21. Figure 8-2 illustrates the module exchange program.

NOTE

Do not send a defective module to the HP office until the replacement module is received.

8-22. **Voltage Requirements.** All power required to operate the Model 86601A is provided by the mainframe.

8-23. **Servicing Aids on Printed Circuit Boards.** Servicing aids on printed circuit boards include test points, transistor and integrated circuit reference designations, adjustment callouts and assembly stock numbers.

8-24. **Circuit Board Extenders.** Circuit board extenders are provided with the mainframe. These extender boards enable the technician to extend plug-in boards clear of the assembly to provide easy access to components and test points. See Figure 8-3 for a typical example of extender board Use.



8-25. **Diagram Notes.** Table 8-1, Schematic Diagram Notes, provides information relative to symbols and values shown on the schematic diagrams.

8-26. **Part Location Aids.** The locations of chassis mounted parts and major assemblies are shown in Figure 8-6. The locations of individual components mounted on printed circuit boards or other assemblies are shown on the appropriate schematic page or on the page opposite it. The part reference designator (as listed in Section VI) is the assembly designation plus the part designation (Example A10R1 is R1 on the A10 assembly). For specific component descriptions refer to the parts list in Section VI of this manual.


8-27. Table 8-2 lists all assemblies and provides location information for photos, schematics, etc.

8-28. **Integrated Circuits.** Integrated circuit packaging is shown in Figure 8-5. Many types of IC's are used in the Model 86601A. In order to avoid duplicating information on the individual schematics, all IC outlines and pin numbers are shown in Figure 8-5.


The module exchange program described here is a method of keeping your Hewlett-Packard instrument in service without repairing the instrument to the component level.

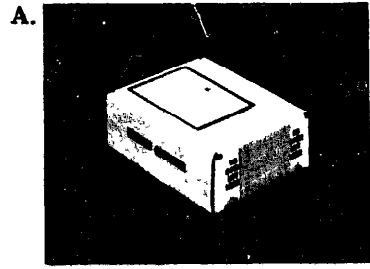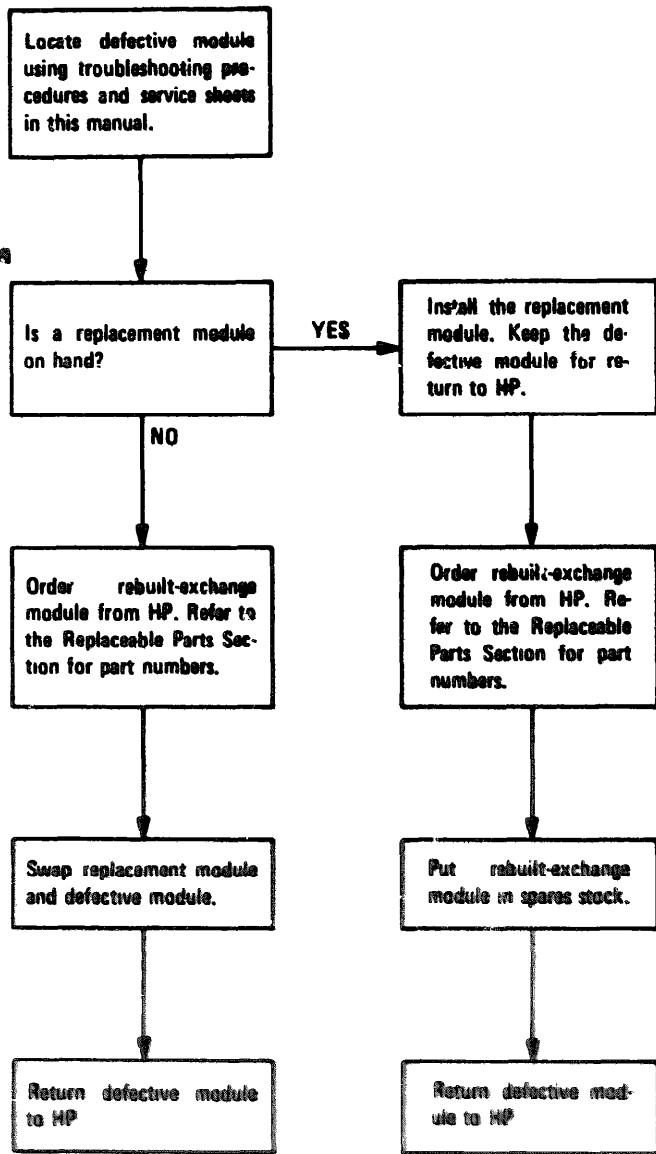

A.
Rebuilt-exchange modules are shipped individually in boxes like this. In addition to the circuit module, the box contains:
Module repair report
Return address label
Tape for resealing box

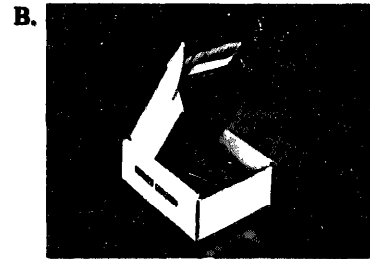

B.
Open box carefully - it will be used to return defective module to HP. Complete repair report. Place it and defective module in box. Be sure to remove enclosed return address label.

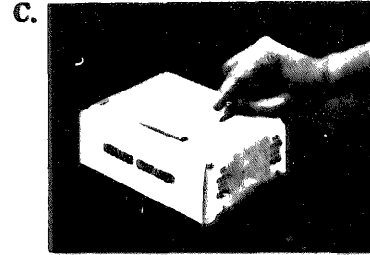

C.
Seal box with tape provided. Inside U.S.A., stick preprinted return address label over label already on box, and return box to HP. Outside U.S.A., do not use address label; instead, address box to the nearest HP office.

Figure 8-2. Diagram of Module Exchange Program

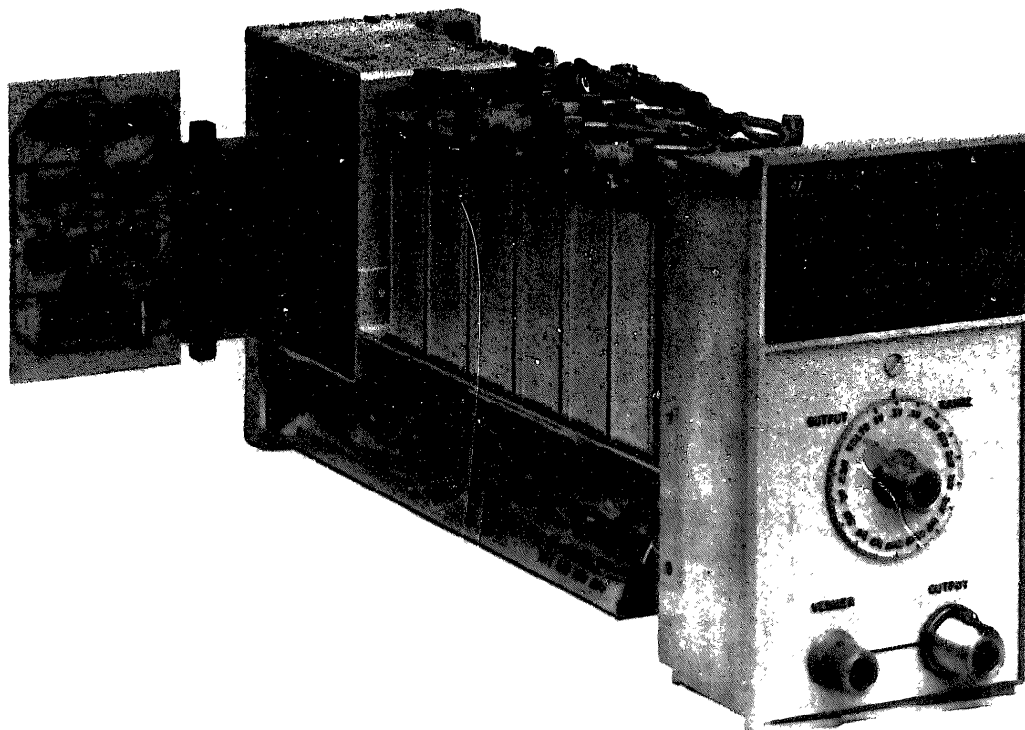














Figure 8-3. *Model 86601A with Circuit Board Extended for Maintenance*

Table 8-1. Schematic Diagram Notes

SCHEMATIC DIAGRAM NOTES

	Inductance is in microhenries, Resistance is in ohms and Capacitance is in microfarads unless otherwise noted.	
P/O	part of	
	Screwdriver Adjustment	
	Encloses Front Panel designations	
	Circuit assembly borderline	
	Other assembly borderline	
	Wiper moves toward CW with clockwise rotation of control as viewed from shaft or knob.	
	Numbers in stars on circuit assemblies show locations of test points	
	Encloses WIPE color code. Code used (MIL-STD-681) is the same as the resistor color code. First number identifies the base color, second number the wider stripe, and the third number the narrower stripe. Example; (947) denotes white base, yellow wide stripe, violet narrow stripe.	
	Indicates an output from a schematic that goes to an input identified as (A) on Service Sheet 2	
	Indicates an input to a schematic that comes from an output identified as (K) on Service Sheet 6.	
	Indicates Circuit ground	

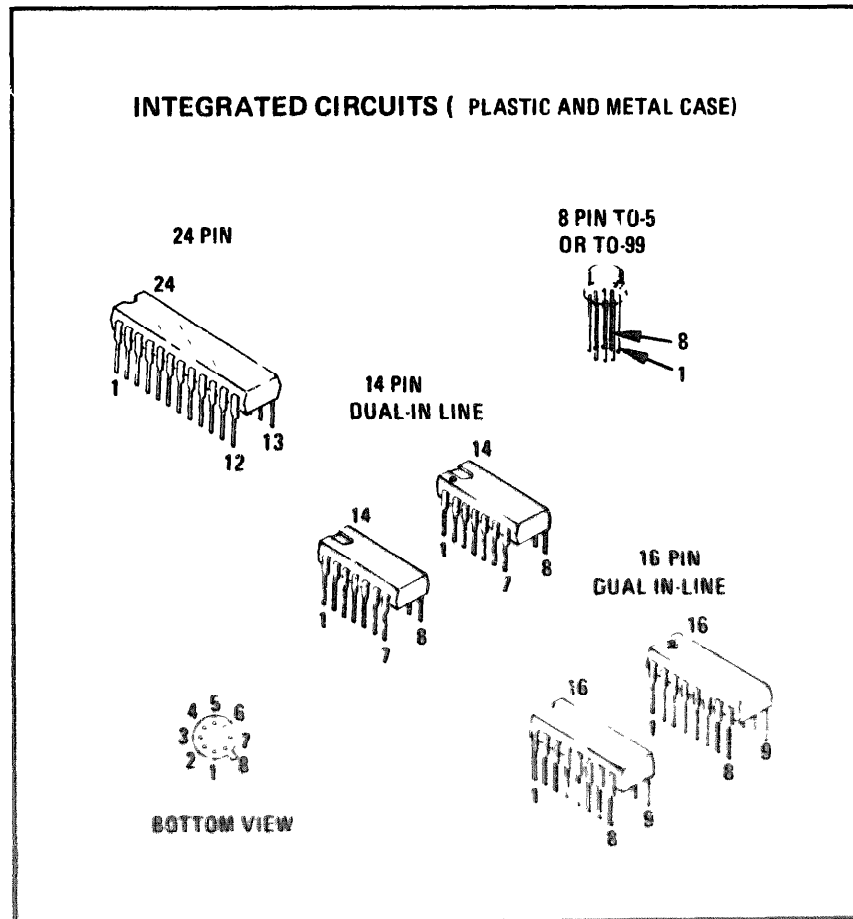


Figure 8-4. *Integrated Circuit Packaging*

Table 8-2. Assembly Locations

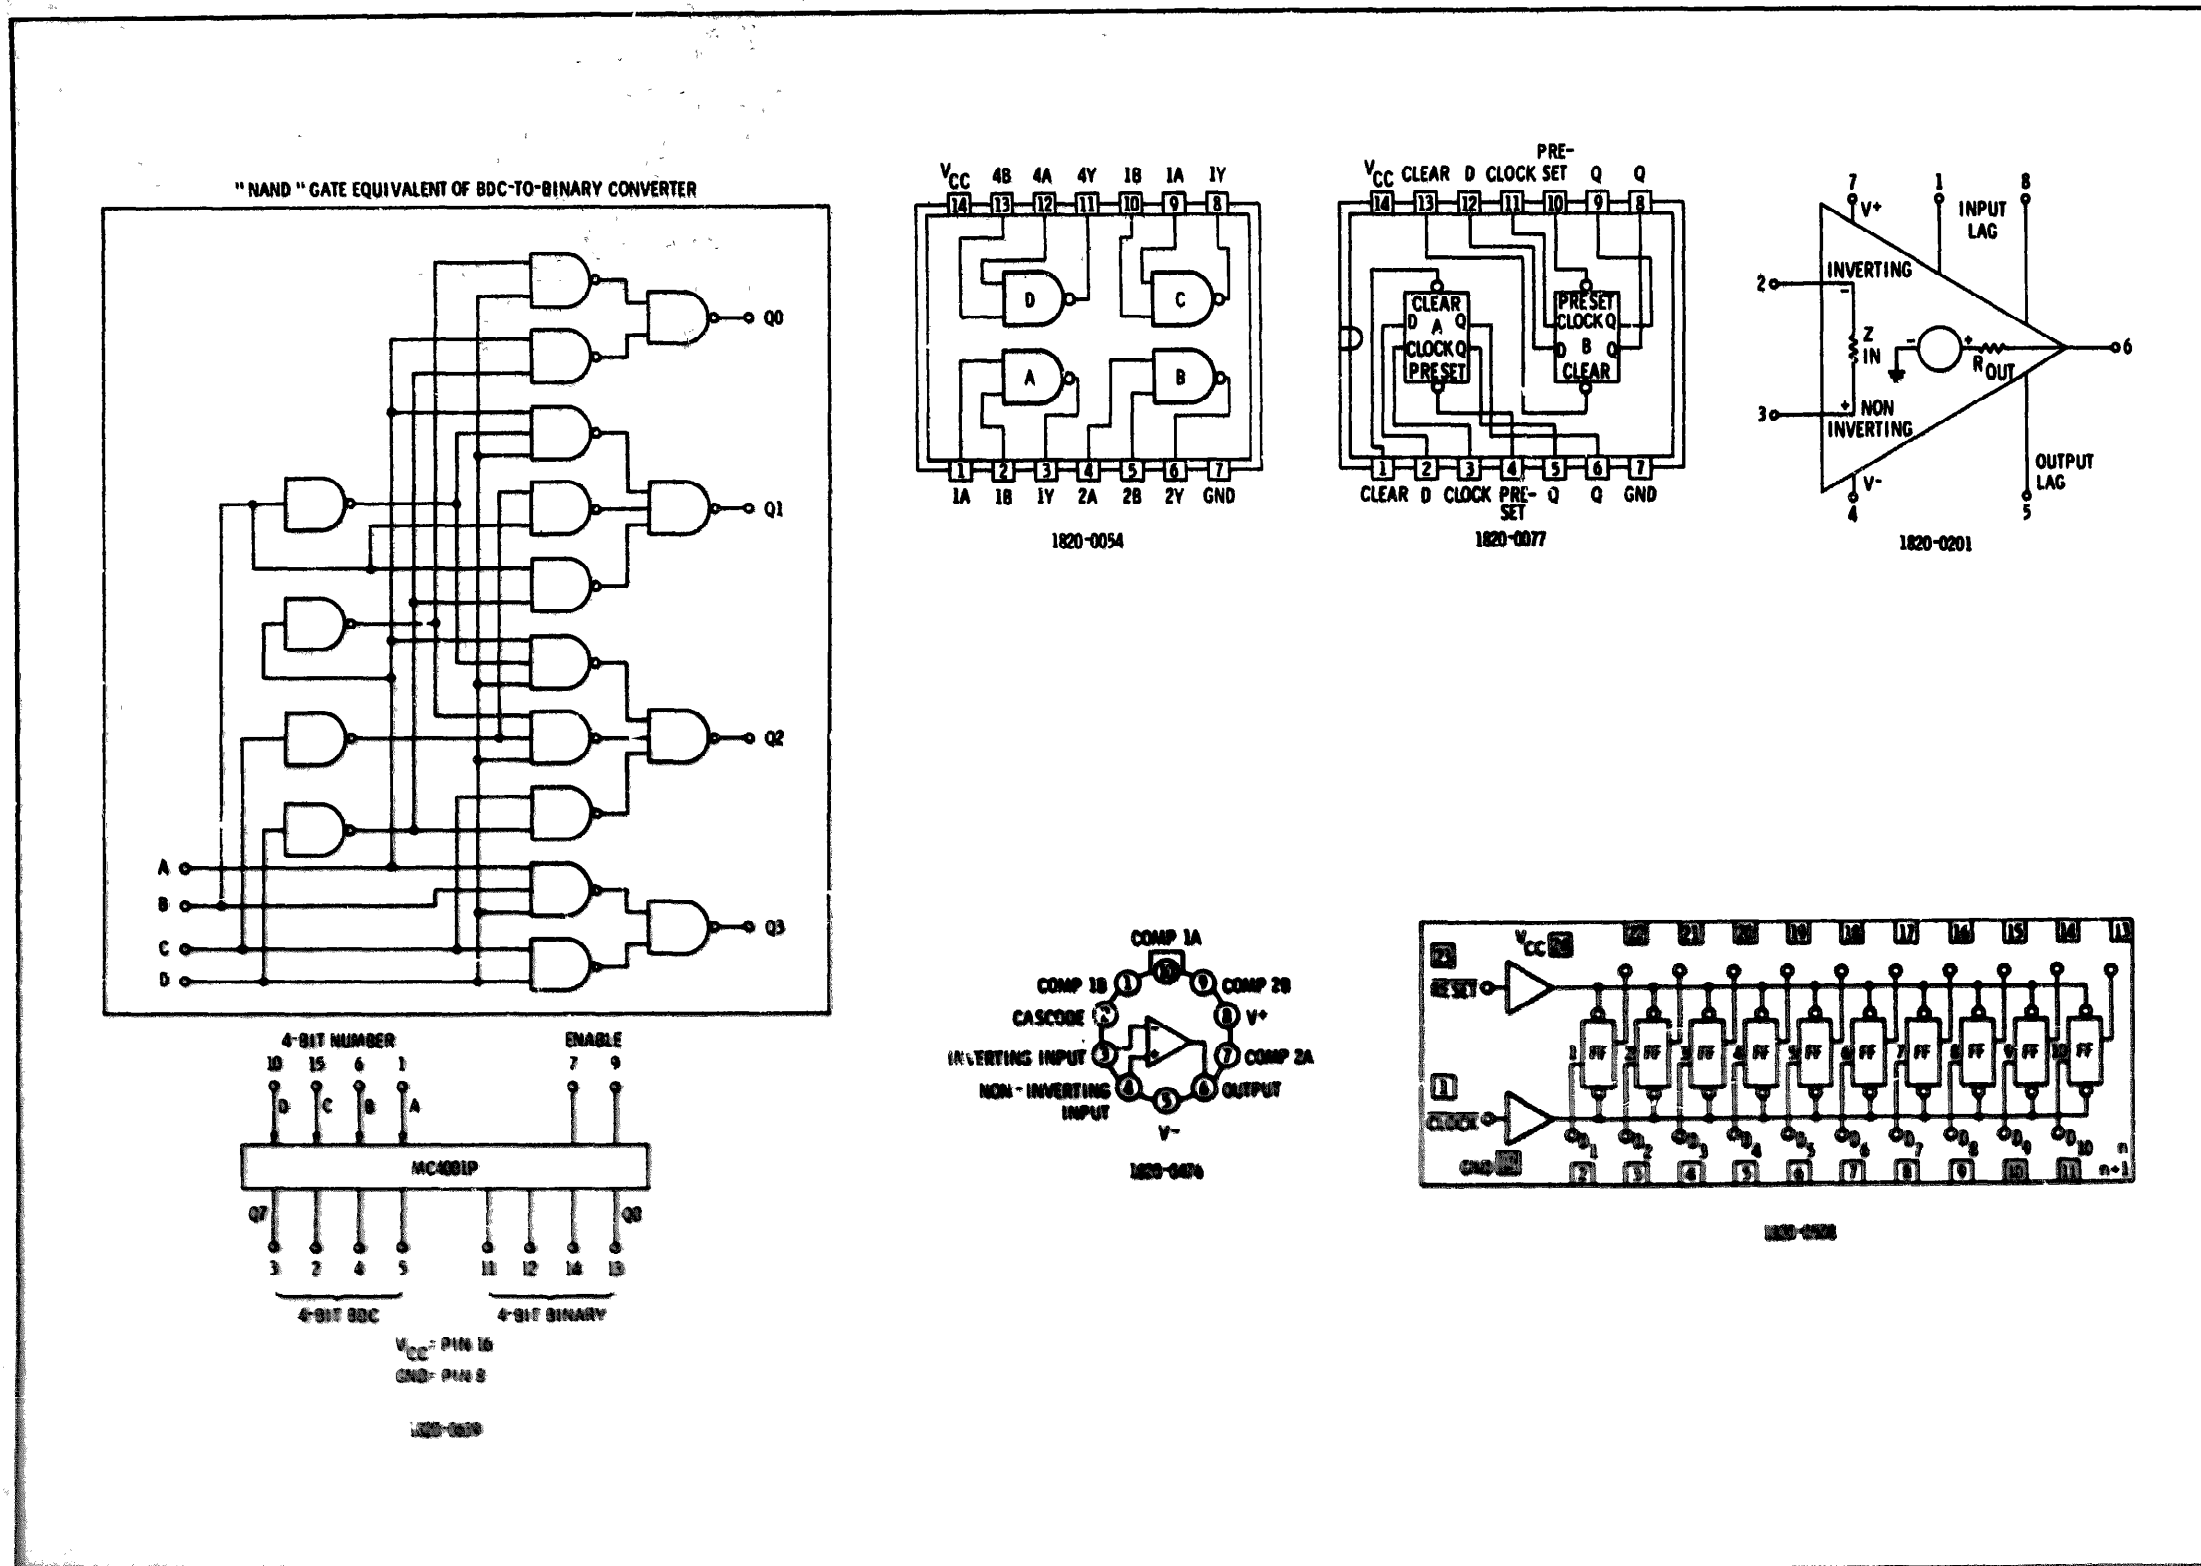
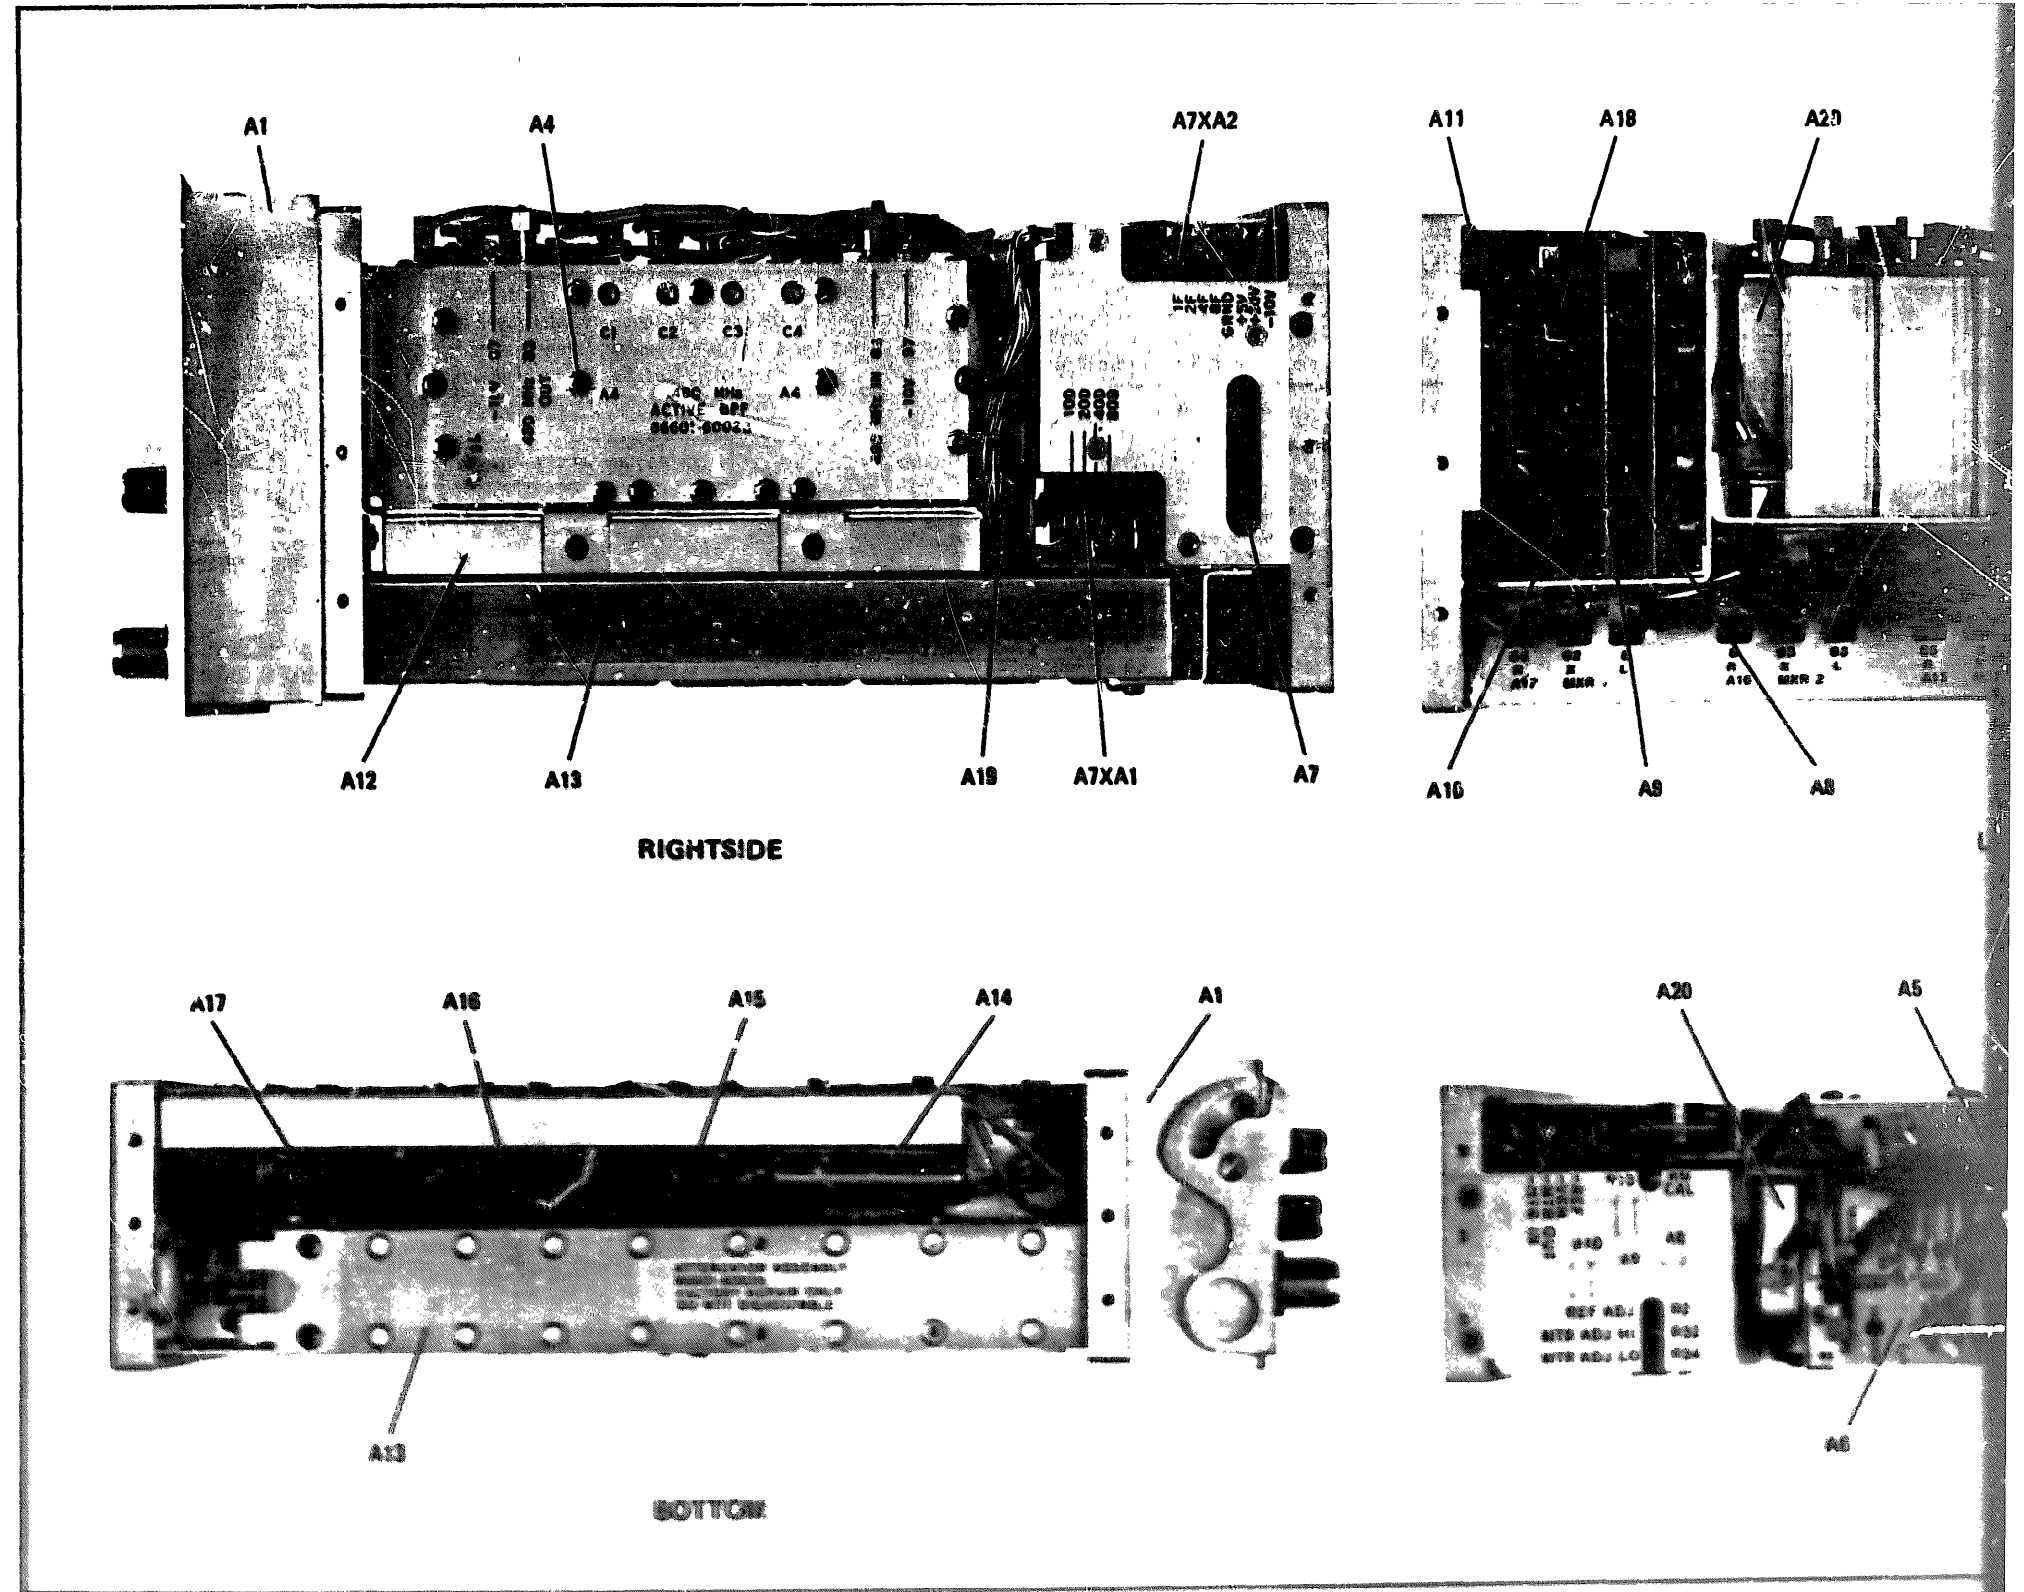


Figure 8-5. Integrated Circuits used in Model 86601A

Assy No. and Description	Service Sheet
A1 Front Housing	
A2 Power Amplifier	3
A3 Feedback Amplifier	4
A4 480 MHz Bandpass Filter	2
A5 Modulator Assembly	2
A6 Preamplifier	3
A7 Mother Board	2
A8 Attenuator Driver	6
A9 Reference Assembly	4
A10 Logic Assembly	5
A11 Rear Connector Assembly	
A12 Dual Filter	2
A13 Programmable Attenuator	6
A15 Mixer III	2
A16 Mixer II	2
A17 Mixer I	2
A18 Wiring Harness	
A19 Wiring Harness	
A20 Filter	

Table 5-8. Assembly Locations

Assy No. and Description	Service Sheet	Photo Figure 8-2
A1 Front Housing		6, 21
A2 Power Amplifier	3	6, 19
A3 Feedback Amplifier	4	6, 22
A4 480 MH. Bandpass Filter	2	6, 13
A5 Modulator Assembly	2	6, 16
A6 Preamp:ifier	3	6, 18
A7 Mother Board	2	6, 10
A8 Attenuator Driver	6	6, 27
A9 Reference Assembly	4	6, 23
A10 Logic Assembly	5	6, 25
A11 Rear Connector Assembly		1
A12 Dual Filter	2	6, 15
A13 Programmable Attenuator	6	8
A15 Mixer III	2	6
A16 Mixer II	2	6
A17 Mixer I	2	6
A18 Wiring Harness		6
A19 Wiring Harness		6
A20 Filter		6, 14






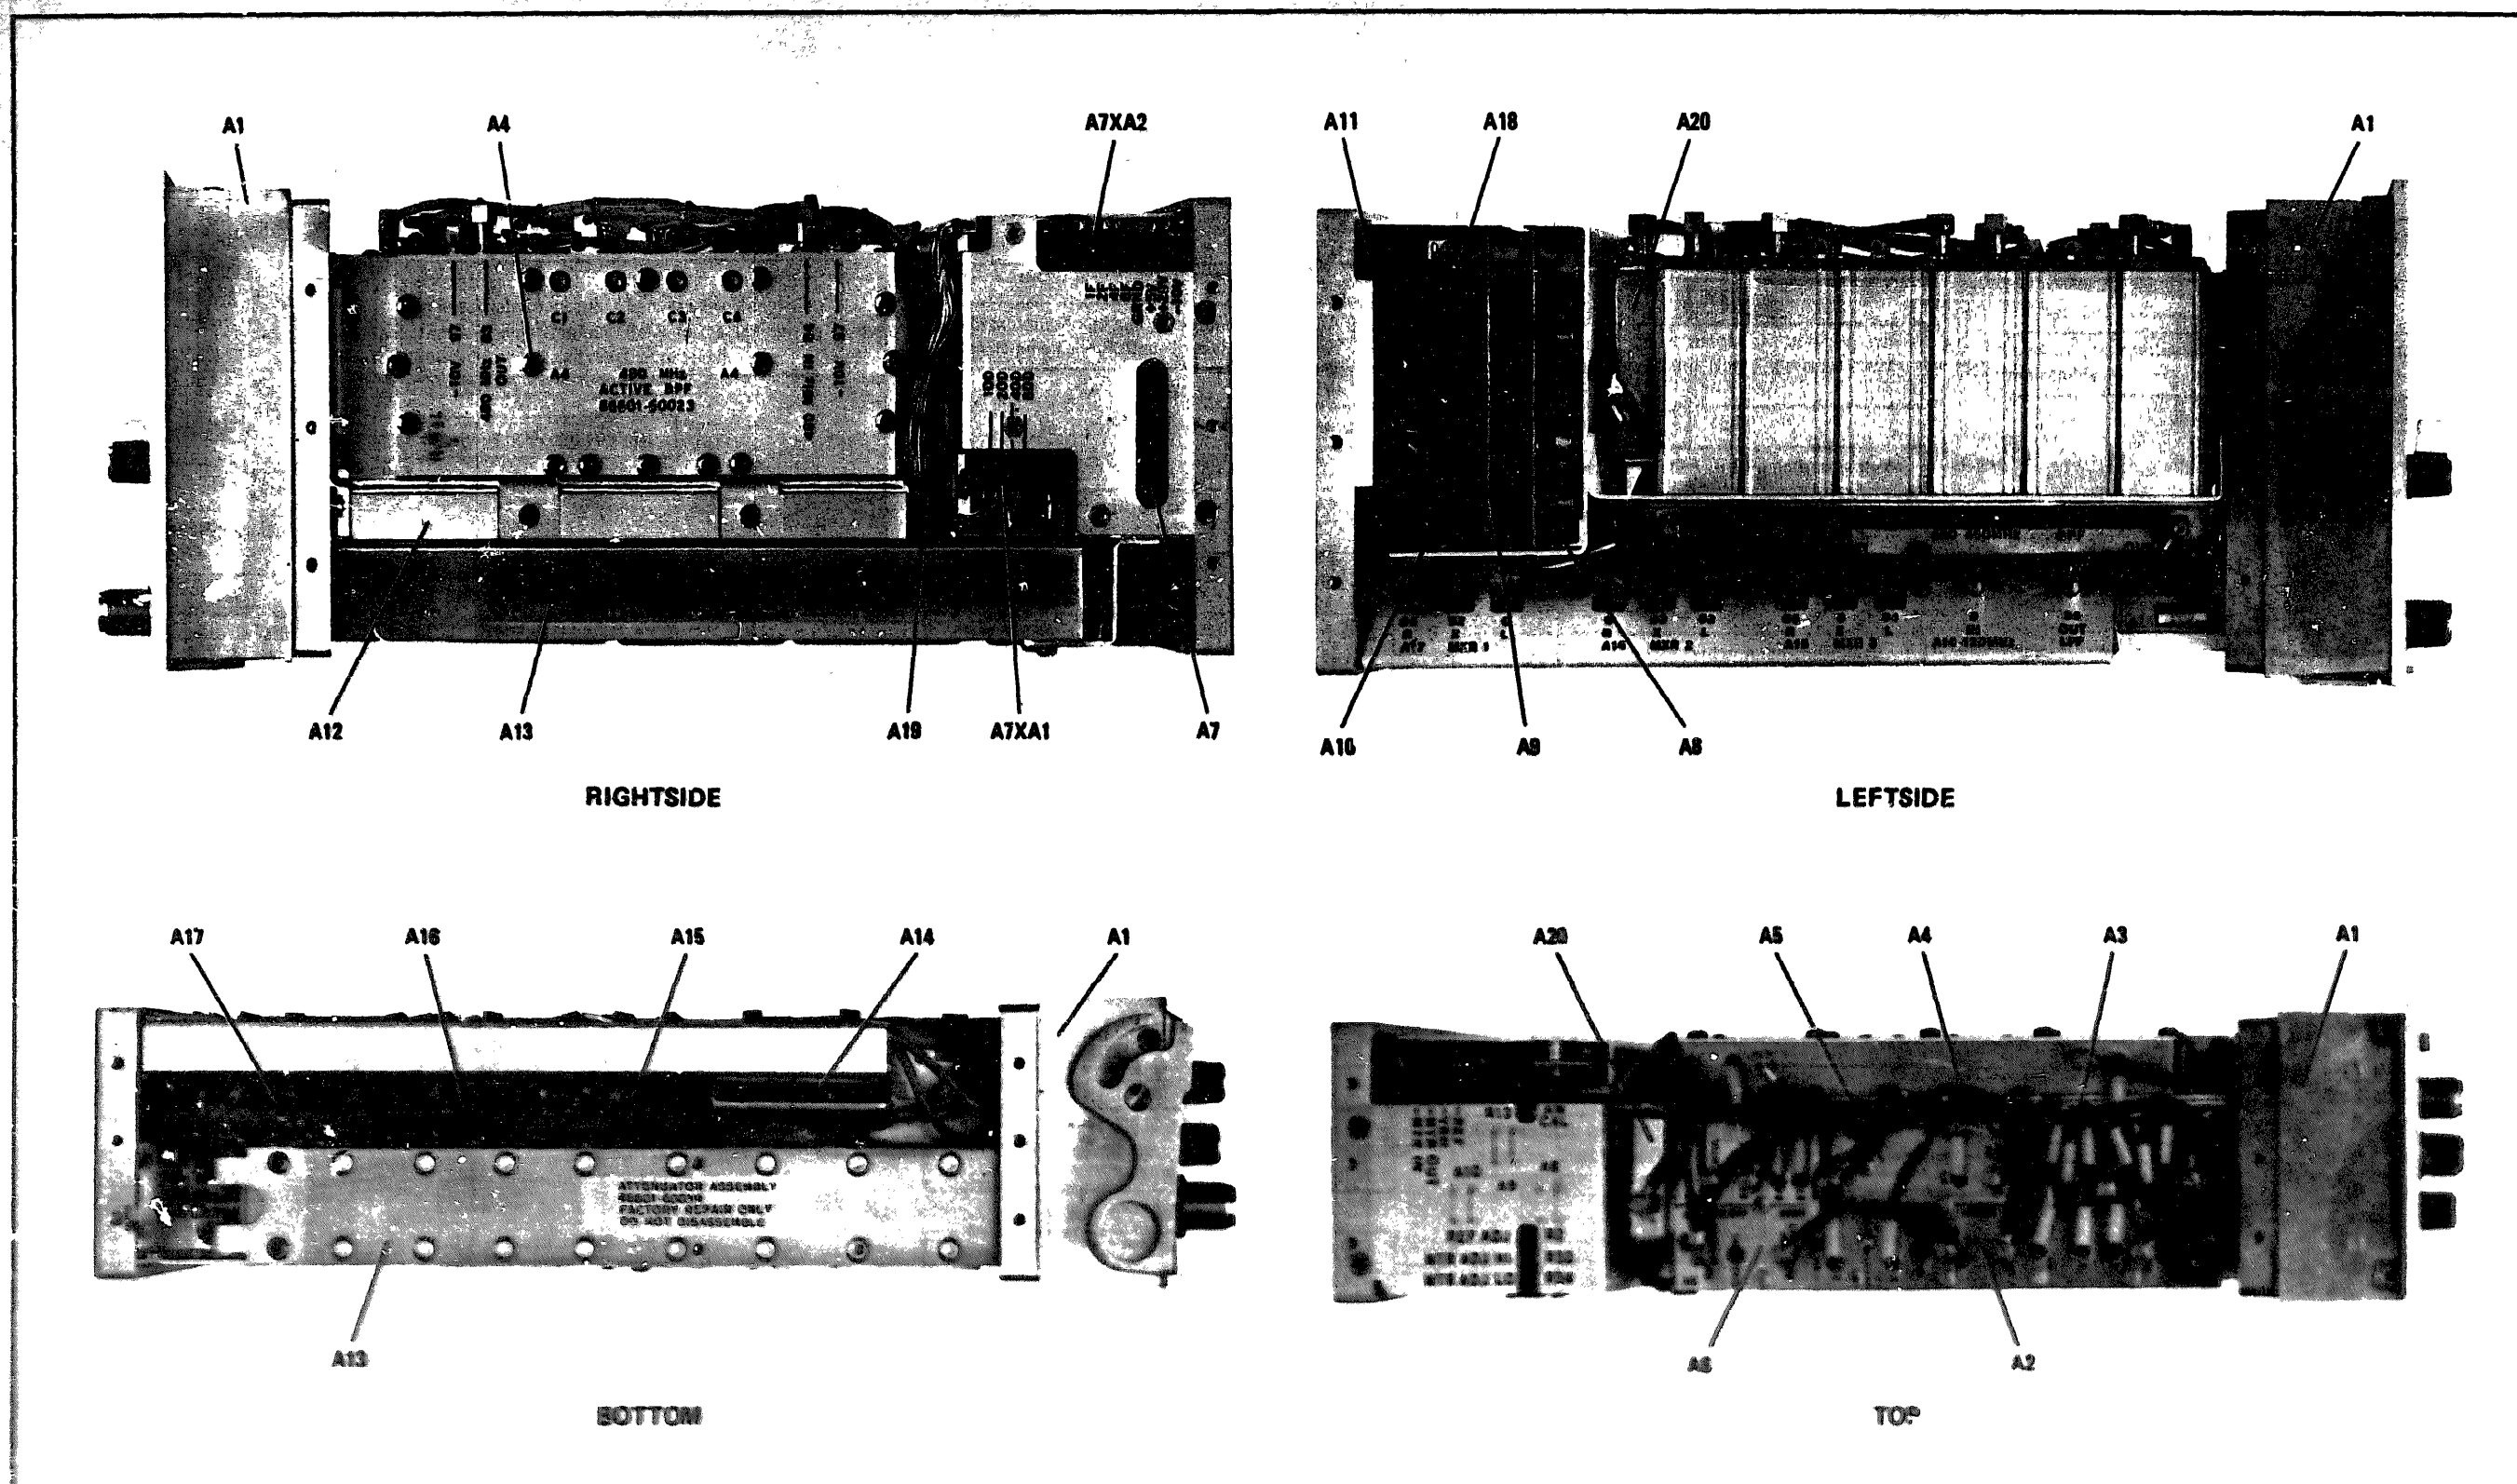


Figure 8-6. Chassis Mounted Parts and Assembly Locations

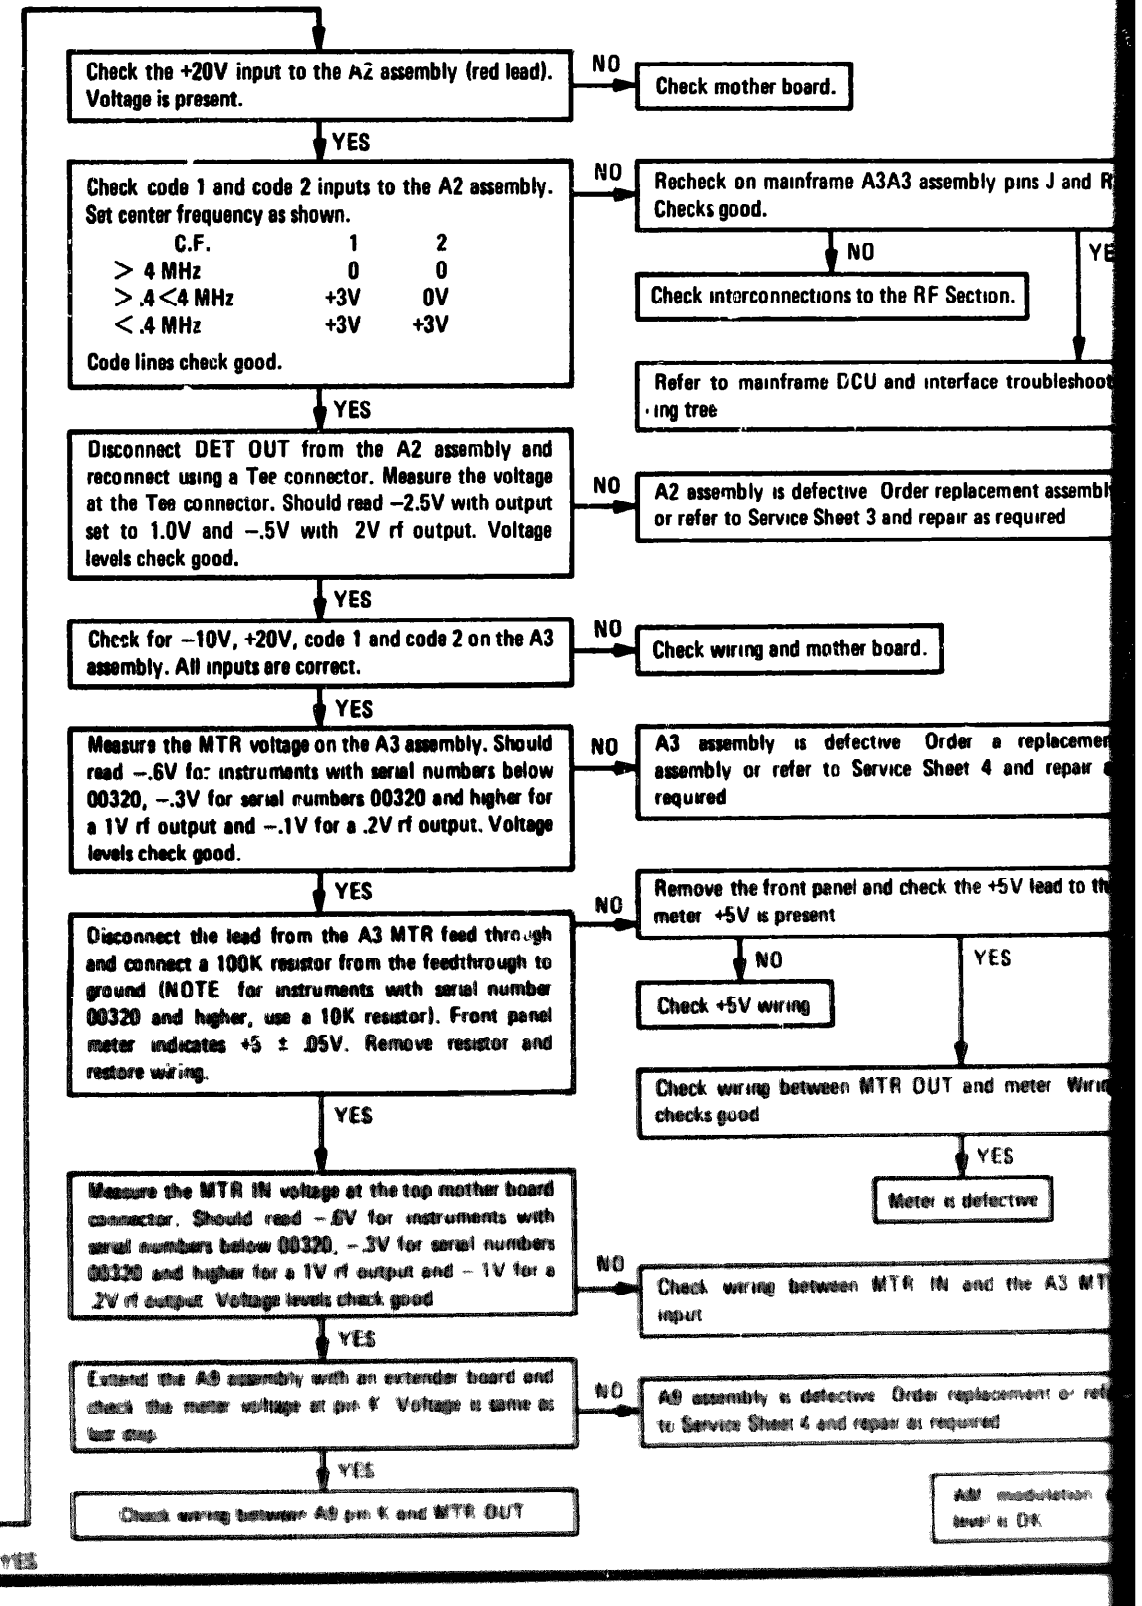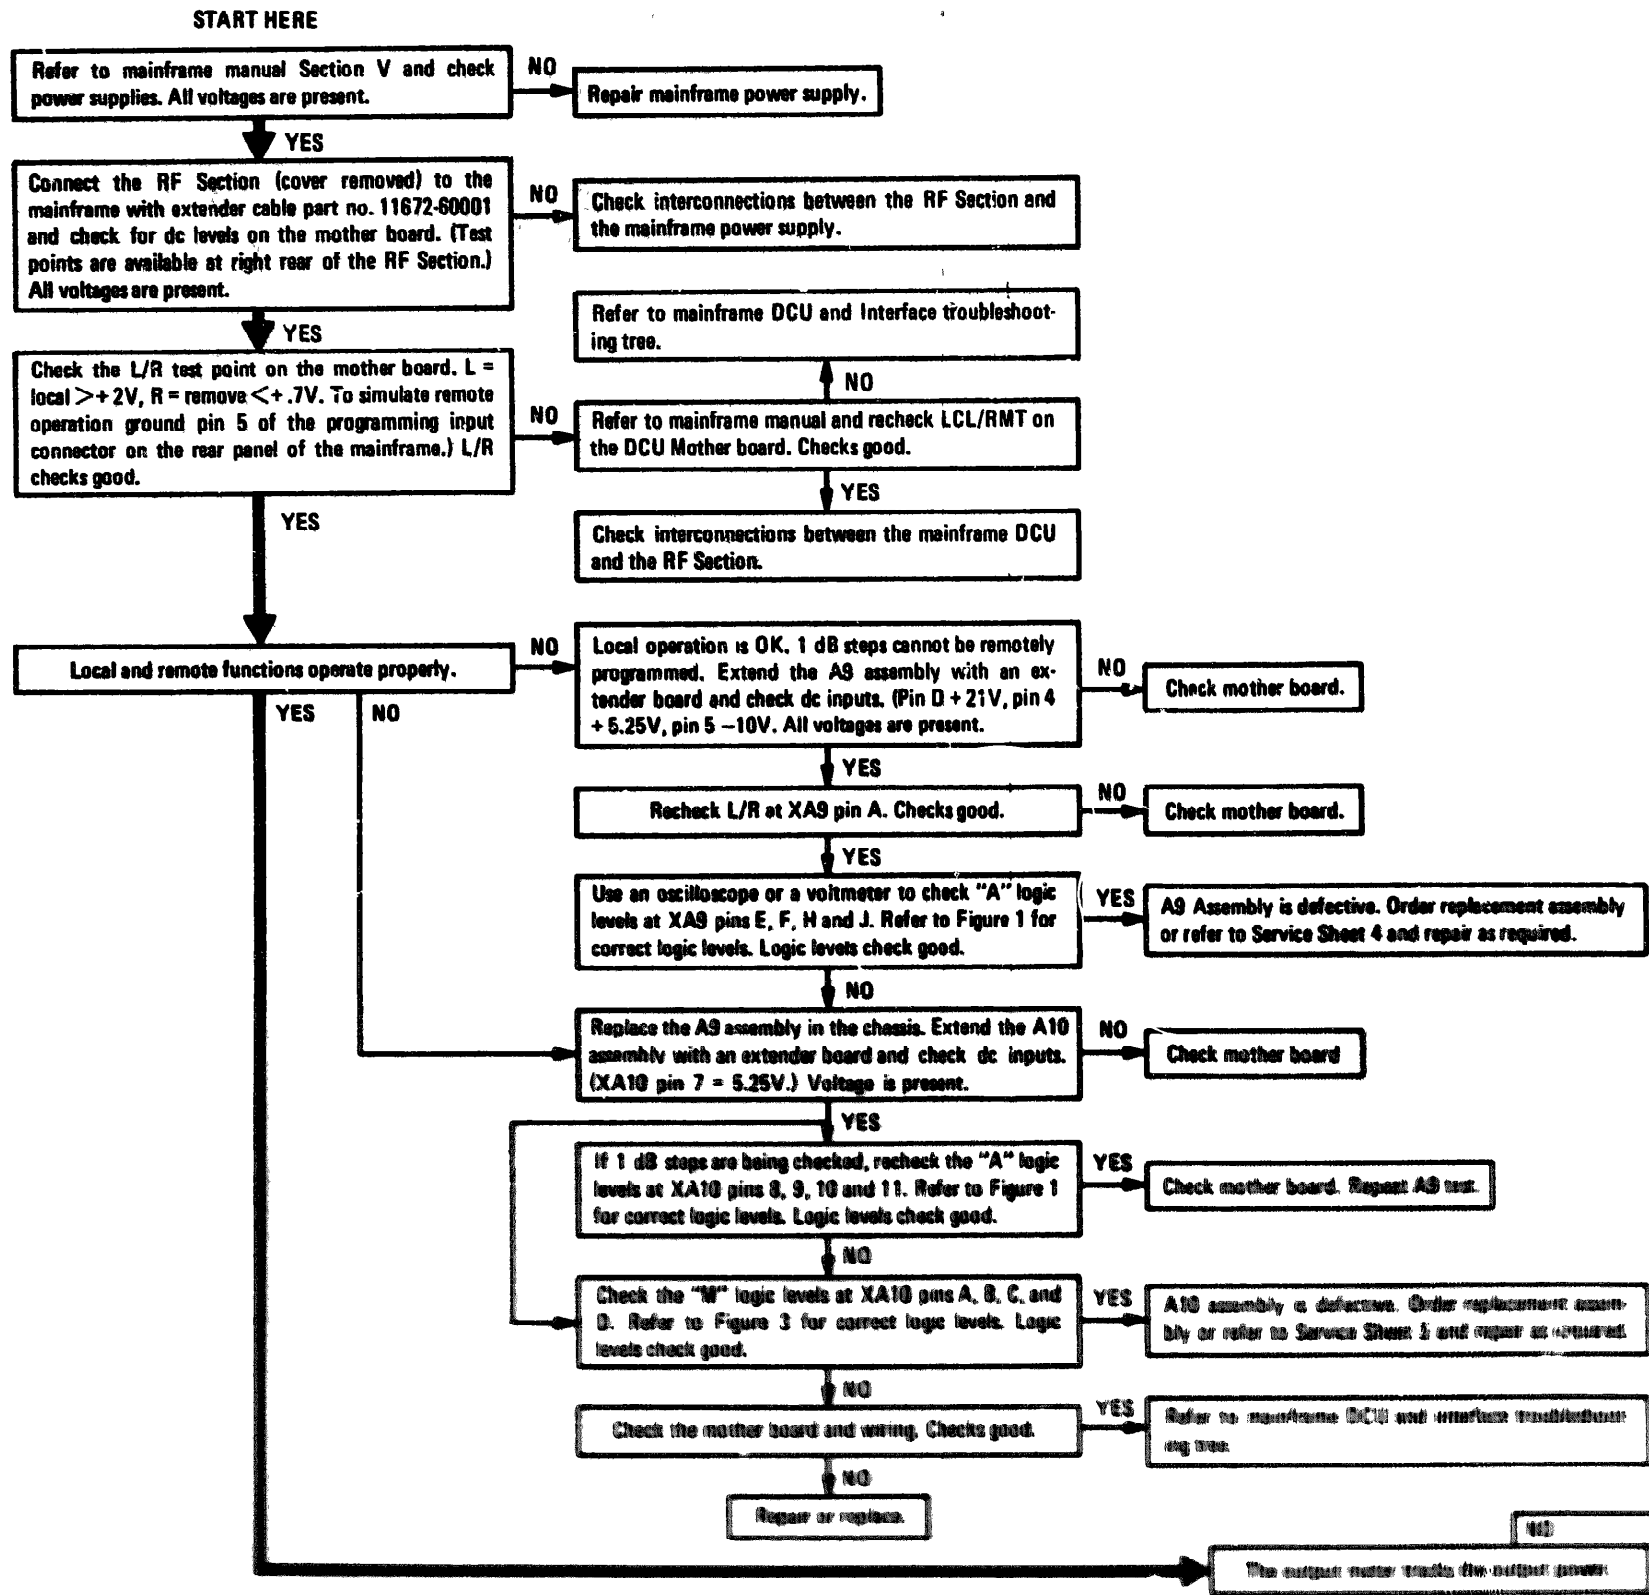

Code lines check good.

C.F.	1	2
> 4 MHz	0	0
> .4 < 4 MHz	+3V	0V
< .4 MHz	+3V	+3V

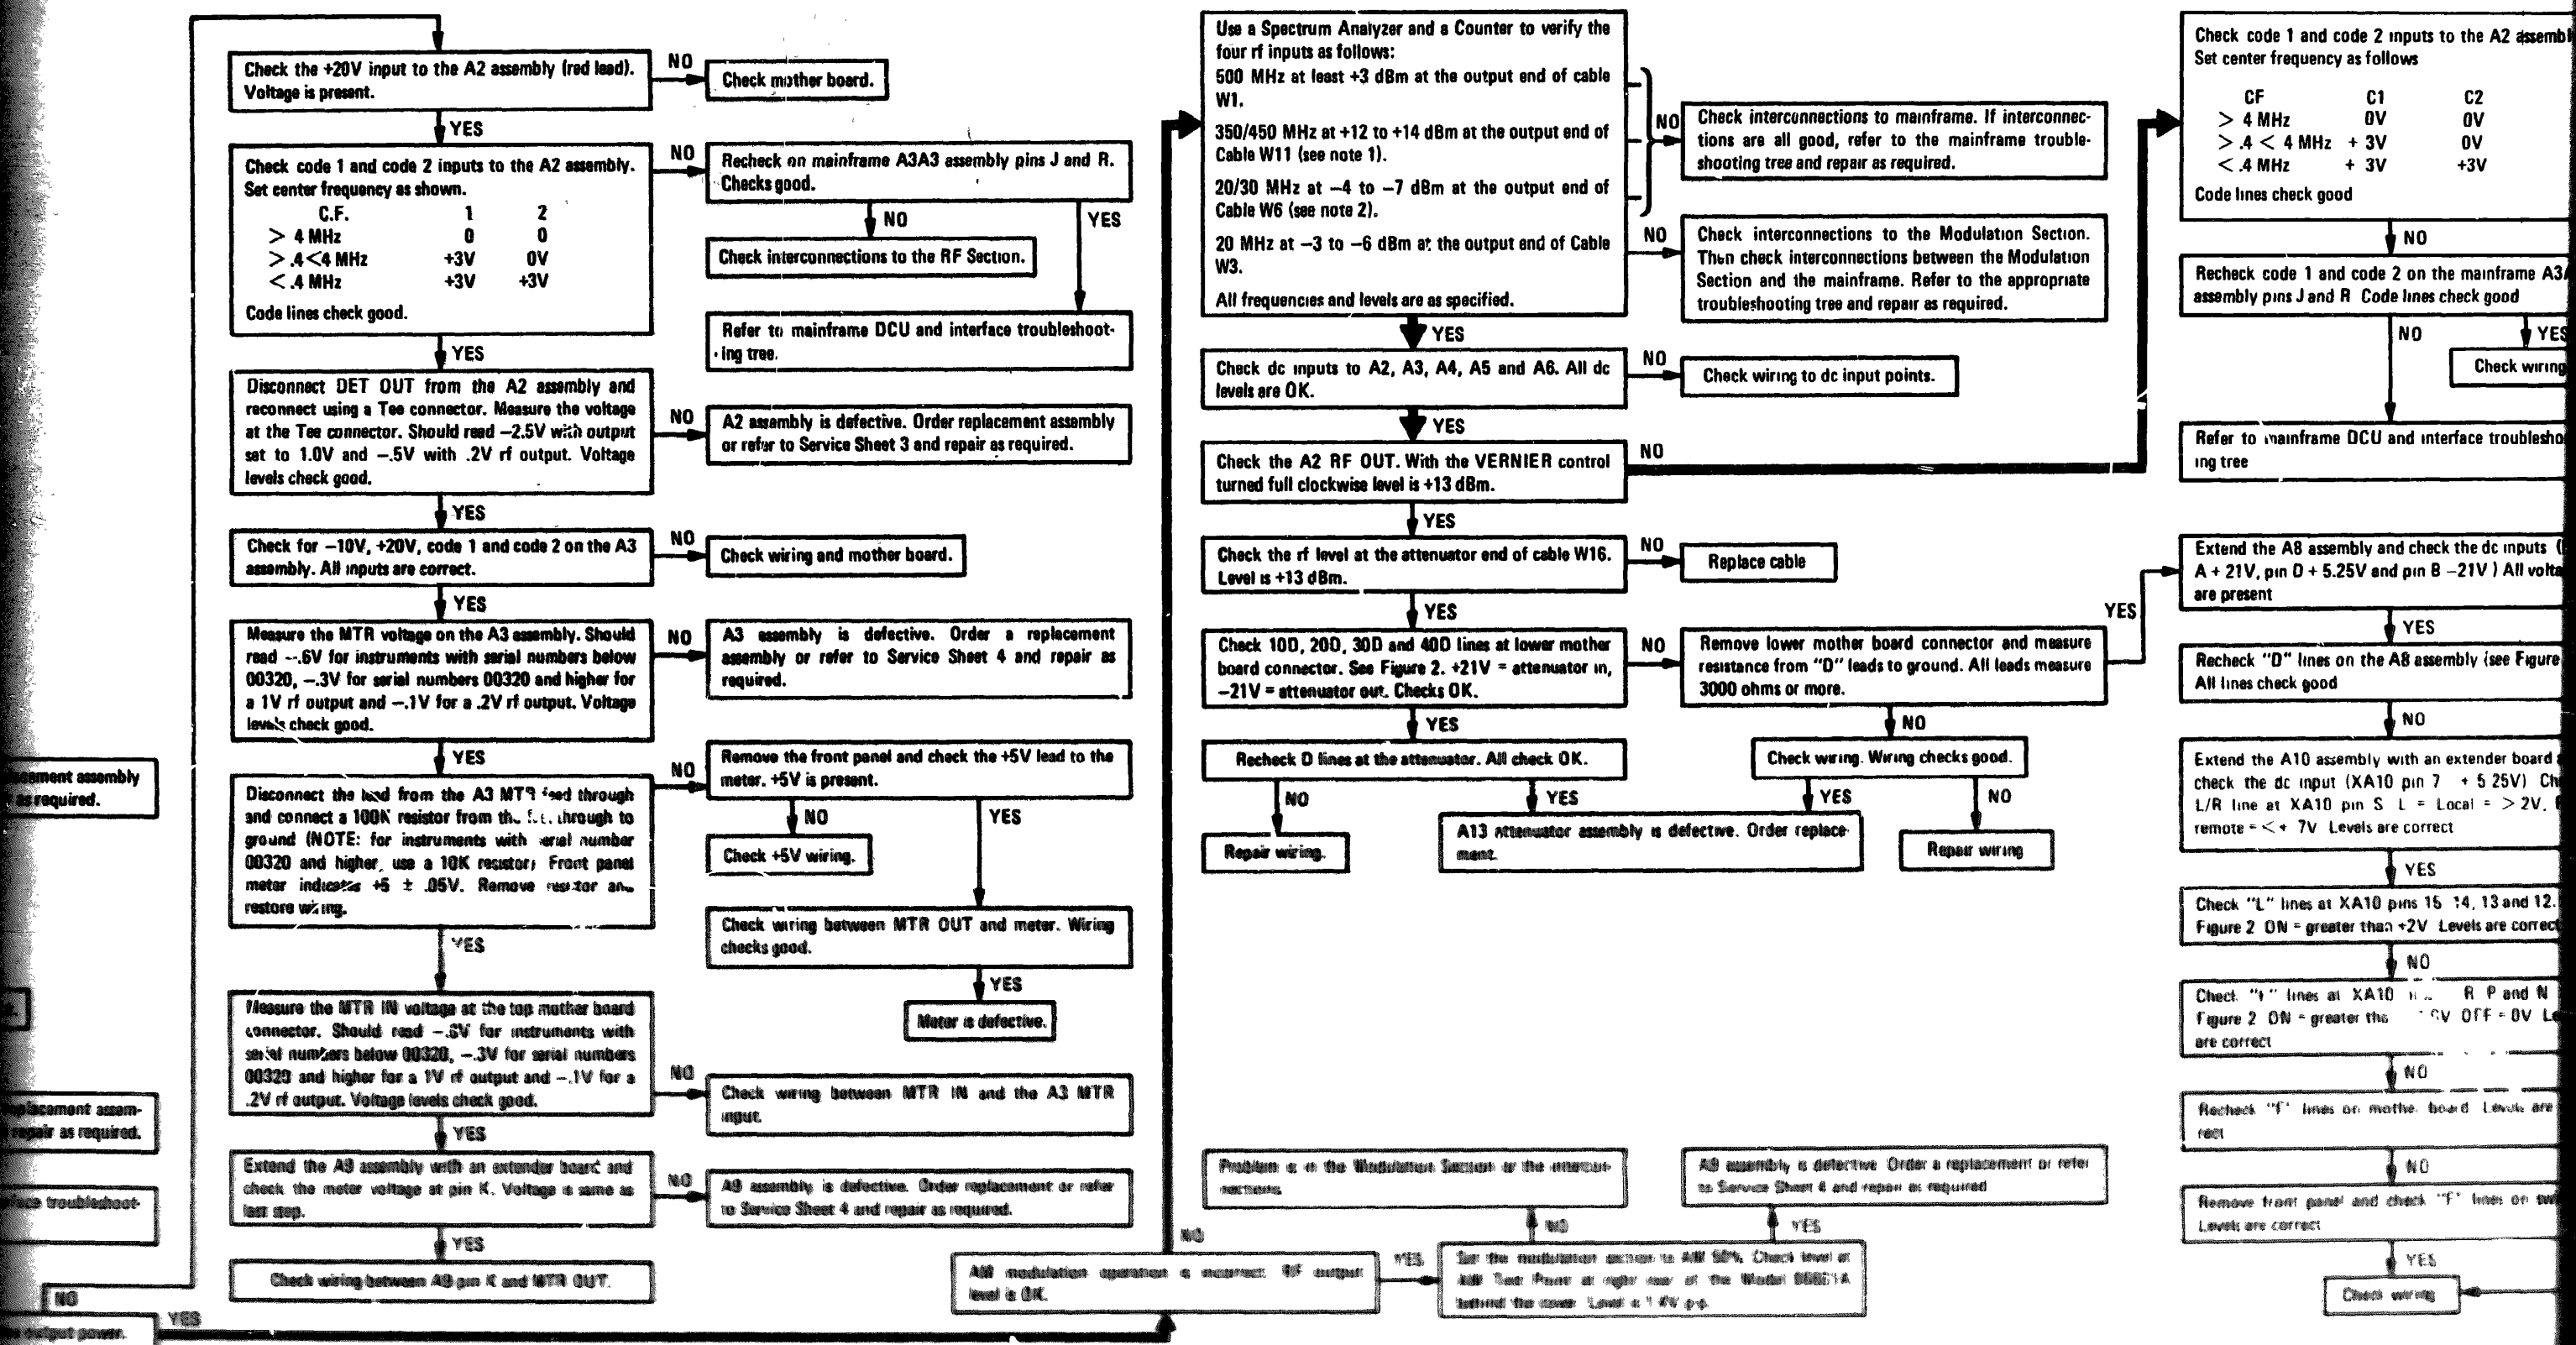

Check the +20V input to the A2 assembly (red lead). Voltage is present.

Check code 1 and code 2 inputs to the A2 assembly. Set center frequency as shown.

C.F.	1	2
> 4 MHz	0	0
> .4 < 4 MHz	+3V	0V
< .4 MHz	+3V	+3V

Code lines check good.

Disconnect DET OUT from the A2 assembly and reconnect using a Tee connector. Measure the voltage at the Tee connector. Should read -2.5V with output set to 1.0V and -5V with .2V rf output. Voltage levels check good.

Check for -10V, +20V, code 1 and code 2 on the A3 assembly. All inputs are correct.

Measure the MTR voltage on the A3 assembly. Should read -.6V for instruments with serial numbers below 00320, -.3V for serial numbers 00320 and higher for a 1V rf output and -.1V for a .2V rf output. Voltage levels check good.

Disconnect the lead from the A3 MTR lead through and connect a 100K resistor from the f.c. through to ground (NOTE: for instruments with serial number 00320 and higher, use a 10K resistor; Front panel meter indicates +5 ± .05V. Remove resistor and restore wiring.

Measure the MTR IN voltage at the top mother board connector. Should read -.6V for instruments with serial numbers below 00320, -.3V for serial numbers 00320 and higher for a 1V rf output and -.1V for a .2V rf output. Voltage levels check good.

Extend the A9 assembly with an extender board and check the meter voltage at pin K. Voltage is same as last step.

Check wiring between A9 pin K and MTR OUT.

Check mother board.

Recheck on mainframe A3A3 assembly pins J and R. Checks good.

Check interconnections to the RF Section.

Refer to mainframe DCU and interface troubleshooting tree.

A2 assembly is defective. Order replacement assembly or refer to Service Sheet 3 and repair as required.

Check wiring and mother board.

A3 assembly is defective. Order a replacement assembly or refer to Service Sheet 4 and repair as required.

Remove the front panel and check the +5V lead to the meter. +5V is present.

Check +5V wiring.

Check wiring between MTR OUT and meter. Wiring checks good.

Motor is defective.

Check wiring between MTR IN and the A3 MTR input.

A9 assembly is defective. Order replacement or refer to Service Sheet 4 and repair as required.

Use a Spectrum Analyzer and a Counter to verify the four rf inputs as follows:
 500 MHz at least +3 dBm at the output end of cable W1.
 350/450 MHz at +12 to +14 dBm at the output end of Cable W11 (see note 1).
 20/30 MHz at -4 to -7 dBm at the output end of Cable W6 (see note 2).
 20 MHz at -3 to -6 dBm at the output end of Cable W3.
 All frequencies and levels are as specified.

Check dc inputs to A2, A3, A4, A5 and A6. All dc levels are OK.

Check the A2 RF OUT. With the VERNIER control turned full clockwise level is +13 dBm.

Check the rf level at the attenuator end of cable W16. Level is +13 dBm.

Check 10D, 20D, 30D and 40D lines at lower mother board connector. See Figure 2. +21V = attenuator in, -21V = attenuator out. Checks OK.

Recheck D lines at the attenuator. All check OK.

Repair wiring.

A13 attenuator assembly is defective. Order replacement.

Repair wiring.

Problem is in the Modulation Section or the interconnections.

A8 assembly is defective. Order a replacement or refer to Service Sheet 4 and repair as required.

Set the modulation section to AM 50%. Check level at AM Test Point at right side of the Model 88821A behind the cover. Level is 1.4V p-p.

Check code 1 and code 2 inputs to the A2 assembly. Set center frequency as follows:

CF	C1	C2
> 4 MHz	0V	0V
> .4 < 4 MHz	+3V	0V
< .4 MHz	+3V	+3V

Code lines check good

Recheck code 1 and code 2 on the mainframe A3 assembly pins J and R. Code lines check good

Check wiring

Refer to mainframe DCU and interface troubleshooting tree

Extend the A8 assembly and check the dc inputs (A + 21V, pin D + 5.25V and pin B - 21V). All voltages are present

Recheck "D" lines on the A8 assembly (see Figure 2). All lines check good

Extend the A10 assembly with an extender board and check the dc input (XA10 pin 7 + 5.25V). Check L/R line at XA10 pin 5. L = Local = > 2V, remote = < + 7V. Levels are correct

Check "L" lines at XA10 pins 15, 14, 13 and 12. Figure 2 ON = greater than +2V. Levels are correct

Check "I" lines at XA10 pins R, P and N. Figure 2 ON = greater than 1.0V. OFF = 0V. Levels are correct

Recheck "F" lines on mother board. Levels are correct

Remove front panel and check "F" lines on sub-assembly. Levels are correct

Check wiring


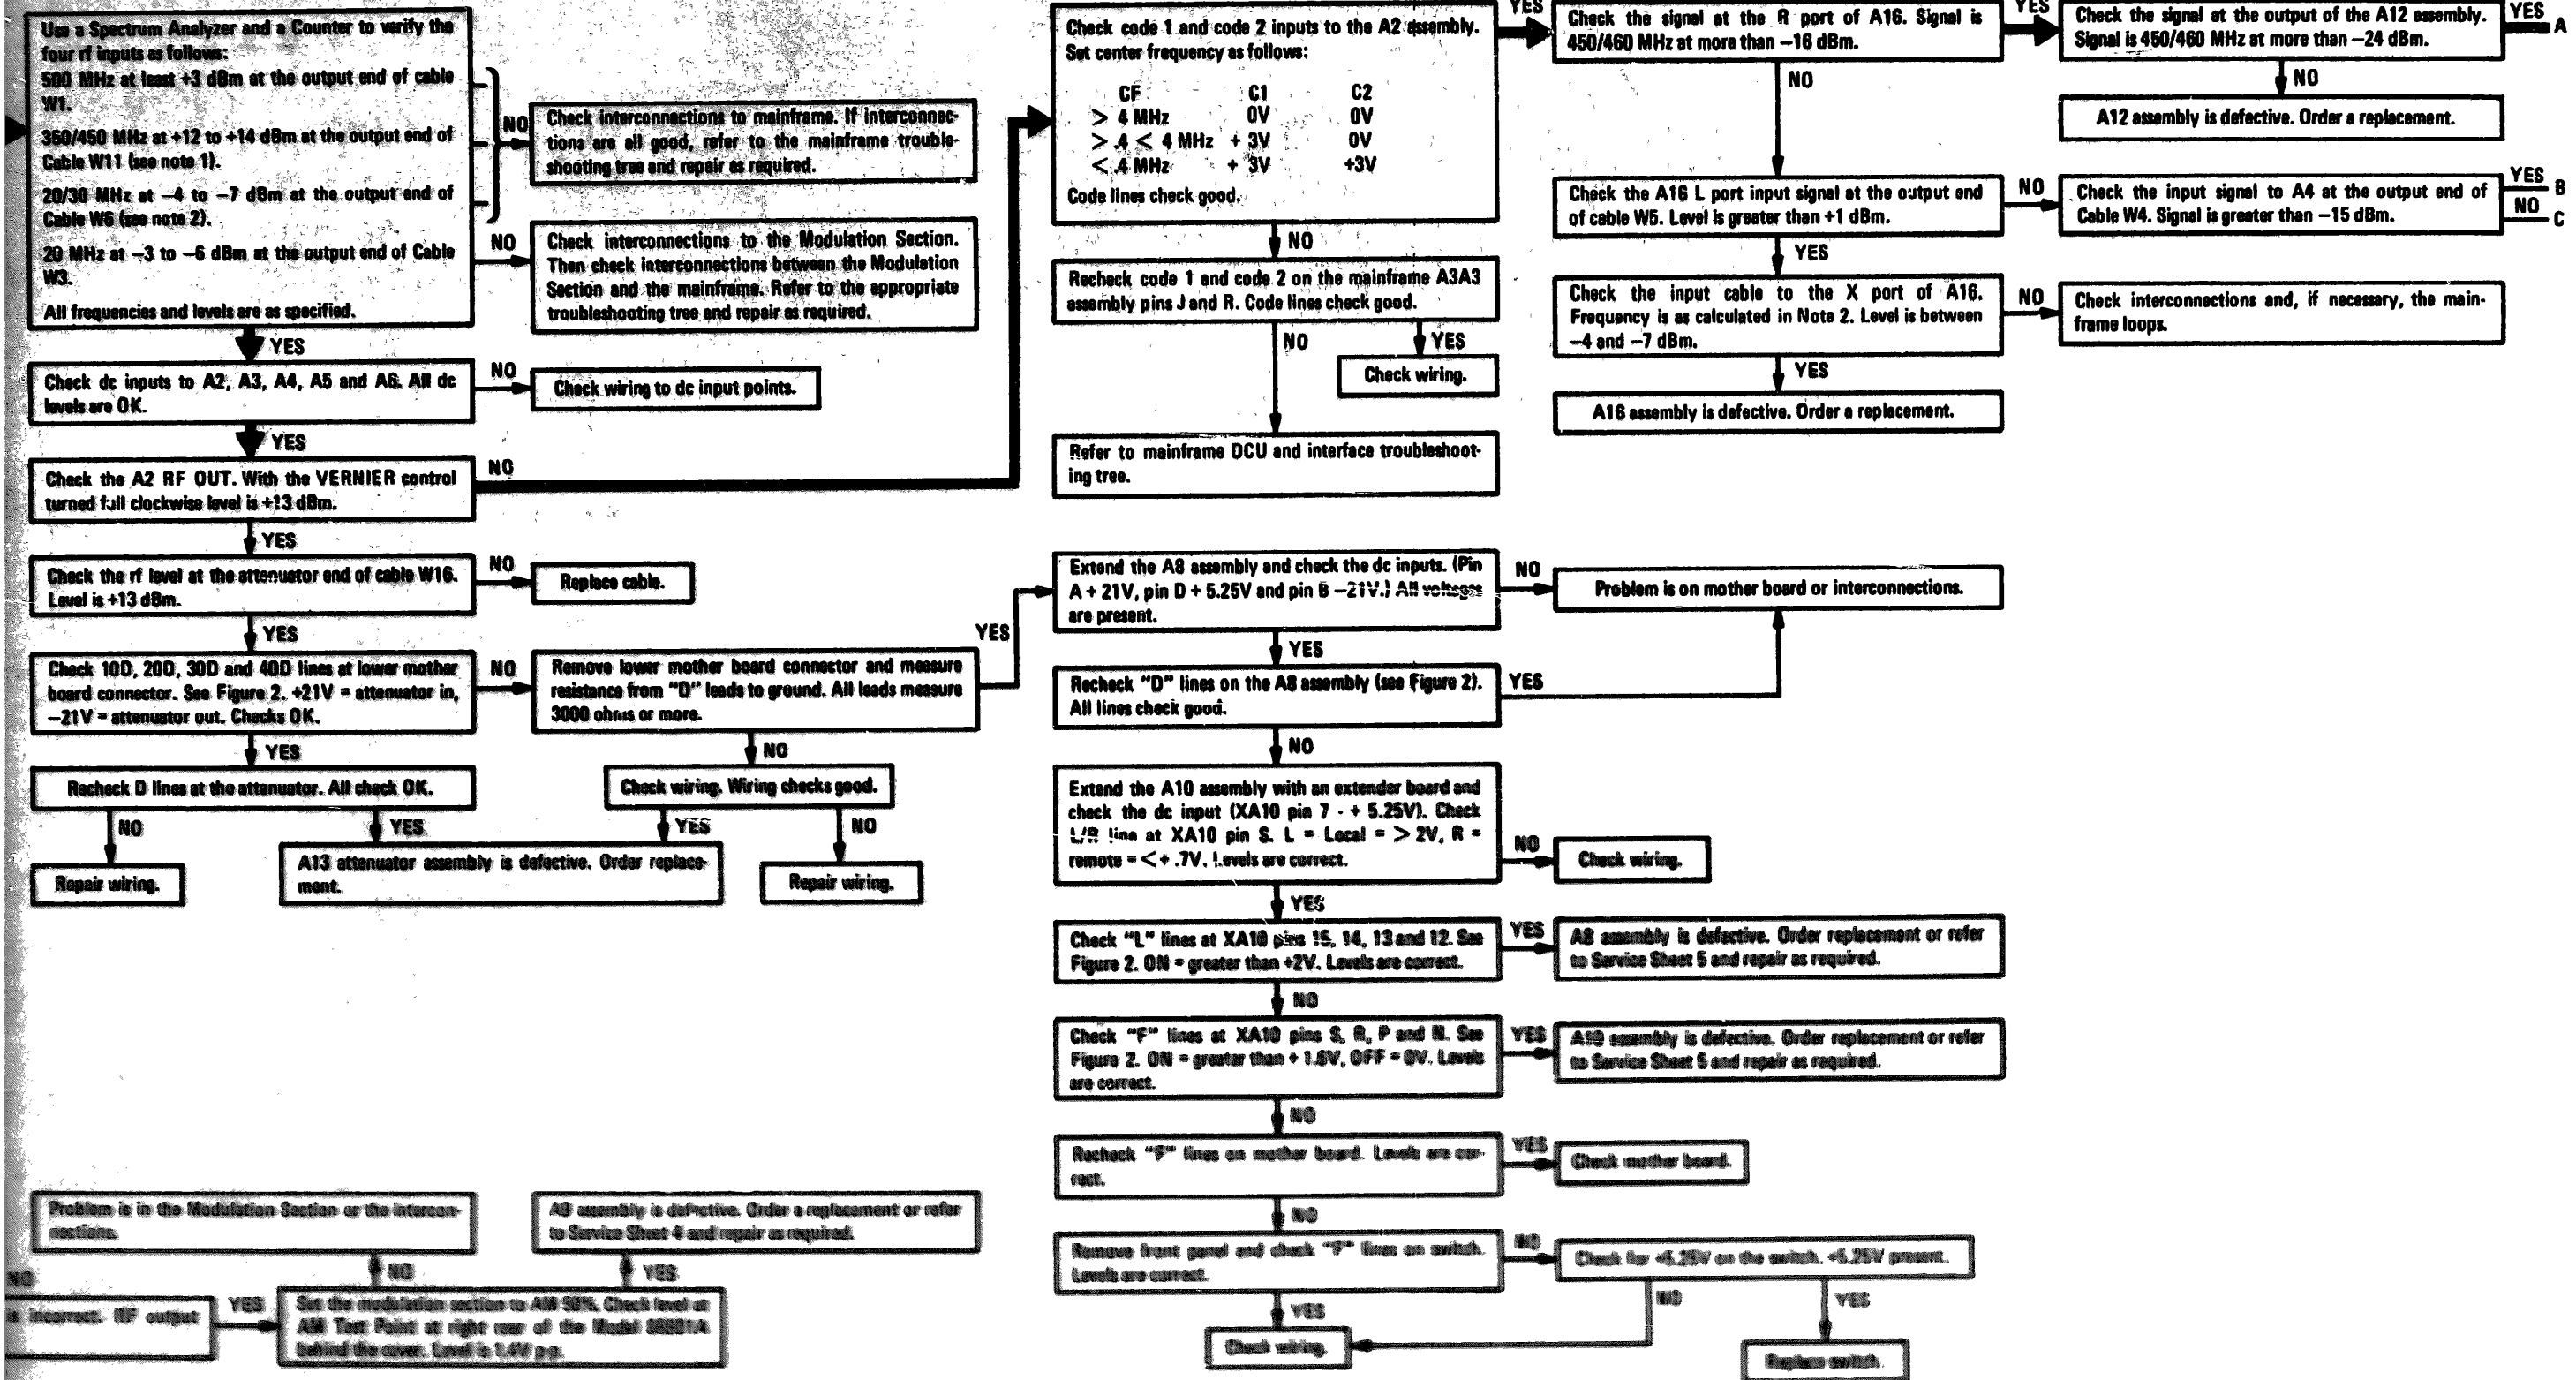


Figure 8-7. Model 86601A Troubleshooting Tree (1 of 2)

CONTINUED FROM SHEET 1

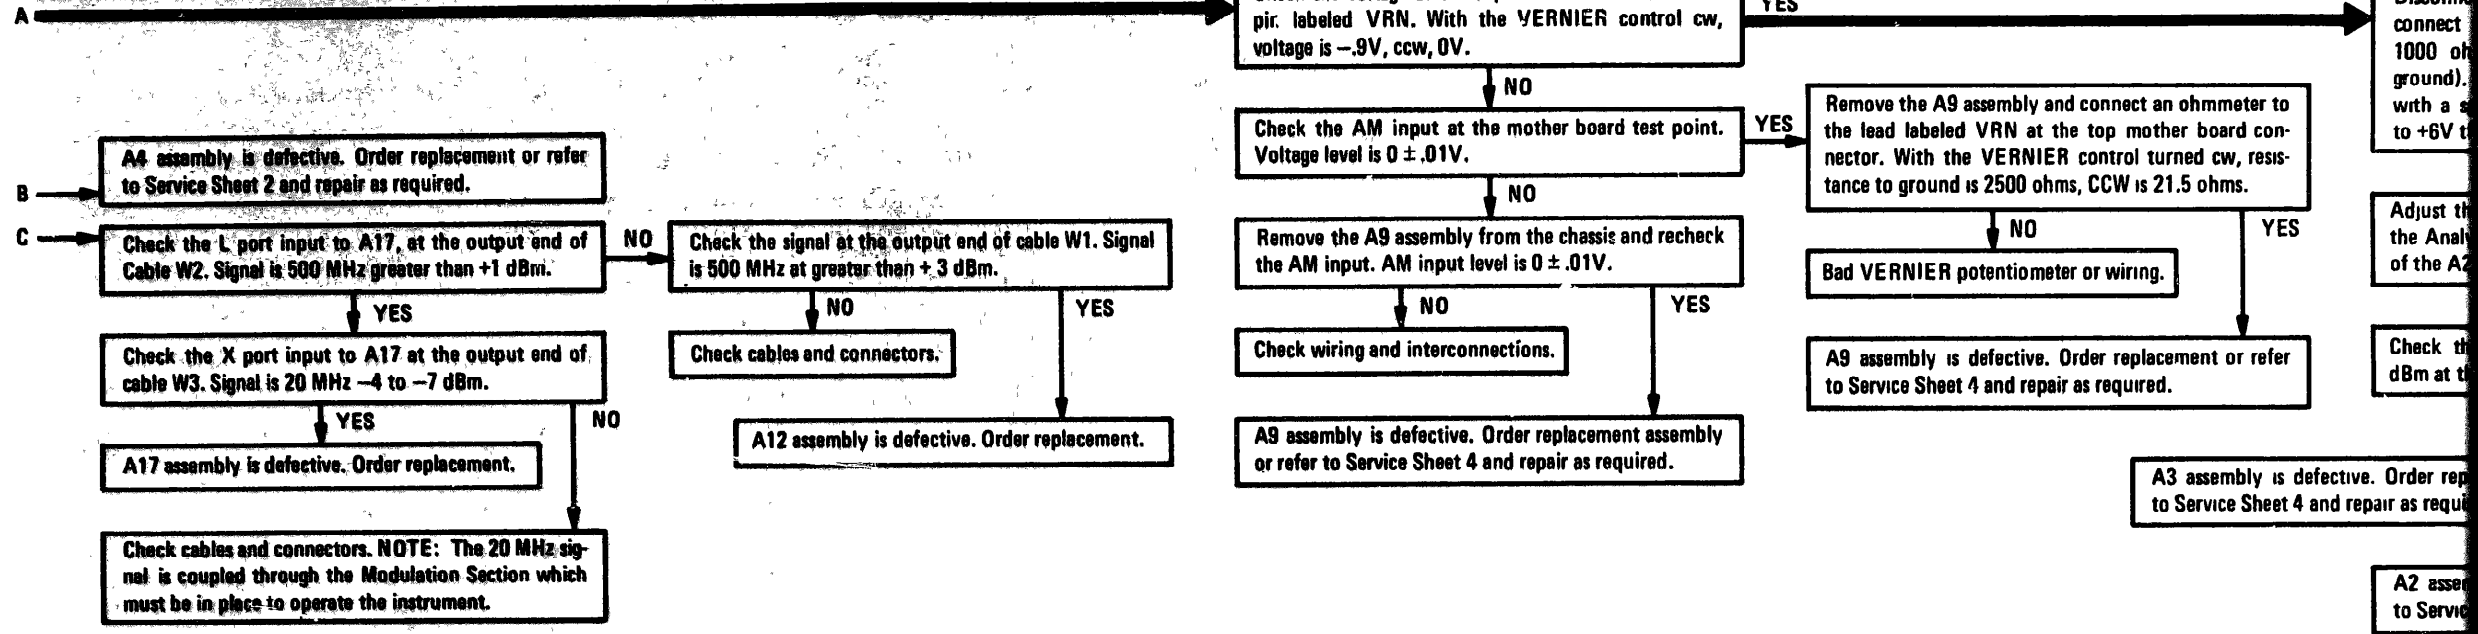

NOTE:

- The output frequency from the high frequency section in the mainframe can be determined by subtracting number 1 of digit 9 and digit 8 from 450 MHz. Example: programmed frequency is 70 MHz.

450 MHz
 70 MHz

 380 MHz

The output frequency is 380 MHz.

- The output frequency of the SL1 loop may be determined by subtracting the last 7 digits of the programmed frequency from 30.000000 MHz. Example: programmed frequency is 7.654321 MHz.

30.000000
 7.654321

SL1 frequency is 22.345679

Figure 1

"A" lines check.
 ON = >+2V OFF = <+.7V

1 dB atten steps	BCD	8	4	2	1
+3		0	0	0	0
+2		0	0	0	1
+1		0	0	1	0
0		0	0	1	1
-1		0	1	0	0
-2		0	1	0	1
-3		0	1	1	0
-4		0	1	1	1
-5		1	0	0	0
-6		1	0	0	1

Figure 2

"D" lines ON = +21V, OFF = -21V
 "L" lines ON = >+2V, OFF = <+.7V
 "F" lines ON = +1.6V, OFF = +.7V

10 dB atten steps	BCD	8	4	2	1
+10 dB		0	0	0	0
0		0	0	0	1
-10		0	0	1	0
-20		0	0	1	1
-30		0	1	0	0
-40		0	1	0	1
-50		0	1	1	0
-60		0	1	1	1
-70		1	0	0	0
-80		1	0	0	1
-90		1	0	1	0
-100		1	0	1	1
-110		1	1	0	0
-120		1	1	0	1
-130		1	1	1	0
-140		1	1	1	1

Figure 3

"M" lines check.
 ON = >+2V, OFF = <+.7V

the
with

See
See

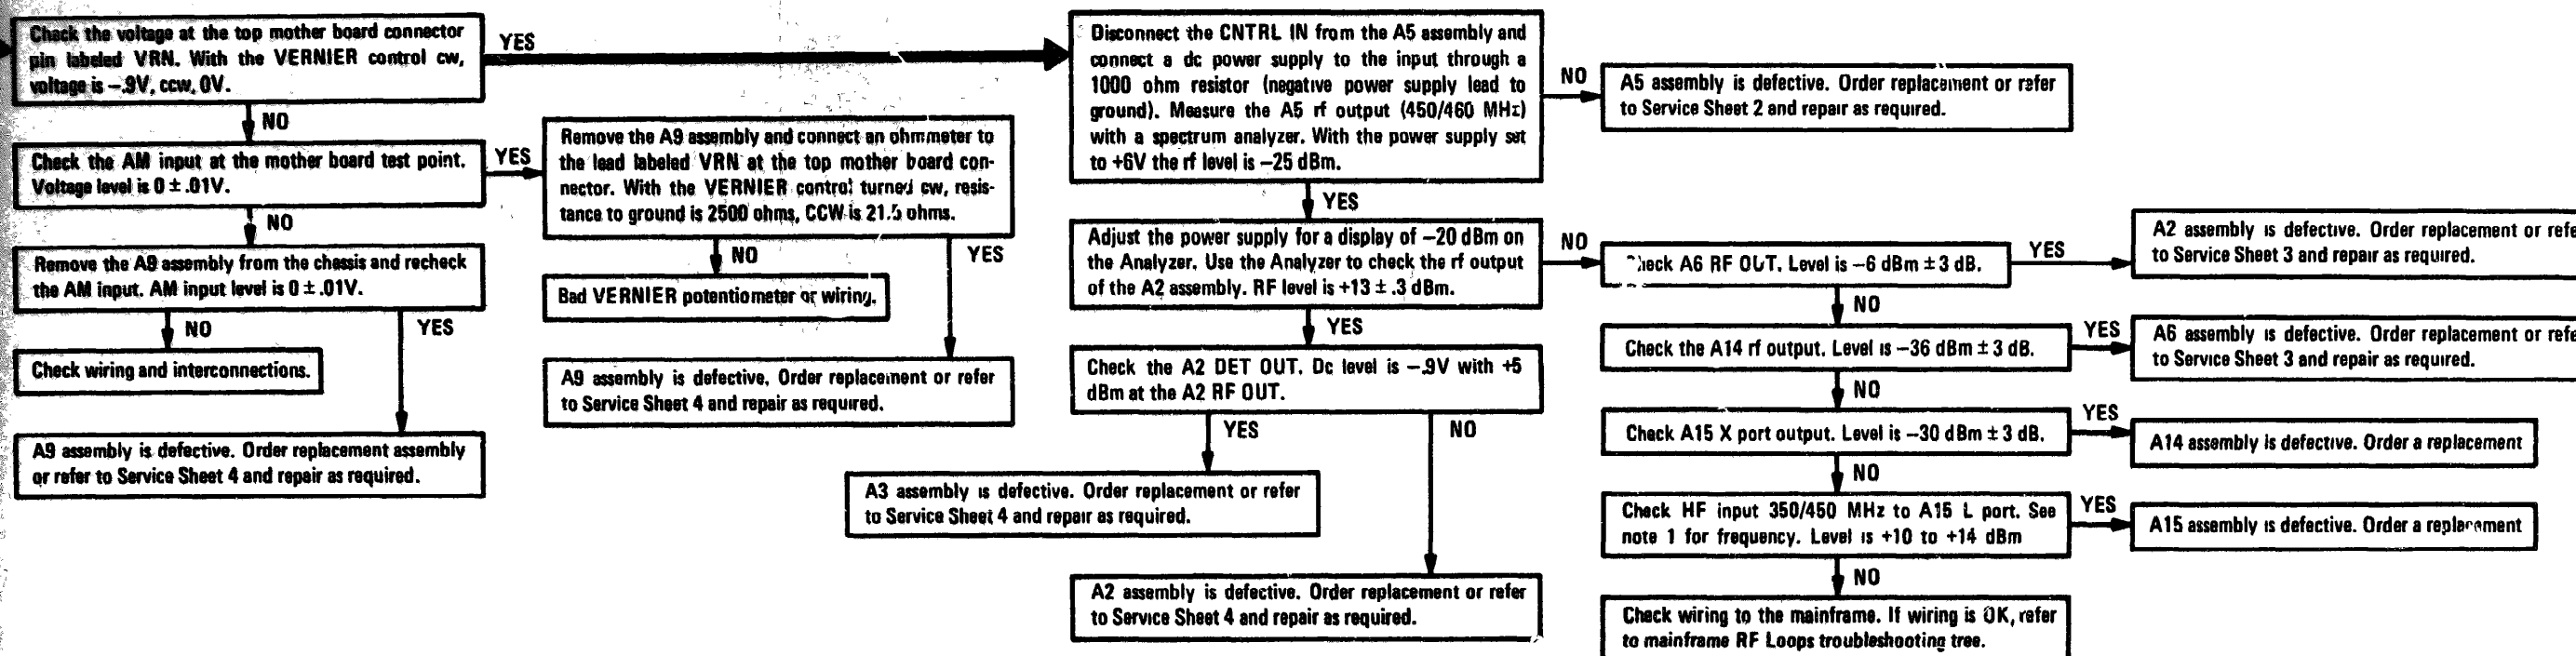


Figure 2

BCD	8	4	2	1
0	0	0	0	0
0	0	0	1	
0	0	1	0	
0	0	1	1	
0	1	0	0	
0	1	0	1	
0	1	1	0	
0	1	1	1	
1	0	0	0	
1	0	0	1	

"D" lines ON = +21V, OFF = -21V
 "L" lines ON = >+2V, OFF = <+.7V
 "F" lines ON = +1.6V, OFF = +.7V

10 dB atten steps	BCD	8	4	2	1
+10 dB		0	0	0	0
0		0	0	0	1
-10		0	0	1	0
-20		0	0	1	1
-30		0	1	0	0
-40		0	1	0	1
-50		0	1	1	0
-60		0	1	1	1
-70		1	0	0	0
-80		1	0	0	1
-90		1	0	1	0
-100		1	0	1	1
-110		1	1	0	0
-120		1	1	0	1
-130		1	1	1	0
-140		1	1	1	1

Figure 3

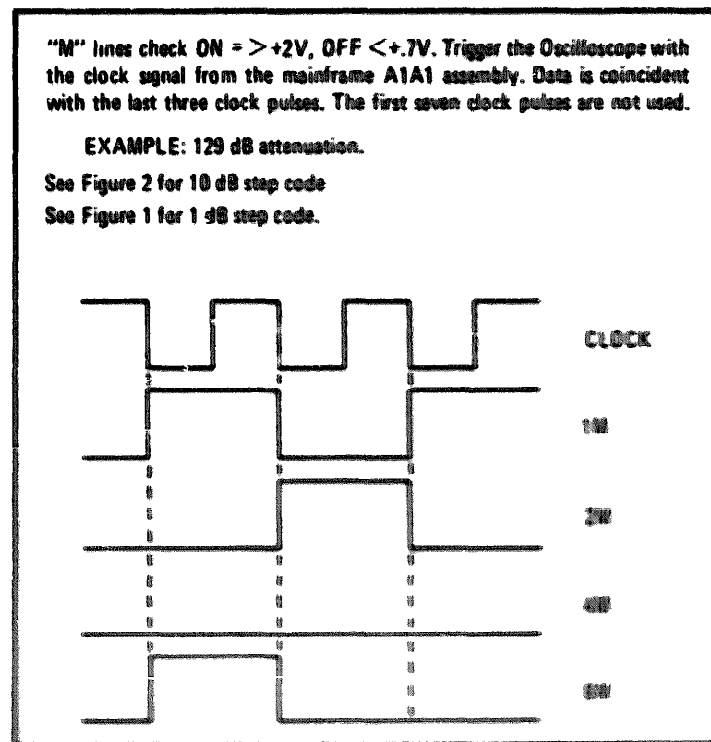


Figure 8-7. Model 86601A Troubleshooting Tree (2 of 2)

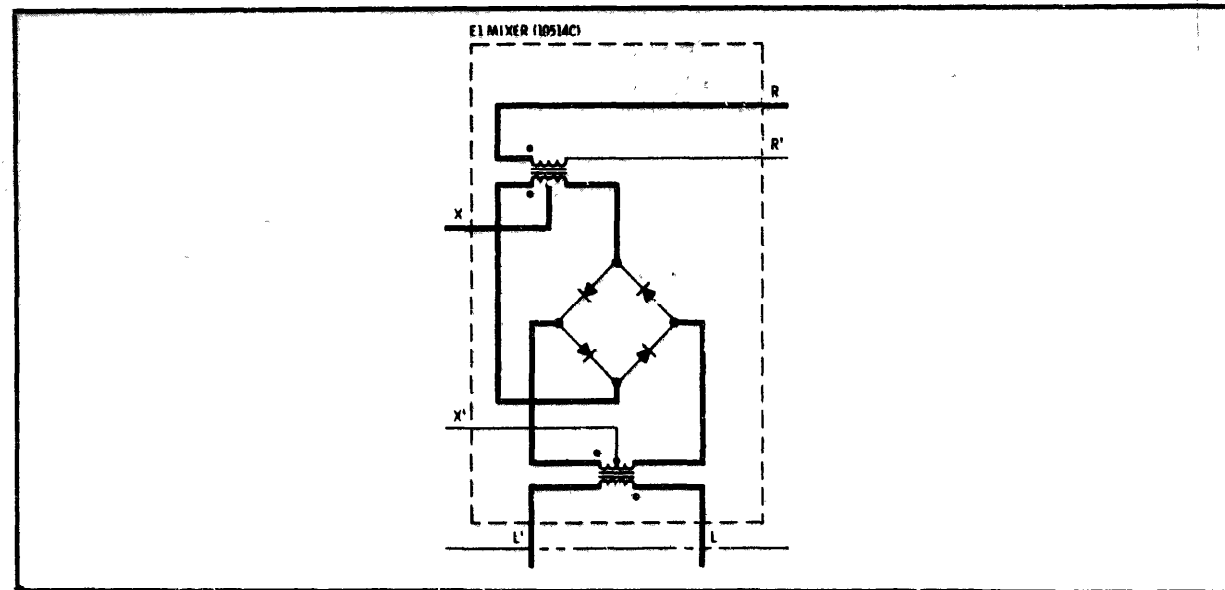


Figure 8-9. Mixer Schematic Diagram


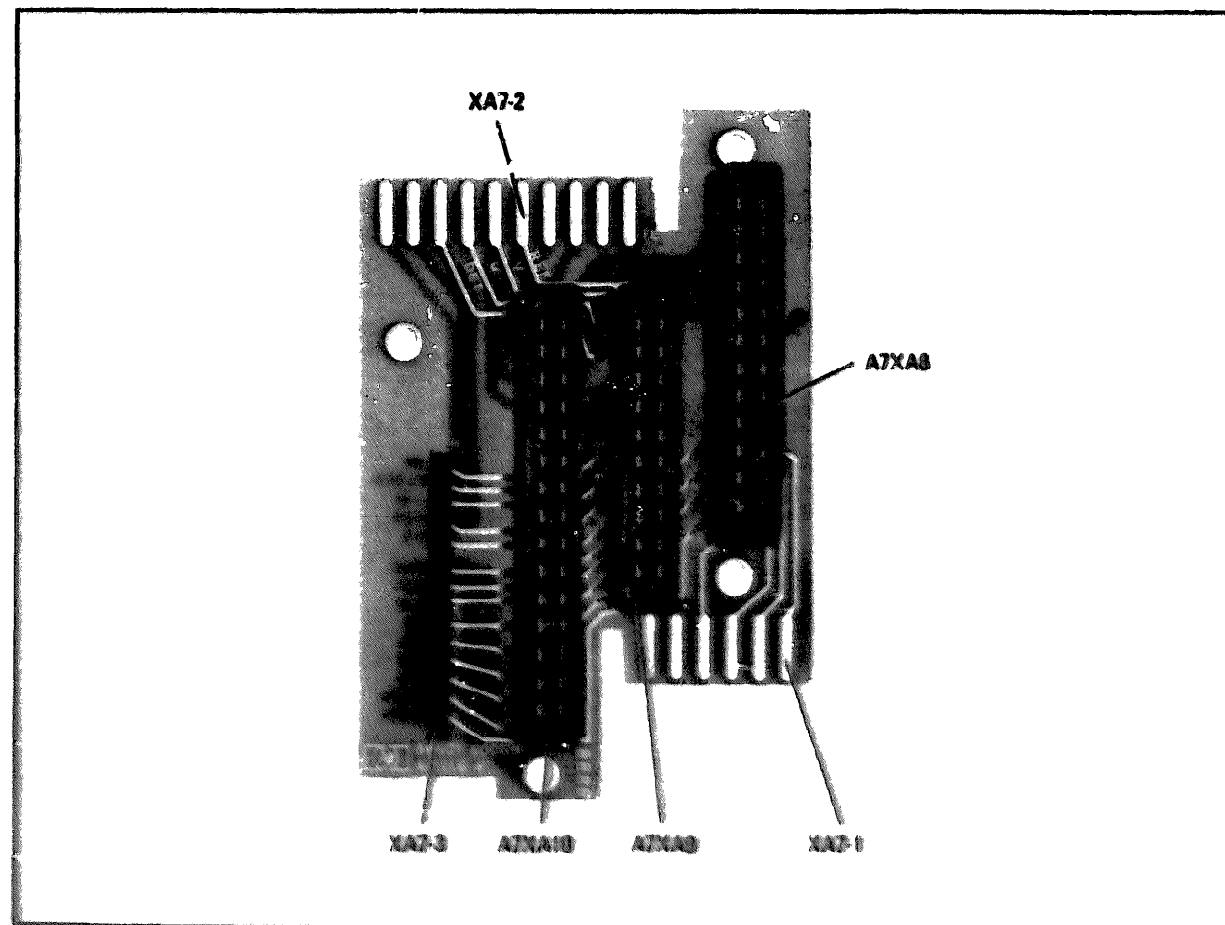


Figure 8-10. Mother Board Component Locations

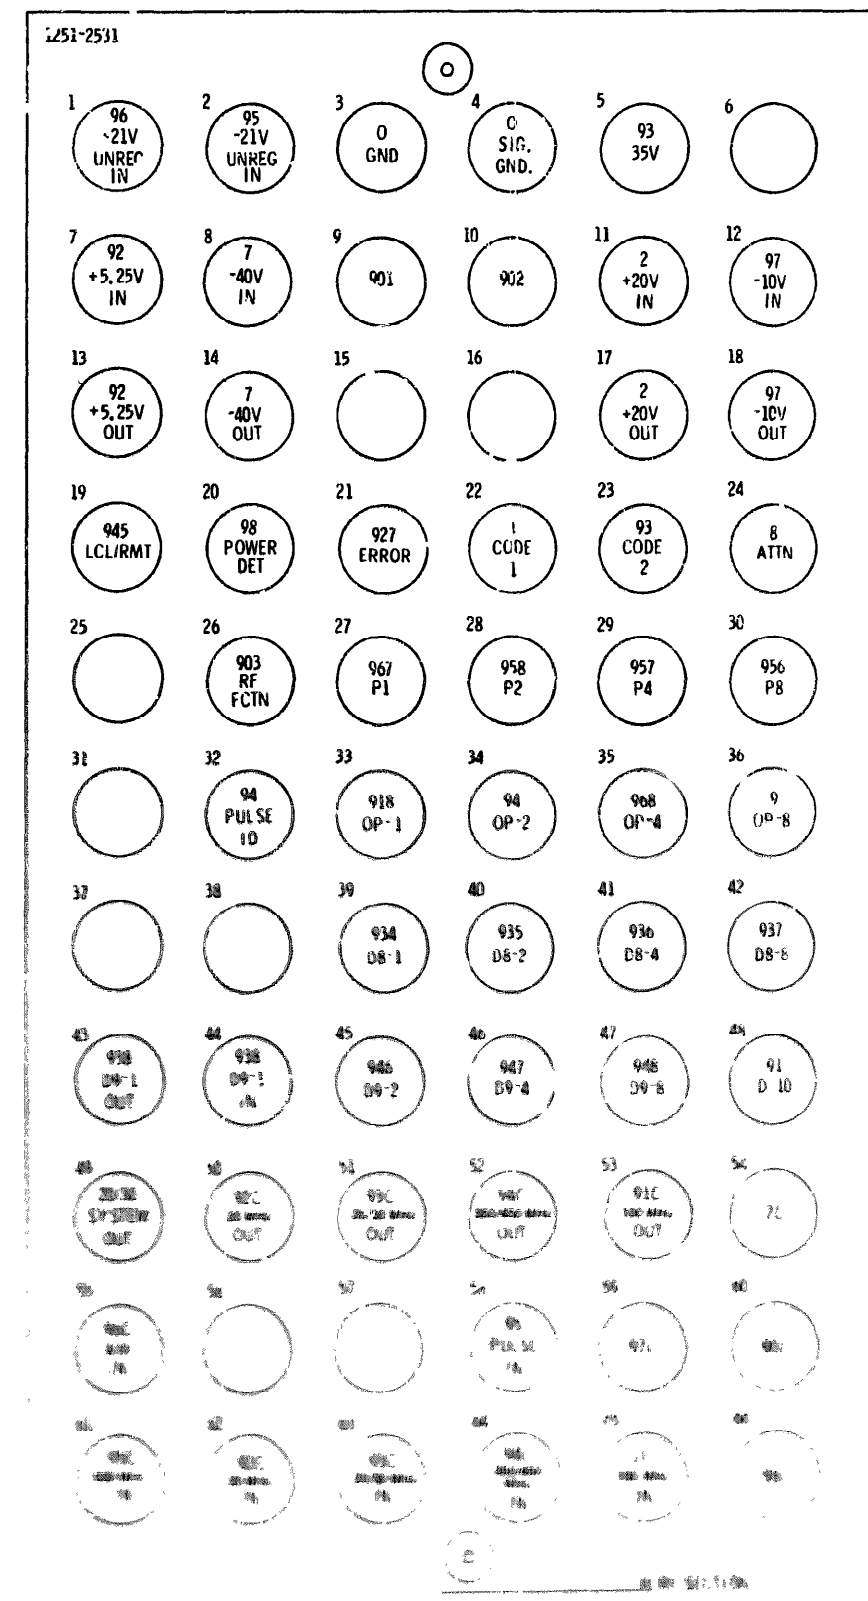

- NOTES
1. PART NUMBERS SHOWN INCLUDE PINS
 2. COAX PINS ARE HF PAIR. REGULAR PINS ARE HP
 3. A TOOL KIT WITH WINCHESTER 1074 IS REQUIRED TO PINS
 4. A TOOL KIT WITH WINCHESTER 1074 AND A TOOL KIT CATALOG NUMBER 1074 IS REQUIRED TO INSTALL COAX PINS

Figure 8-11 Input Connector



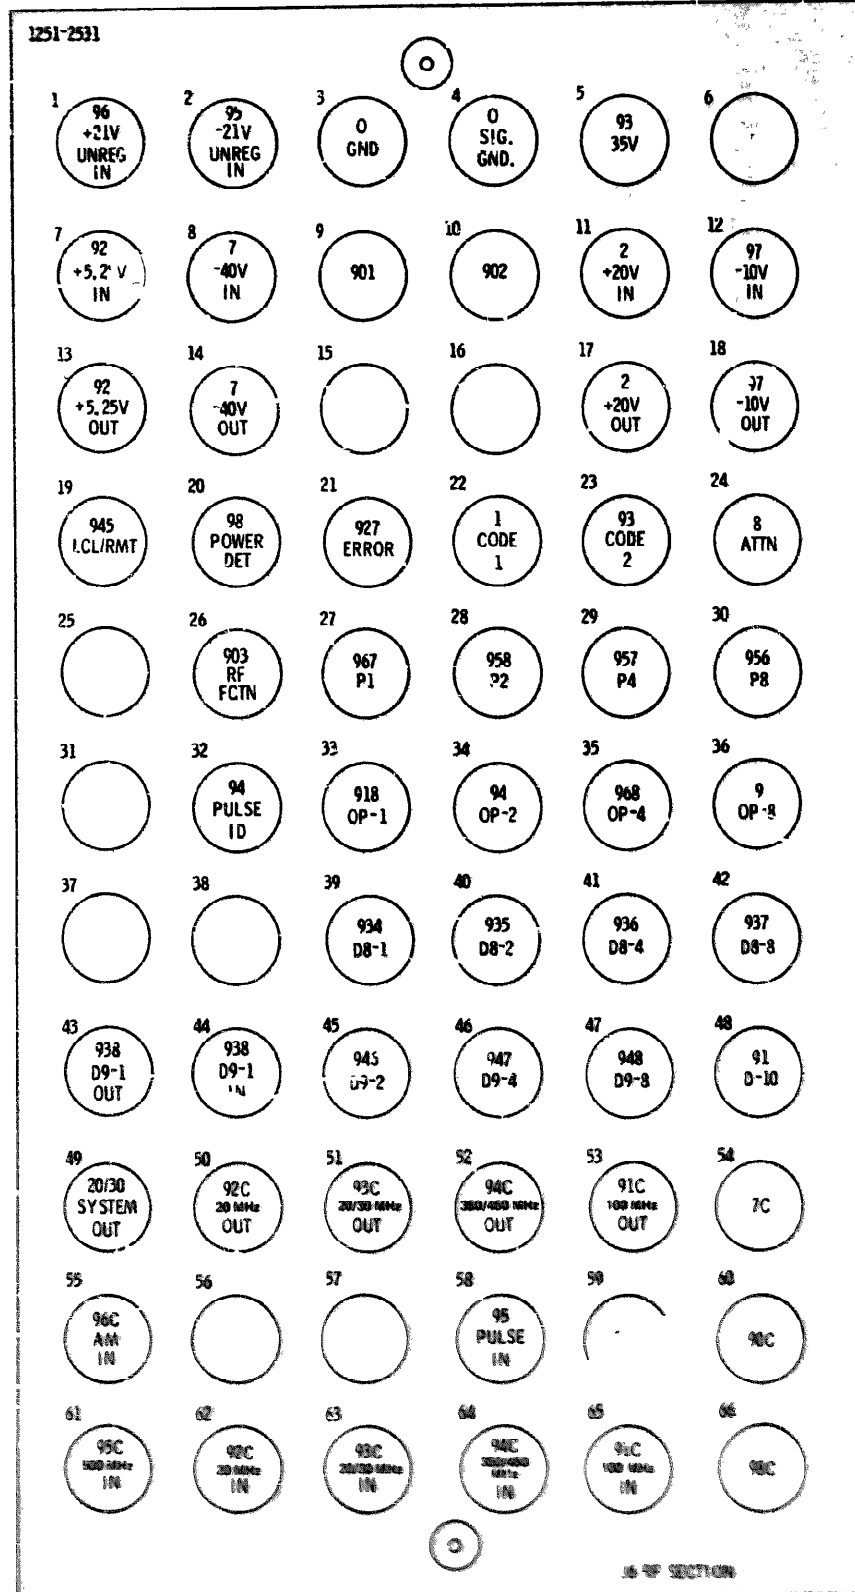


Figure 8-11. Input Connector

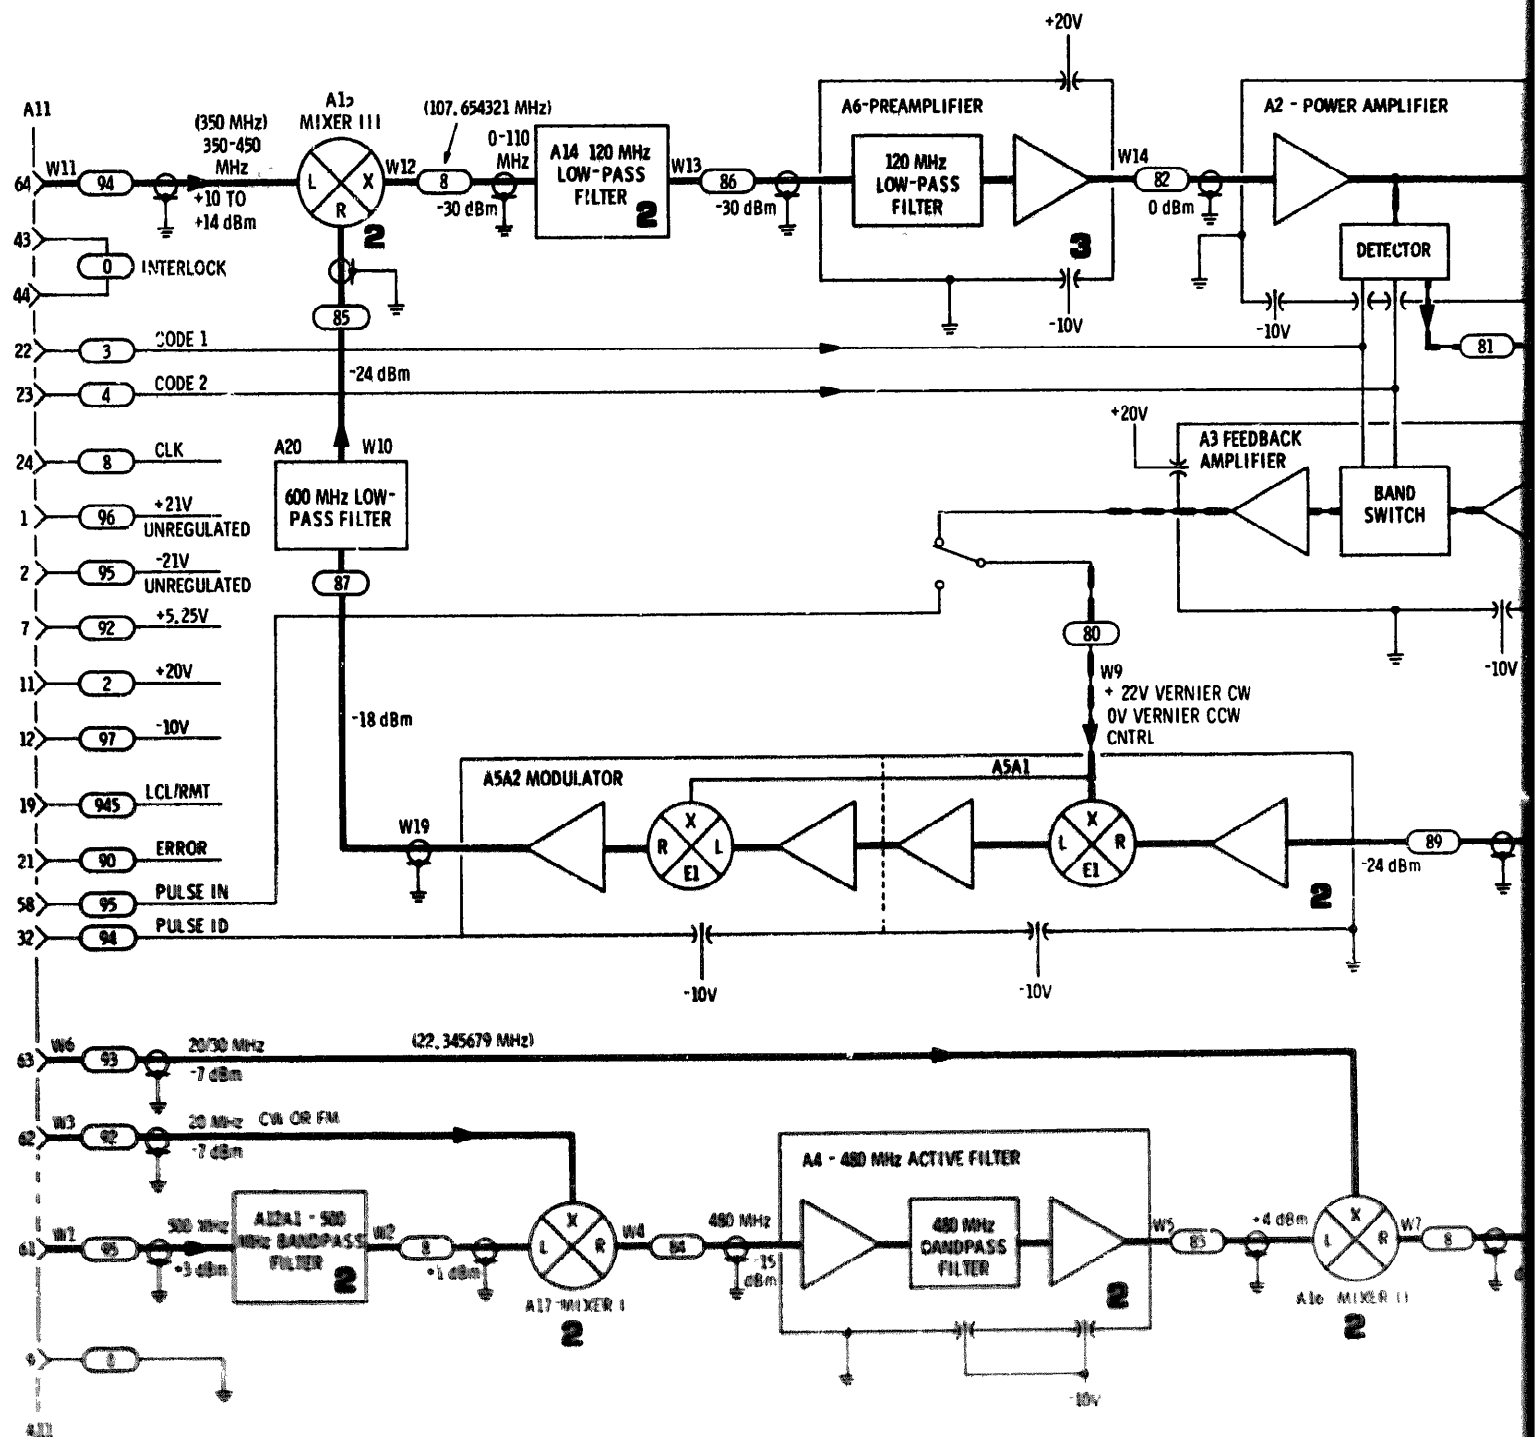

- NOTES:
1. PART NUMBERS SHOWN FOR CONNECTORS DO NOT INCLUDE PINS
 2. COAX PINS ARE HP PART NUMBER 1251-2041 REGULAR PINS ARE HP PART NUMBER 1251-1908
 3. A TOOL KIT, WINCHESTER CATALOG NUMBER 107K41 IS REQUIRED TO INSTALL THE REGULAR PINS.
 4. A TOOL KIT, WINCHESTER CATALOG NUMBER 107-0400 AND A TOOL LOCATOR WINCHESTER CATALOG NUMBER 107-0602 IS REQUIRED TO INSTALL COAX PINS.

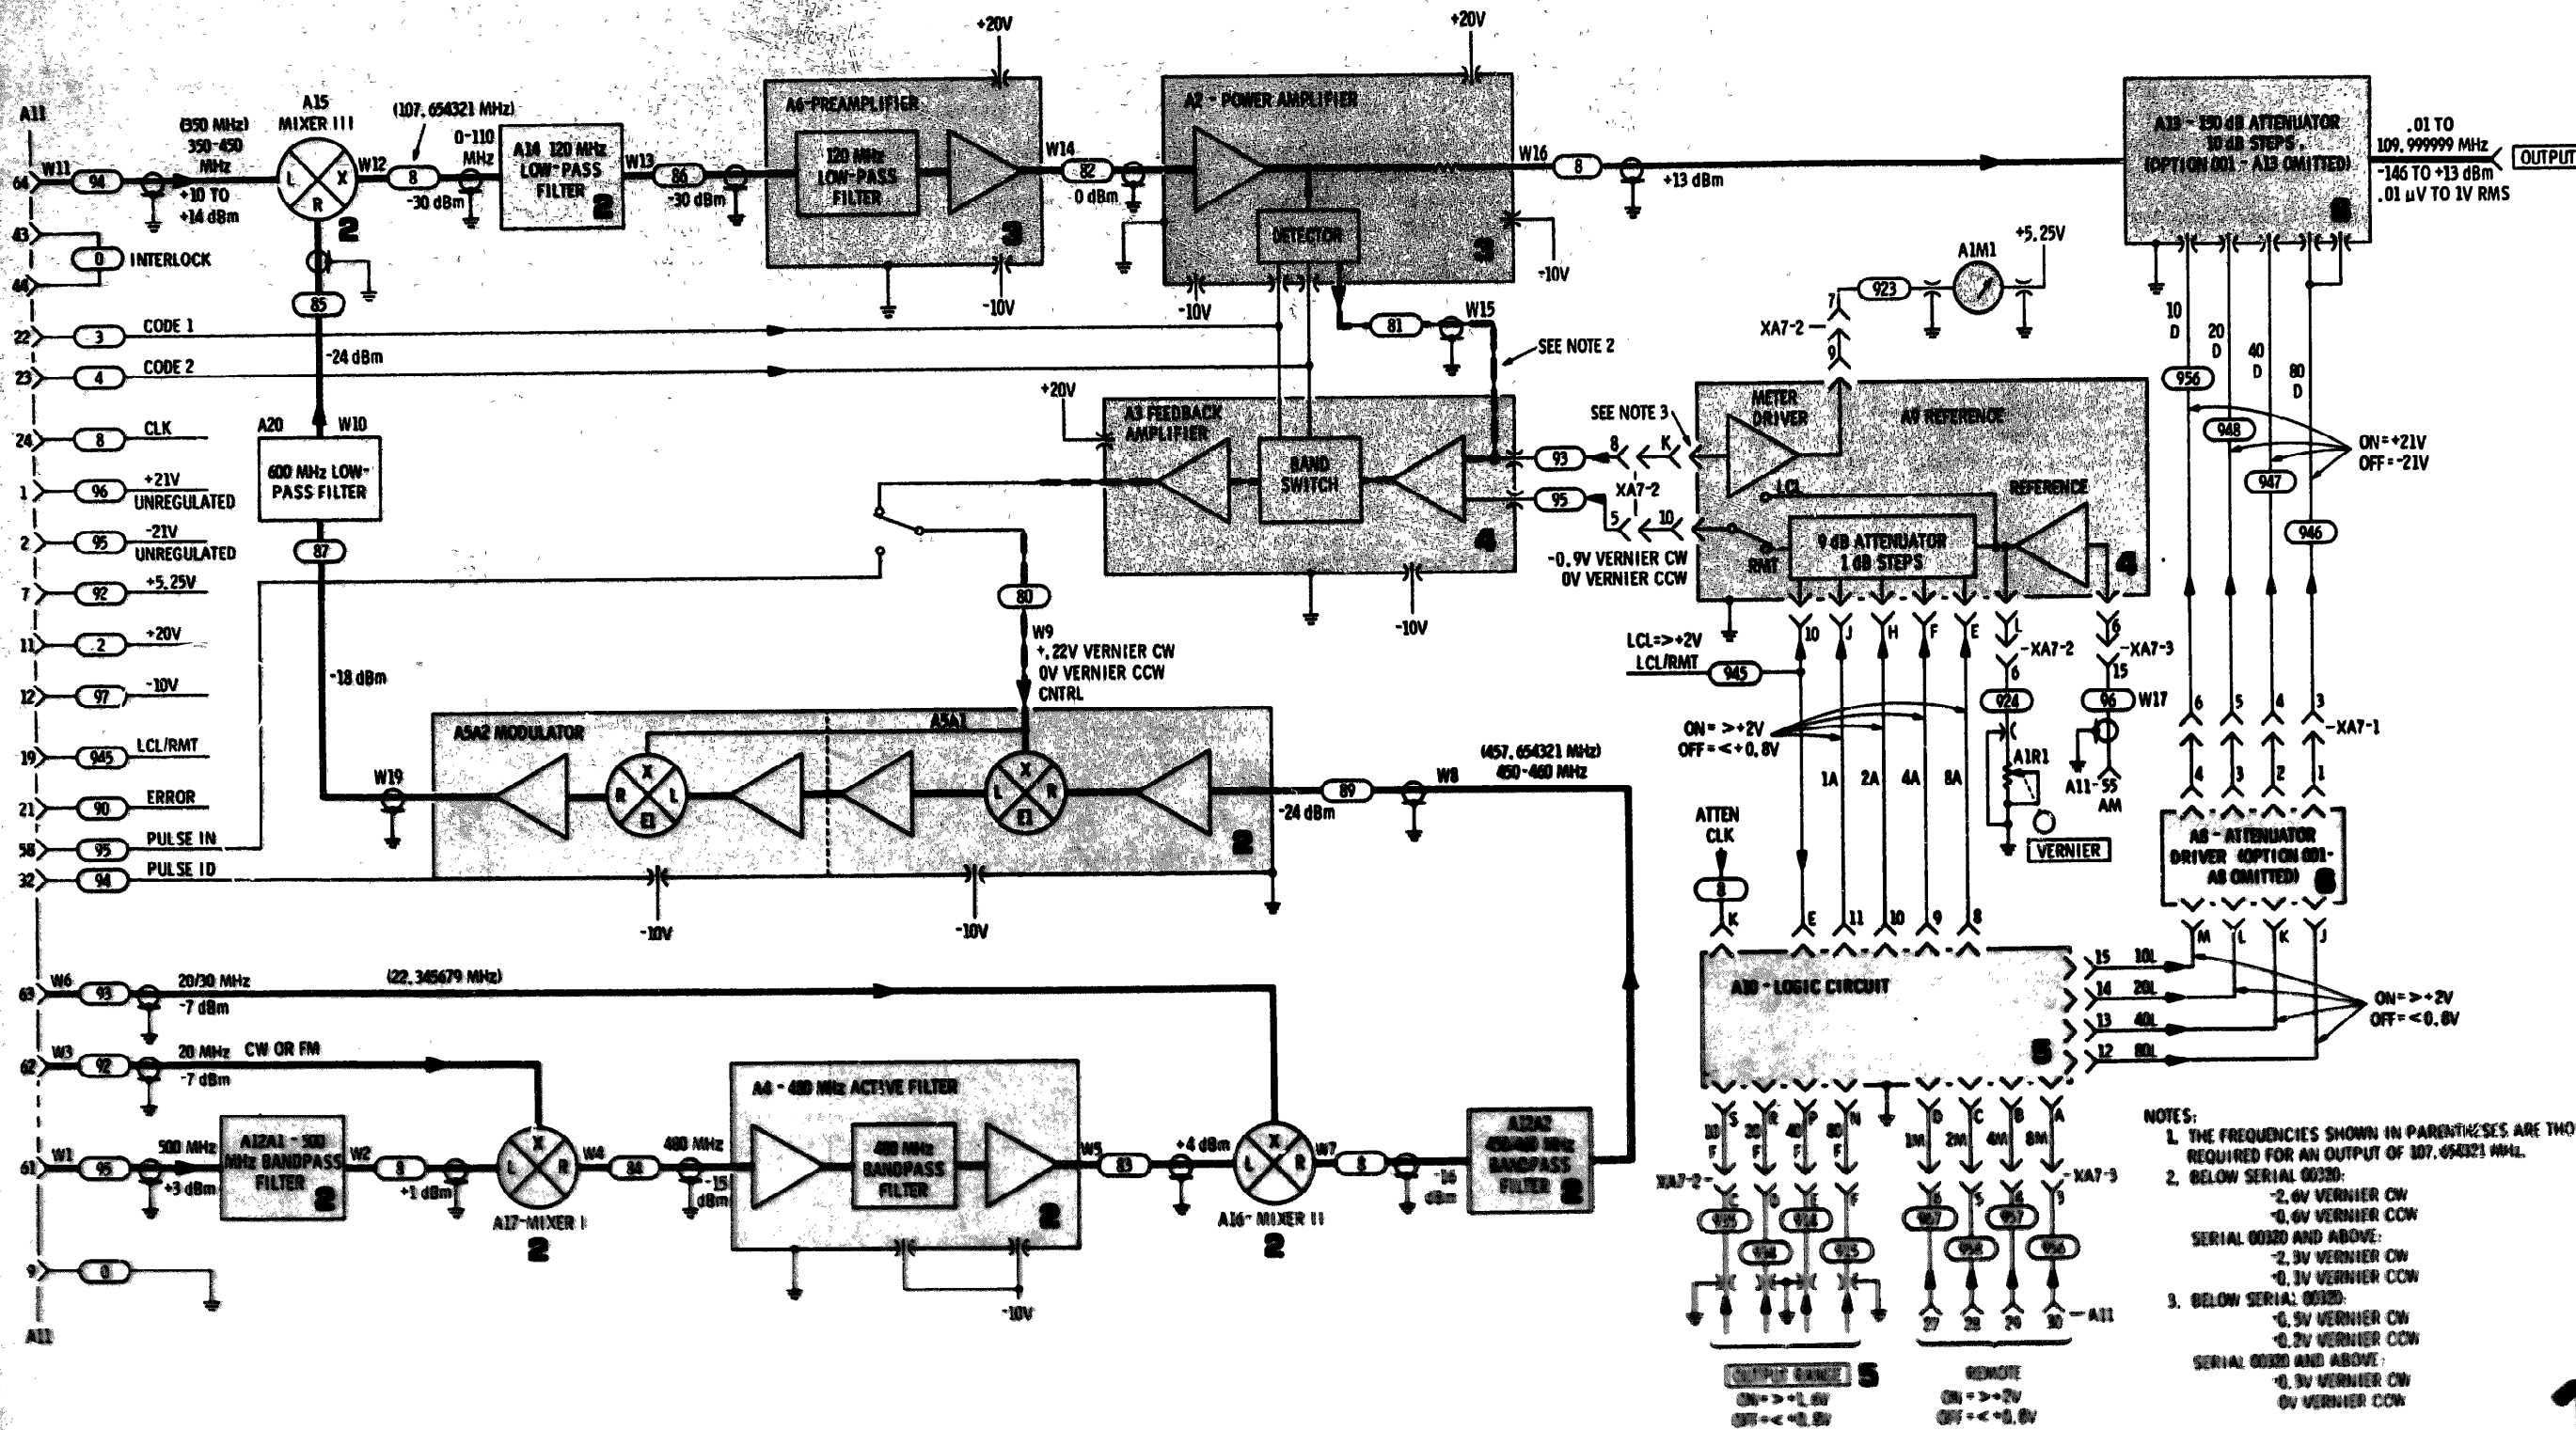

- NOTES:
1. THE FREQUENCIES SHOWN IN PARENTHESES ARE THOSE REQUIRED FOR AN OUTPUT OF 107.654321 MHz.
 2. BELOW SERIAL 0030:
-2.0V VERNIER CW
-0.6V VERNIER CCW
SERIAL 0030 AND ABOVE:
-2.3V VERNIER CW
-0.3V VERNIER CCW
 3. BELOW SERIAL 0030:
-0.5V VERNIER CW
-0.2V VERNIER CCW
SERIAL 0030 AND ABOVE:
-0.3V VERNIER CW
0V VERNIER CCW

Figure 8-12. Model 86601A Block Diagram

SERVICE SHEET 2

INPUT SIGNALS PROCESSING

Normally, causes of a malfunction in the Model 86601A will be isolated to a circuit board or assembly as a result of performing the tests specified in the troubleshooting trees.

When trouble has been isolated to a specific circuit board or assembly it should be removed and reinstalled in a position which provides easy access to test points and components. In some cases this may be accomplished by using extender boards; in others, it will be necessary to reconnect rf and dc inputs and outputs with the assembly removed from the housing in which it is normally contained.

TEST EQUIPMENT REQUIRED (See Table 1-2)

Digital Voltmeter Low Voltage Power Supply
Electronic Counter Spectrum Analyzer
Vector Voltmeter

GENERAL INFORMATION

The circuits shown and described on Service Sheet 2 convert the 4 inputs from the mainframe, by means of mixing and filtering processes, to the selected output frequency. The various filters greatly reduce harmonic signals, undesired mixing products, and spurious signals. The amplifiers between the mixers compensate for the insertion losses of the filters and mixers.

500 MHz BANDPASS FILTER (A12A1)

The 500 MHz bandpass filter effectively traps all harmonics of the 500 MHz input signal and the 100 MHz signal from which it is derived. Insertion loss is about 2 dB and the bandpass is typically 3 MHz at 3 dB points on the response curve.

MIXER I (A17)

Mixer I is a matched-quad-diode double-balanced mixer. The inputs to the mixer are the precise 500 MHz output from the reference section in the mainframe and a precise 20 MHz signal from the reference section in the mainframe or a 20 MHz signal which is generated in the modulator section plug-in. Both of the input signals are balanced out in the mixer and only the sum and difference signals are available at the output port. The output of Mixer I is coupled to the A4 assembly.

480 MHz ACTIVE FILTER (A4)

The A4 active filter consists of two identical two-stage tuned amplifiers separated by a bandpass filter. Each of the two-stage amplifiers has a gain of about 10 dB. The filter has an insertion loss of about 2 dB and the bandpass is typically 6 MHz at 3 dB points on the response curve.

MIXER II (A16)

Mixer II is the same as Mixer I. This mixer mixes the 480 MHz signal from the A4 assembly with a signal between 20.000001 and 30.000000 MHz from the SL1 loop in the mainframe. The difference signal (450/460 MHz) at the output port is coupled to the A12A2 assembly.

450/460 MHz BANDPASS FILTER (A12A2)

The A12A2 450/460 MHz bandpass filter has an insertion loss of about 5 dB. The passband is centered at 455 MHz and typically is 12 MHz at 2 dB points on the response curve.

MODULATOR ASSEMBLY (A5)

The signal from the 450/460 MHz bandpass filter is coupled to the A5 modulator assembly. A two-stage amplifier amplifies the signal before it is coupled to the L port of a double balanced mixer (E1) which acts as an attenuator to control the rf output level of the 86601A.

SERVICE SHEET 2 (cont'd)

When the instrument is operated in the CW or FM modes the input to the X port of E1 is dc bias level that is controlled by the leveling loop and the reference assembly. Its purpose is to assure that the rf output from the instrument remains constant at a specific level.

When the instrument is operated in the AM mode, an ac modulating signal is superimposed on the dc bias level to the X port of E1. The amplitude of the ac signal controls the percentage of modulation of the Model 86601A output rf signal.

The output of the modulator is applied through a 600 MHz lowpass filter (A20) which has an insertion loss of about 7 dB and a 4 dB pad to Mixer III.

MIXER III (A15)

Mixer III is the same as Mixers I and II. This mixer mixes the 450/460 MHz output of the A5 assembly with a 350/450 MHz (10 MHz steps) from the high frequency loop in the mainframe. The output of Mixer III is between .01 and 110 MHz. The exact output frequency is selected by the mainframe in increments as low as 1 Hz except when the mainframe is an option 004 instrument. Mainframe option 004 limits frequency selection to 100 Hz increments (frequency selection is still exact).

120 MHz LOWPASS FILTER (A14)

The output of Mixer III is applied to the pre-amplifier (A6 shown on Service Sheet 3) through a 120 MHz lowpass filter. This filter sharply attenuates all harmonic and spurious signals above 120 MHz. Insertion loss for signals below 120 MHz is typically less than 1 dB.

NOTES

1. Verify the presence of dc operating voltages before taking other measurements. If dc voltages are not present check connections to the mainframe. If interconnections are good refer to the mainframe manual and make necessary repairs.
2. All measurements are taken with the Spectrum Analyzer unless otherwise specified.

TEST PROCEDURE

Test 1-a. Measure the amplitude of the 500 MHz signal at the output end of W2. If the amplitude is greater than, or equal to +1 dBm, proceed to test 2-a. If the amplitude is less than +1 dBm, proceed to test 1-b.

Test 1-b. Measure the amplitude of the 500 MHz signal at the output end of cable W1. If the amplitude is equal to, or greater than +3 dBm, use a counter to verify that the frequency is exactly 500 MHz. If the amplitude and frequency are correct, repair or replace the A12 assembly or cable W2. If the specified signal is not present check cable W1. If Cable W1 is good, refer to the mainframe manual. trouble is in the mainframe reference section or in interconnections.

SERVICE SHEET 2 (cont'd)

TEST PROCEDURE

Test 2-a. Measure the 480 MHz signal at the output end of Cable W4. If the amplitude is -14 dBm, ± 2 dB, proceed to test 3-a. If the amplitude is low, proceed to test 2-b.

Test 2-b. Measure the amplitude of the 20 MHz signal at the output end of cable W3. If the amplitude is -5 dBm ± 1 dB, use a counter to verify that the frequency is exactly 20 MHz (instrument operating in CW or AM mode). If the amplitude and frequency are correct, replace the A17 assembly or cable W4. If the specified signal is not present check cable W3. If cable W3 is good, refer to the mainframe manual; trouble is in the mainframe reference section or in interconnections.

NOTE

The 20 MHz signal is coupled to the Model 86601A through the Modulation drawer. A modulation or Auxiliary section must be in place in the modulator drawer.

TEST PROCEDURE q

Test 3-a. Measure the amplitude of the 480 MHz signal at the output end of cable W5. If the signal is equal to, or greater than, +1 dBm, proceed to test 4-a. If the amplitude is low, proceed to test 3-b.

3-b. Measure the 480 MHz signal at the output of the A4 assembly at J1.

TEST PROCEDURE

Test 4-a. Measure the 450/460 MHz signal at the output end of cable W7. If the amplitude is -14 dBm ± 2 dB, proceed to TEST PROCEDURE 5. If the amplitude is low, proceed to Test 4-b.

Test 4-b. Measure the 20/30 MHz signal at the output end of cable W6. The amplitude should be -6 dBm ± 2 dB. Use the counter to check the frequency at the output end of cable W6.

NOTE

The 20/30 MHz frequency may be determined by subtracting thumbwheel digits 1 through 7 from 30.000000 MHz. EXAMPLE: Thumbwheels are set to 0107.654321 MHz.

30.000000
7.654321
22.345679

If the signal amplitude and frequency are correct, repair or replace Mixer II or cable W7

FM modes the input controlled by the leveling to assure that the rf is at a specific level.

ode, an ac modulating the X port of E1. The range of modulation of

h a 600 MHz lowpass at 7 dB and a 4 dB pad

This mixer mixes the h a 350/450 MHz (10 the mainframe. The Hz. The exact output ements as low as 1 Hz nstrument. Mainframe 100 Hz increments

mplifier (A6 shown on lter. This filter sharply ls above 120 MHz. pically less than 1 dB.

g voltages before voltages are not e mainframe. If the mainframe

n the Spectrum

Hz signal at the output or equal to +1 dBm, an +1 dBm, proceed to

Hz signal at the output to, or greater than +3 cy is exactly 500 MHz. pair or replace the A12 is not present check e mainframe manual; or in interconnections.

SERVICE SHEET 2 (cont'd)

TEST PROCEDURE

Test 2-a. Measure the 480 MHz signal at the output end of Cable W4. If the amplitude is -14 dBm, ±2 dB, proceed to test 3-a. If the amplitude is low, proceed to test 2-b.

Test 2-b. Measure the amplitude of the 20 MHz signal at the output end of cable W3. If the amplitude is -5 dBm ±1 dB, use a counter to verify that the frequency is exactly 20 MHz (instrument operating in CW or AM mode). If the amplitude and frequency are correct, replace the A17 assembly or cable W4. If the specified signal is not present check cable W3. If cable W3 is good, refer to the mainframe manual; trouble is in the mainframe reference section or in interconnections.

NOTE

The 20 MHz signal is coupled to the Model 86601A through the Modulation drawer. A modulation or Auxiliary section must be in place in the modulator drawer.

TEST PROCEDURE

Test 3-a. Measure the amplitude of the 480 MHz signal at the output end of cable W5. If the signal is equal to, or greater than, +1 dBm, proceed to test 4-a. If the amplitude is low, proceed to test 3-b.

3-b. Measure the 480 MHz signal at the output of the A4 assembly at J1.

TEST PROCEDURE

Test 4-a. Measure the 450/460 MHz signal at the output end of cable W7. If the amplitude is -14 dBm ±2 dB, proceed to TEST PROCEDURE 5. If the amplitude is low, proceed to Test 4-b.

Test 4-b. Measure the 20/30 MHz signal at the output end of cable W6. The amplitude should be -6 dBm ±2 dB. Use the counter to check the frequency at the output end of cable W6.

NOTE

The 20/30 MHz frequency may be determined by subtracting thumbwheel digits 1 through 7 from 30.000000 MHz. EXAMPLE: Thumbwheels are set to 0107.654321 MHz.

30.000000
7.654321

22.345679

If the signal amplitude and frequency are correct, repair or replace Mixer II or cable W7.

SERVICE SHEET 2 (cont'd)

If the signal is missing or level is low, check cable W6; if W6 is good the problem is in the mainframe.

If the frequency is incorrect, trouble is in the mainframe.

TEST PROCEDURE

Test 5-a. Measure the 450/460 MHz signal at the output end of cable W8. If the amplitude is -22 dBm ±2 dB, proceed to TEST PROCEDURE 6. If the amplitude is low, repair or replace the A12 bandpass filter or cable W8.

TEST PROCEDURE

Test 6-a. Measure the signal at the output end of cable W10. If the signal is equal to or greater than -23 dBm, proceed to TEST PROCEDURE 7. If the signal is less than -23 dBm, proceed to test 6-b.

Test 6-b. Disconnect the CNTRL IN lead from the AS assembly and connect a power supply in its place (0 volts initially, 1000 ohms in series with positive lead, negative lead to ground). Monitor the output of cable W10 and slowly raise the power supply output to about 600 millivolts. If the signal at the output end of cable W10 is now about -23 dBm, the problem is in the feedback loop or associated circuits; refer to Service Sheet 3. If the output signal did not increase with application of the dc level, proceed to Test 6-c.

Test 6-c. Remove the A5 assembly from the chassis and reconnect the leads. NOTE: Be sure to use an insulating material between the assembly and the chassis to avoid damage to the circuit.

Connect the Vector Voltmeter channel A input to the RF IN at J2 and lock the meter to the signal. Use the Vector Voltmeter channel B probe to trace the signal through the assembly.

When repairs are completed the A2 and A6 assembly adjustment procedures should be performed.

TEST PROCEDURE

Test 7-a. Measure the signal at the output end of cable W12. The signal should be -30 ±3 dBm at the center frequency selected by the mainframe.

If the correct signal is present proceed to Test 7-b.

If the correct signal is not present, check Mixer III, the 350/450 MHz input from the mainframe (W11) and cables W11 and W12.

NOTE

The 350/450 MHz frequency may be determined by subtracting digits 8 and 9 from 450 MHz. (Digit 9 is always a zero or a one.) Example: Thumbwheels are set to 0107.654321 MHz.

450.000000
x 100.000000

350.000000 MHz

SERVICE SHEET 2 (cont'd)

Test 7-b. Measure the signal at the output end of cable W13. The signal should be -30 ±3 dBm at the center frequency selected by the mainframe.

If the signal is not present, check the 120 MHz low pass filter and cable W13.

SERVICE SHEET 2 (cont'd)

If signal is missing or level is low, check cable W6; if W6 is the problem is in the mainframe.
If frequency is incorrect, trouble is in the mainframe.

PROCEDURE

1. Measure the 450/460 MHz signal at the output end of cable W5. If the amplitude is $-22 \text{ dBm} \pm 2 \text{ dB}$, proceed to TEST PROCEDURE 6. If the amplitude is low, repair or replace the bandpass filter or cable W8.

PROCEDURE

1. Measure the signal at the output end of cable W10. If signal is equal to or greater than -23 dBm , proceed to PROCEDURE 7. If the signal is less than -23 dBm , proceed to test 6-b.

2. Disconnect the CNTRL IN lead from the A5 assembly and connect a power supply in its place (0 volts initially, 1000 ohms in series with positive lead, negative lead to ground). Measure the output of cable W10 and slowly raise the power output to about 500 millivolts. If the signal at the output of cable W10 is now about -23 dBm , the problem is in the feedback loop or associated circuits; refer to Service Sheet 3. If the output signal did not increase with application of the dc power, proceed to Test 6-c.

3. Remove the A5 assembly from the chassis and disconnect the leads. NOTE: Be sure to use an insulating material between the assembly and the chassis to avoid damage to the circuit.

4. Connect the Vector Voltmeter channel A input to the RF IN at the back of the chassis. Lock the meter to the signal. Use the Vector Voltmeter channel B probe to trace the signal through the assembly.

5. After repairs are completed the A2 and A6 assembly adjustment should be performed.

PROCEDURE

1. Measure the signal at the output end of cable W12. The signal should be $-30 \pm 3 \text{ dBm}$ at the center frequency selected by the mainframe.

If correct signal is present proceed to Test 7-b.

If correct signal is not present, check Mixer III, the 350/450 MHz signal output from the mainframe (W11) and cables W11 and W12.

NOTE


The 350/450 MHz frequency may be determined by subtracting digits 8 and 9 from 450 MHz. (Digit 9 is always a zero or a one.) Example: Thumbwheels are set to 07.854321 MHz.

$$\begin{array}{r} 450.000000 \\ \times 10^x \text{xxxx} \\ \hline 350.000000 \text{ MHz} \end{array}$$

SERVICE SHEET 2 (cont'd)

Test 7-b. Measure the signal at the output end of cable W13. The signal should be $-30 \pm 3 \text{ dBm}$ at the center frequency selected by the mainframe.

If the signal is not present, check the 120 MHz low pass filter and cable W13.

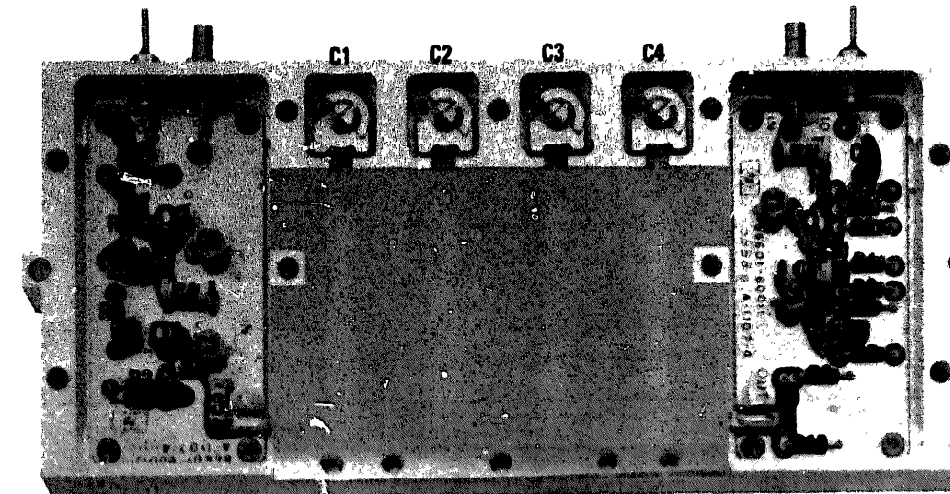

Block Diagram

SERVICE SHEET 1

Figure 8-14. 480 MHz Band Pass Filter Component Locations

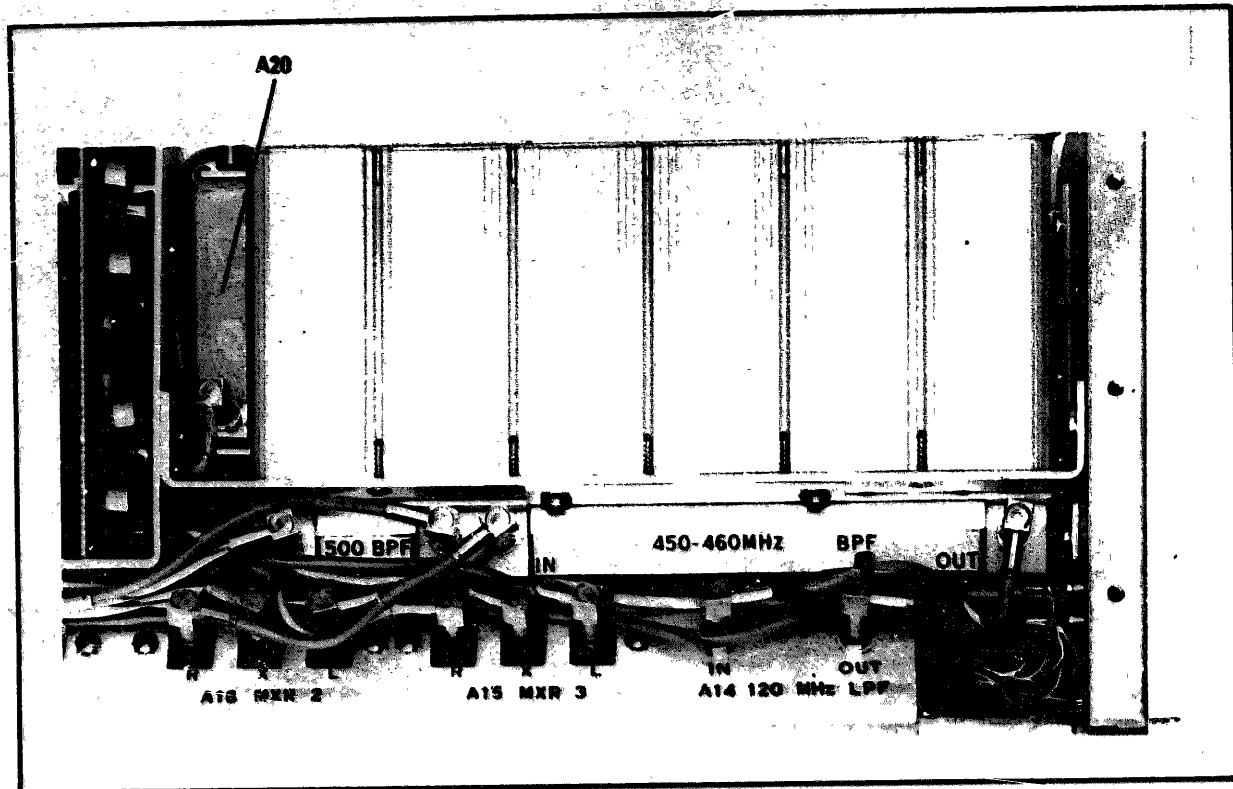


Figure 8-14. 600 MHz Low Pass Filter (A20) Location

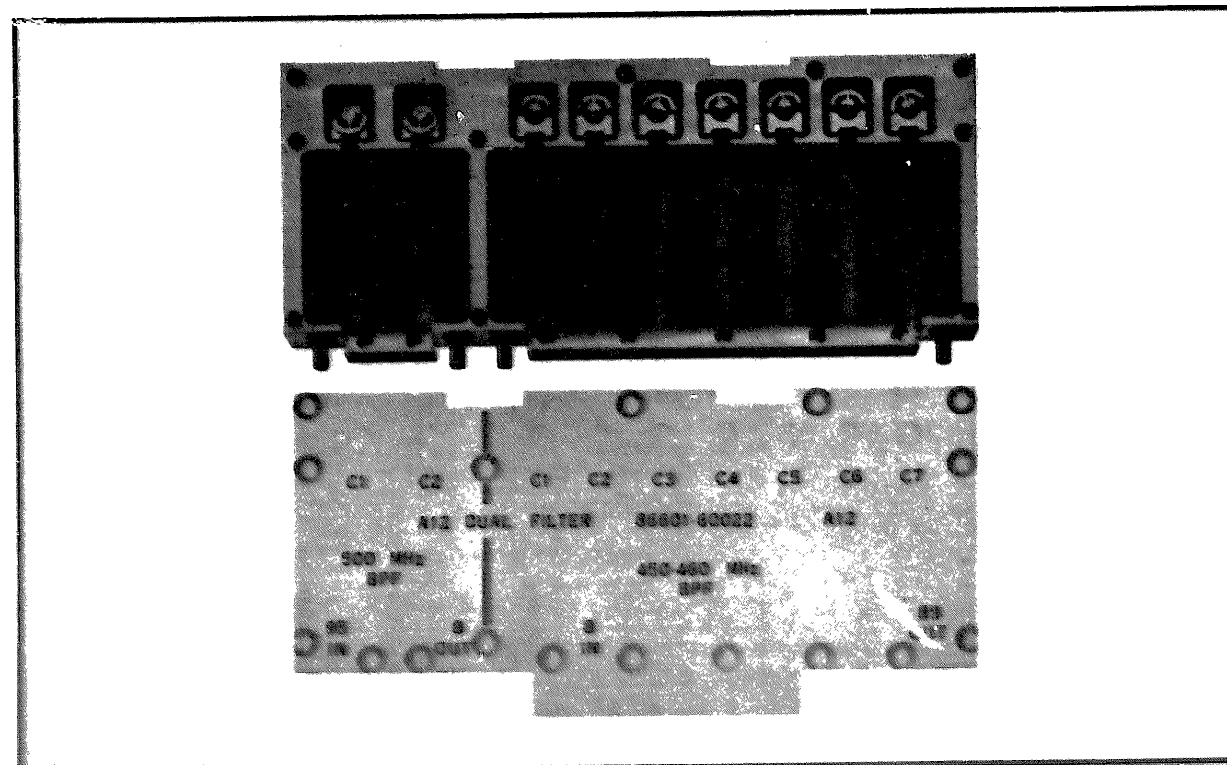


Figure 8-15. Dual Filter Adjustments Locations

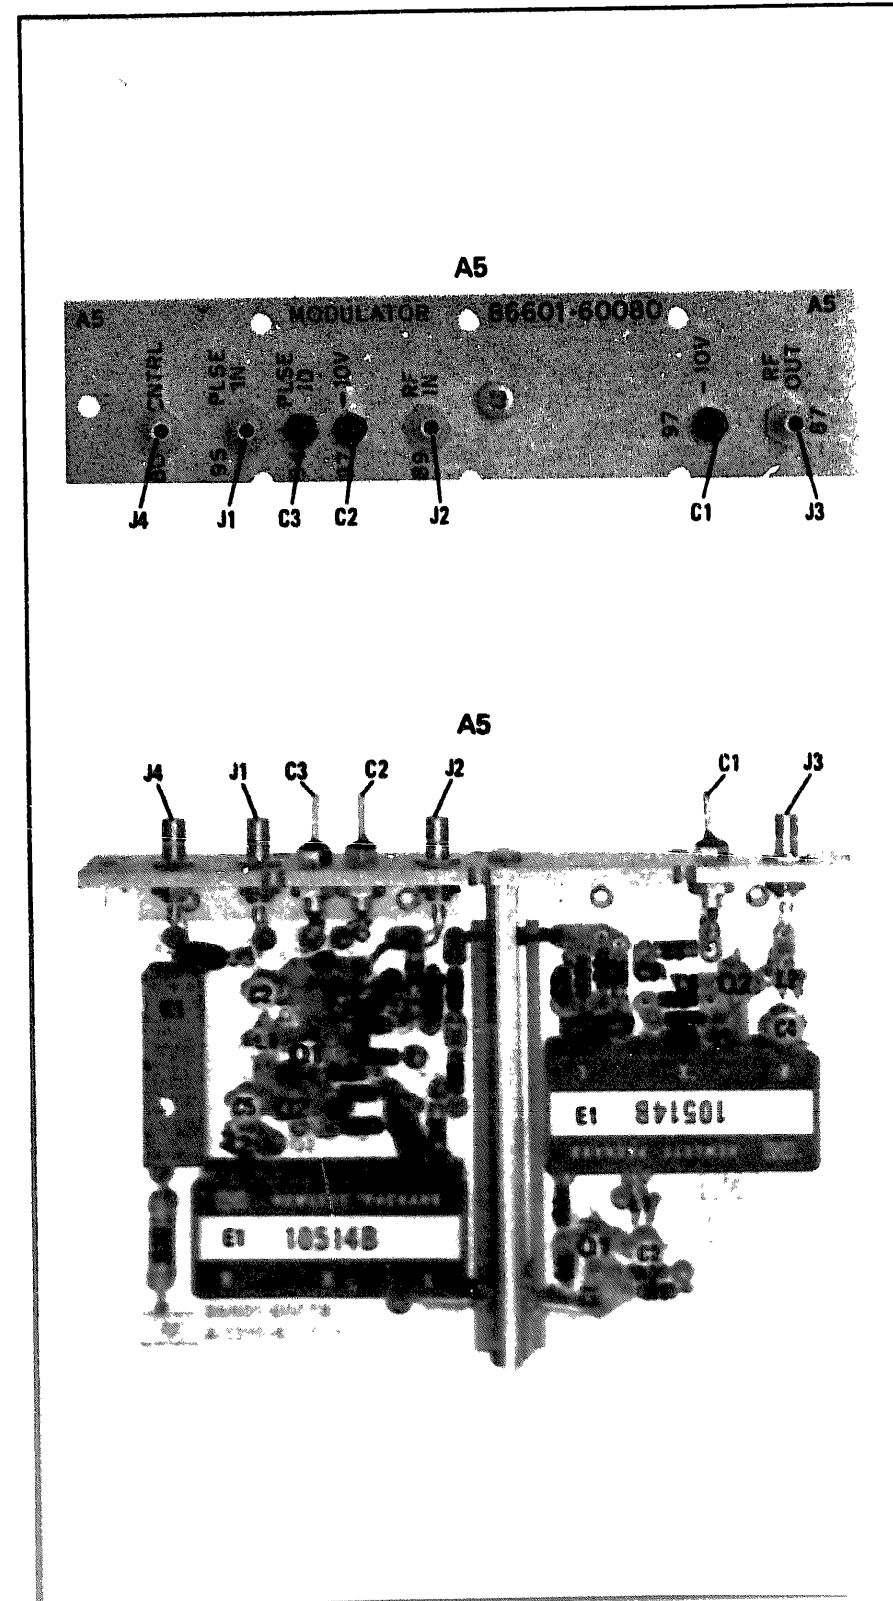
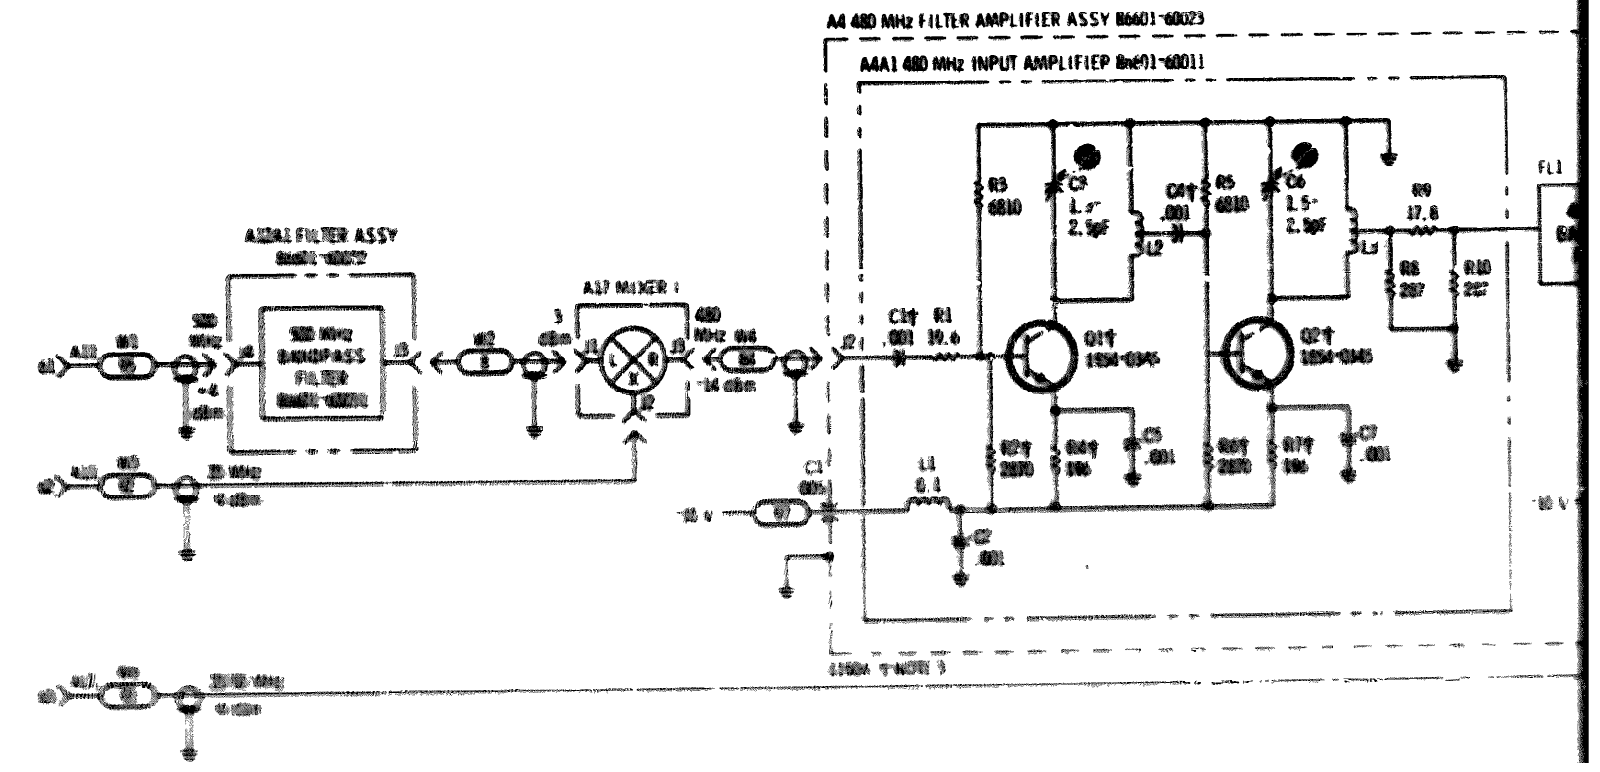
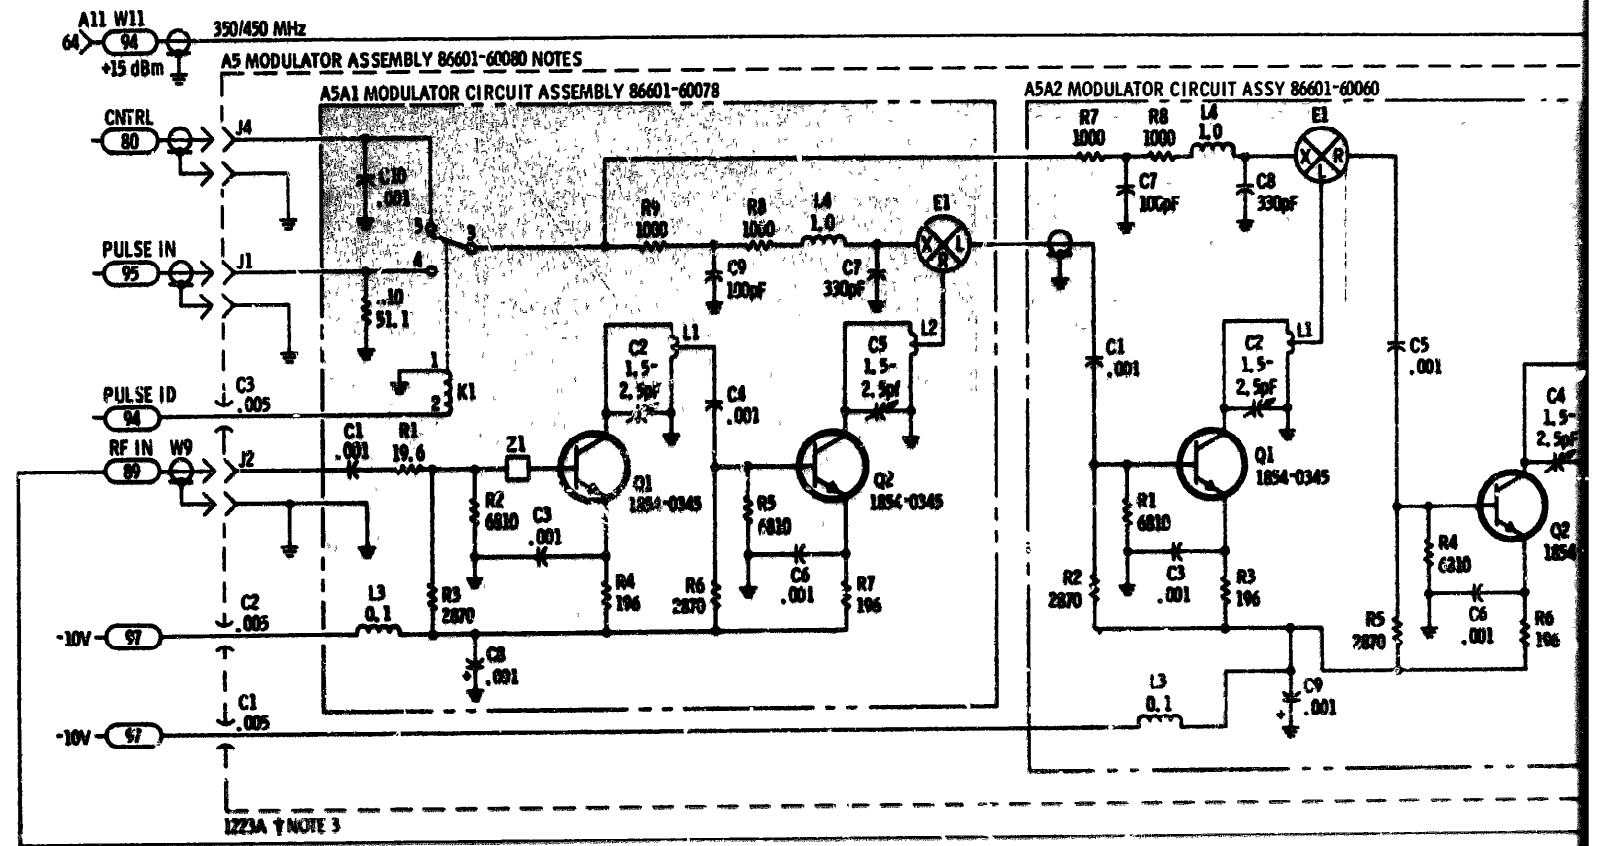


Figure 8-16. Modulator Assembly Component Locations



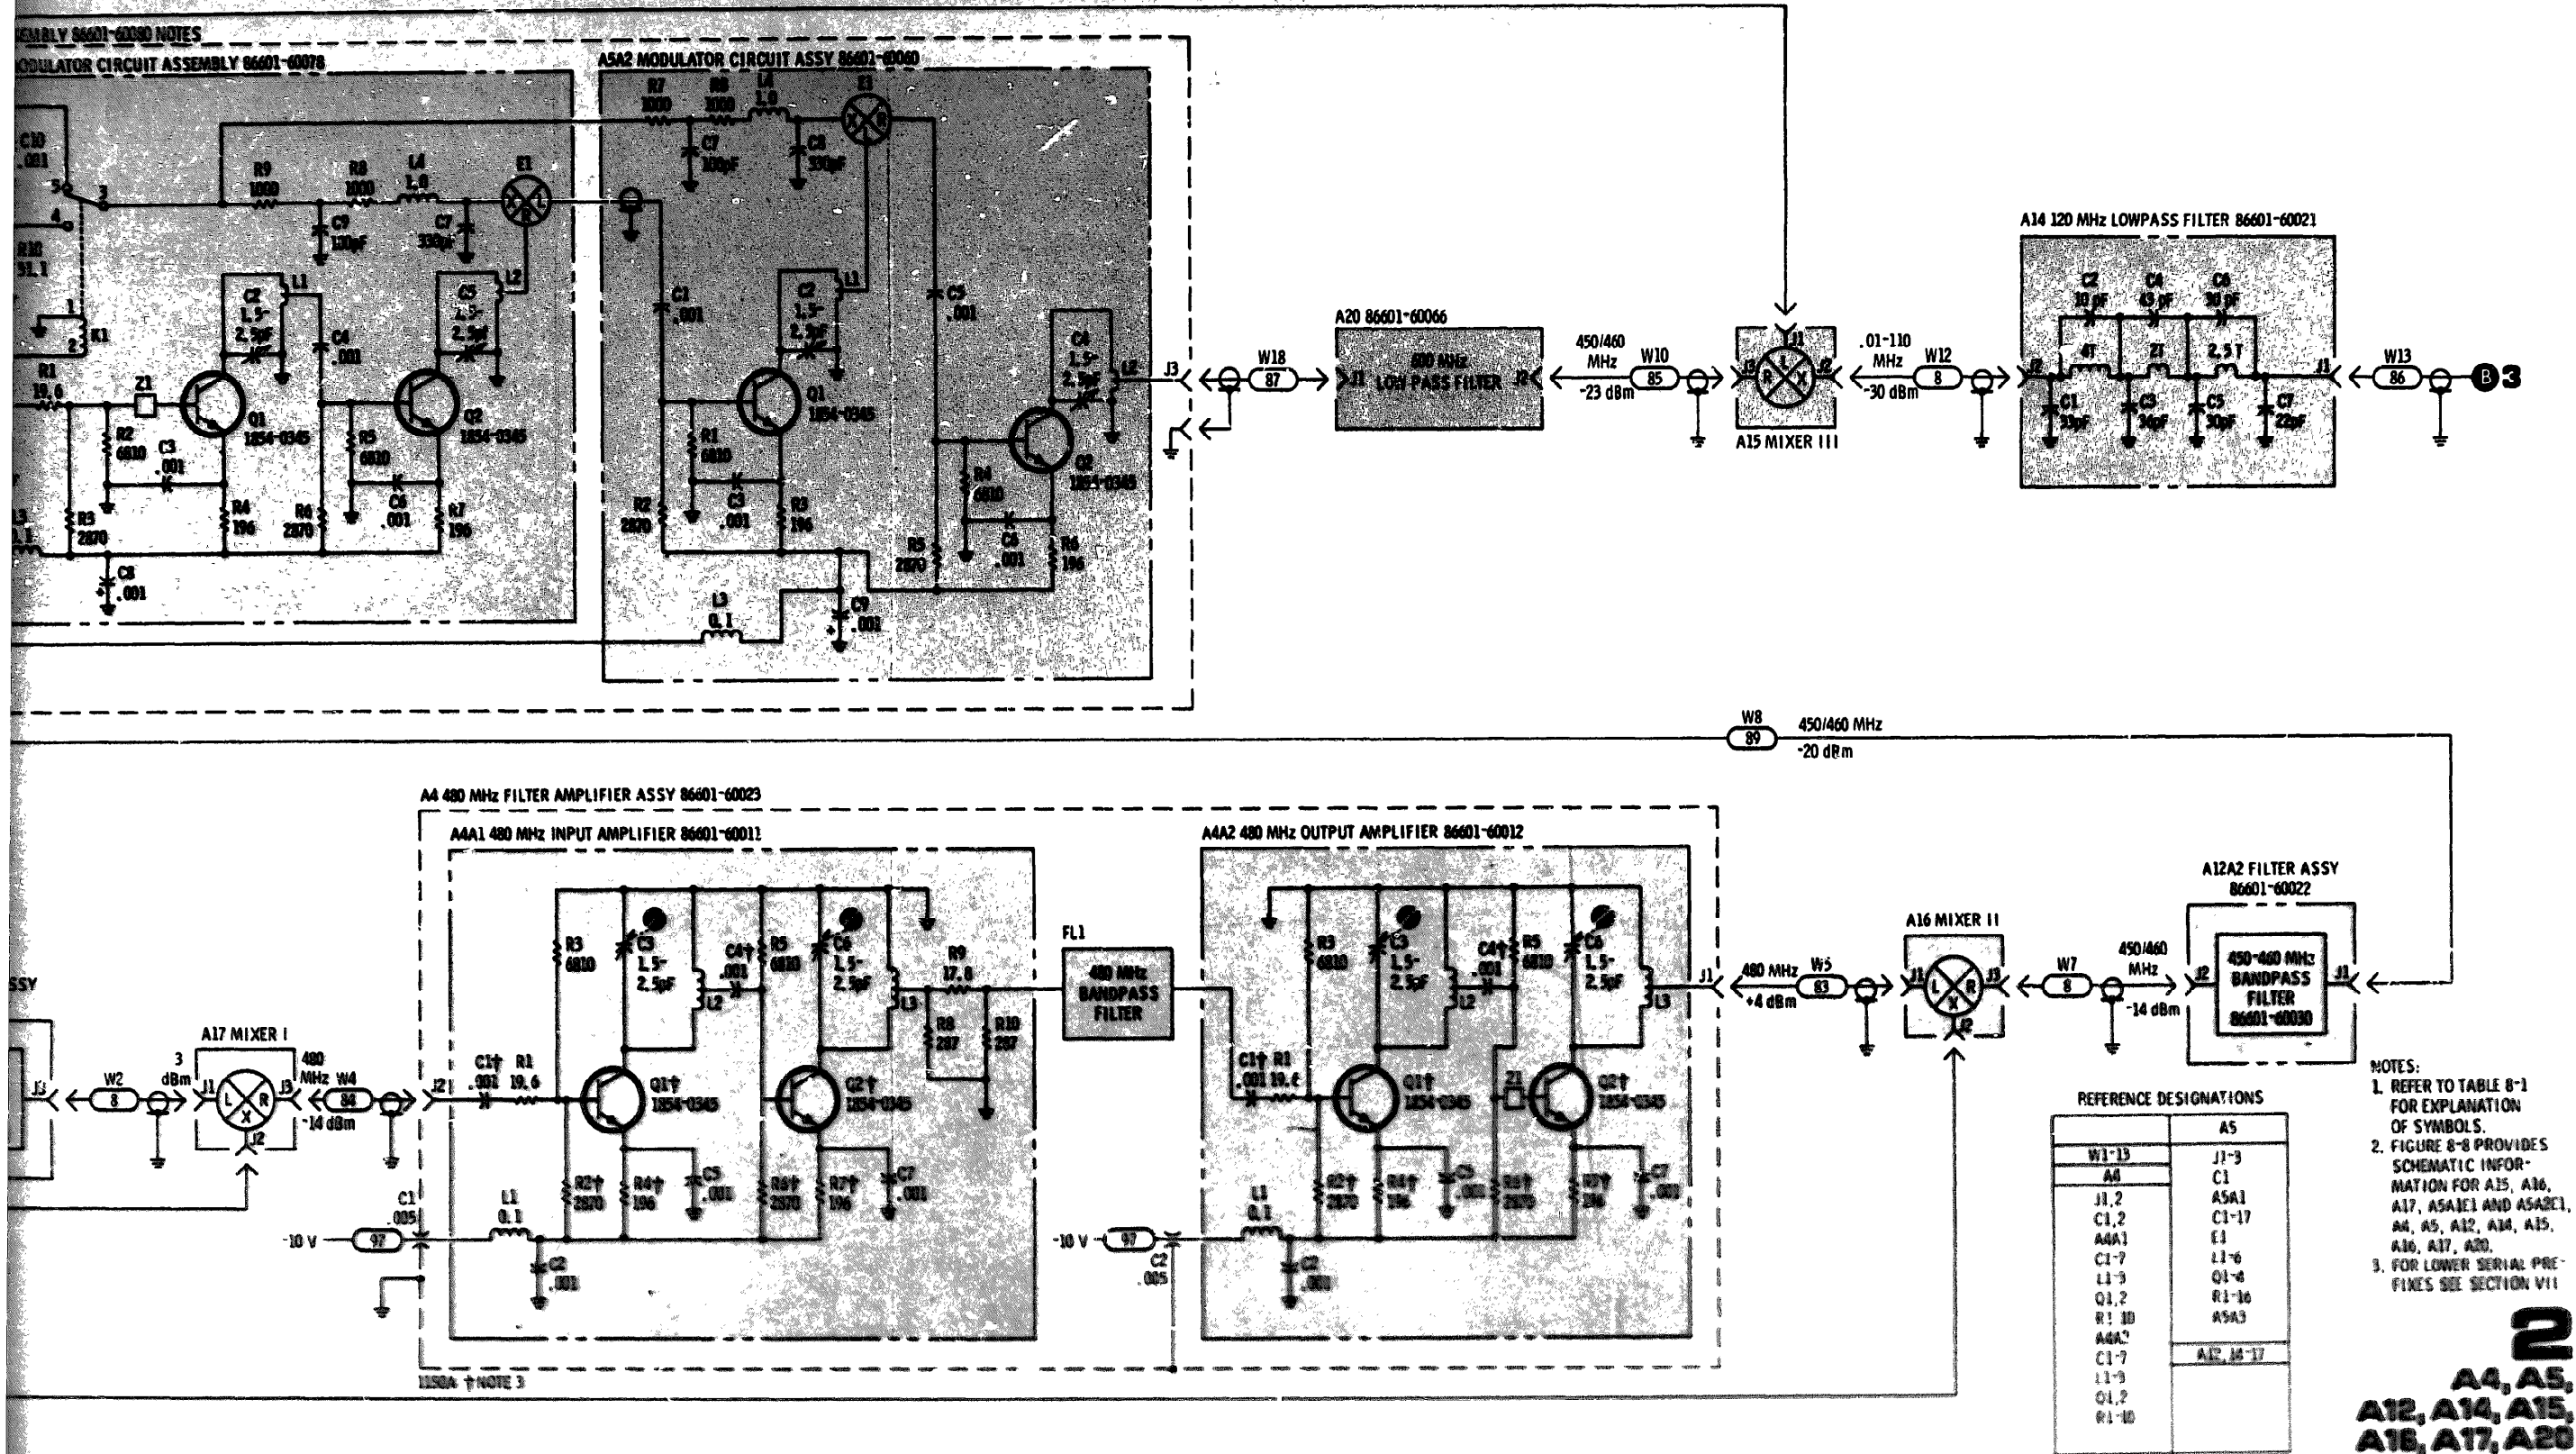


Figure 8-17. Filters, Mixers and Modulator Schematic

SERVICE SHEET 3

PREAMPLIFIER AND POWER AMPLIFIER ASSEMBLIES

Normally, the cause of a malfunction in the Model 86601A will be isolated to a circuit board or assembly as a result of performing the tests specified in the troubleshooting tree.

When trouble is traced to the A6 or A2 assemblies remove the defective assembly from the housing and reconnect the dc and rf inputs and outputs to provide access to test points and components. Be sure to use an insulating material between the circuit board and chassis to prevent short circuits.

TEST EQUIPMENT REQUIRED: (See Table 1-2.)

Digital Voltmeter
Counter
Spectrum Analyzer
Low Voltage DC Power Supply

PREAMPLIFIER ASSEMBLY A6

The rf signal from the A14 120 MHz Low Pass Filter is coupled to the base of Q1 through another 120 MHz Low Pass Filter (L2, 3, 4; C2, 3) and a peaking circuit (R4, C5).

The output of Q1 is amplified by Q2 and applied to the base of emitter-follower Q3. The signal at the emitter of Q2 provides a feedback bias to aid in leveling the flatness of the amplifier over the frequency range.

The output of emitter-follower Q3 is coupled through R14 and C13 to the input of the power amplifier assembly A2. The gain of the A6 preamplifier assembly is about 30 dB.

POWER AMPLIFIER AND AGC ASSEMBLY A2

The rf signal from the preamplifier is coupled through C1 to the base of emitter-follower Q1. The signal from Q1 is used to drive complementary symmetry amplifier Q2/Q3. The output of Q2/Q3 provides:

- A feedback signal to optimize flatness of the output signal.
- The rf output to the 150 dB programmable attenuator.
- The signal to drive the Automatic Gain Control Circuit (AGC).

Q4 and Q5 couple the rf signal to detector CR2/CR3 and also provides isolation between the AGC circuits and the rf output.

When the output frequency of the Model 86601A is above 4 MHz, transistors Q6 through Q11 have no effect on AGC operation. The effective time constant of the detector circuit is controlled solely by R23/C18 and R24/C23.

When the output frequency of the Model 86601A is between 400 kHz and 4 MHz, the Code 1 input from the mainframe DCU is high (about +3V) and Q7 is turned on to provide a ground

SERVICE SHEET 3 (cont'd)

return for C22. The Code 1 signal also turns off Q10 to turn on Q11 and provide a ground return for C21. With C21 and C22 in the circuit the effective time constant is enlarged to improve the response of the detector circuit.

When an output rf signal below 400 kHz is selected the Code 2 input also goes high. This high level turns on Q8 to provide a ground return for C19. Q9 is turned off to turn on Q6 which provides a ground return for C17. The effective time constant of the detector is again increased to improve the response of the AGC circuit for the lower frequency signals.

The output of emitter-follower Q13 is applied across a voltage divider and the desired output level is controlled by R31. C24 and C25 by-pass remaining rf signals to ground.

NOTES

- Verify the presence of dc operating voltages before taking other measurements. If dc voltages are not present, check connections to the mainframe. If the interconnections are good, refer to the mainframe manual and make repairs as required.
- Unless otherwise specified, all measurements are taken with the Spectrum Analyzer.
- If repairs are made in any part of the circuits shown on Service Sheet 3, the appropriate adjustment procedures in Section V of this manual should be performed.
- These procedures assume that the cause of malfunction has been isolated to the A2 or A6 assembly as a result of performing the tests specified in the troubleshooting tree.

TEST PROCEDURE 0

Test 1-a. Use the Spectrum Analyzer to trace the input signal to the defective stage in the A6 assembly and repair as required.

SERVICE SHEET 3 (cont'd)

TEST PROCEDURE 1

If the rf output is low, or not present at all, at the RF connector on the A2 assembly proceed to test 2-a. If output level flatness is not correct at low frequencies proceed to test 2-b.

Test 2-a. Use the Spectrum Analyzer to trace the input signal to the defective stage and repair as required.

Test 2-b. Recheck the code 1 and code 2 inputs at the assembly.

Frequency	Code 1	Code 2
> 4 MHz	< 150 mV	< 150 mV
> .4 MHz < 4 MHz	> +3 v	< 150 mV
< .4 MHz	> +3 v	> +3 v

If code 1 and code 2 levels are not as specified recheck inputs from the mainframe. If the inputs from the mainframe are not present refer to the mainframe manual and repairs as required.

If code 1 and code 2 signals are present and the rf flatness is as specified above 4 MHz but is not as specified below 4 MHz, proceed to Test 2-c. If the code 1 and code 2 signals are present and the rf flatness is as specified above .4 MHz but below .4 MHz, proceed to Test 2d. If the rf output flatness is also incorrect above 4 MHz, proceed to Test 2-e.

Test 2-c. Check Q7, Q10, Q11 and associated components. Q8 and Q11 should be on (saturated), and Q10 should be off.

Test 2-d. Check Q8, Q9, Q6 and associated components. Q8 should be on (saturated) and Q9 should be off.

Test 2-e. Disconnect the DET OUT and reconnect it using the connector. Connect the digital voltmeter to the third terminal and monitor the dc level of the AGC signal. With the rf set to +13 dBm the digital voltmeter should indicate approximately -2.6V. With the VERNIER control set to 10 dBm on the Model 86601A meter the digital voltmeter should indicate approximately -0.6V.

If the AGC dc levels are not as specified perform the appropriate adjustment procedures in Section V of this manual.

If the adjustment procedures do not eliminate the problem check Q4, Q5, Q12, Q13 and associated components.

SERVICE SHEET 3 (cont'd)

return for C22. The Code 1 signal also turns off Q10 to turn on Q11 and provide a ground return for C21. With C21 and C22 in the circuit the effective time constant is enlarged to improve the response of the detector circuit.

When an output rf signal below 400 kHz is selected the Code 2 input also goes high. This high level turns on Q8 to provide a ground return for C19. Q9 is turned off to turn on Q6 which provides a ground return for C17. The effective time constant of the detector is again increased to improve the response of the AGC circuit for the lower frequency signals.

The output of emitter-follower Q13 is applied across a voltage divider and the desired output level is controlled by R31. C24 and C25 by-pass remaining rf signals to ground.

NOTES

1. Verify the presence of dc operating voltages before taking other measurements. If dc voltages are not present, check connections to the mainframe. If the interconnections are good, refer to the mainframe manual and make repairs as required.
2. Unless otherwise specified, all measurements are taken with the Spectrum Analyzer.
3. If repairs are made in any part of the circuits shown on Service Sheet 3, the appropriate adjustment procedures in Section V of this manual should be performed.
4. These procedures assume that the cause of malfunction has been isolated to the A2 or A6 assembly as a result of performing the tests specified in the troubleshooting tree.

TEST PROCEDURE

Test 1-a. Use the Spectrum Analyzer to trace the input signal to the defective stage in the A6 assembly and repair as required.

SERVICE SHEET 3 (cont'd)**TEST PROCEDURE**

If the rf output is low, or not present at all, at the RF OUT connector on the A2 assembly proceed to test 2-a. If the rf output level flatness is not correct at low frequencies proceed to test 2-b.

Test 2-a. Use the Spectrum Analyzer to trace the input signal to the defective stage and repair as required.

Test 2-b. Recheck the code 1 and code 2 inputs at the A2 assembly.

Frequency	Code 1	Code 2
> 4 MHz	< 150 mV	< 150 mV
> .4 MHz < 4 MHz	> +3 V	< 150 mV
< .4 MHz	> +3 V	> +3 V

If code 1 and code 2 levels are not as specified recheck the inputs from the mainframe. If the inputs from the mainframe are not present refer to the mainframe manual and repair as required.

If code 1 and code 2 signals are present and the rf output flatness is as specified above 4 MHz but is not as specified below 4 MHz, proceed to Test 2-c. If the code 1 and code 2 signals are present and the rf flatness is as specified above .4 MHz but not below .4 MHz, proceed to Test 2-d. If the rf output flatness is also incorrect above 4 MHz, proceed to Test 2-e.

Test 2-c. Check Q7, Q10, Q11 and associated components. Q7 and Q11 should be on (saturated), and Q10 should be off.

Test 2-d. Check Q8, Q9, Q6 and associated components. Q6 and Q8 should be on (saturated) and Q9 should be off.

Test 2-e. Disconnect the DET OUT and reconnect it using a Tee connector. Connect the digital voltmeter to the third Tee port and monitor the dc level of the AGC signal. With the rf output set to +13 dBm the digital voltmeter should indicate approximately -2.6V. With the VERNIER control set for a reading of -10 dBm on the Model 86601A meter the digital voltmeter should indicate approximately -0.6V.

If the AGC dc levels are not as specified perform the applicable adjustment procedures in Section V of this manual.

If the adjustment procedures do not eliminate the problem check Q4, Q5, Q12, Q13 and associated components.

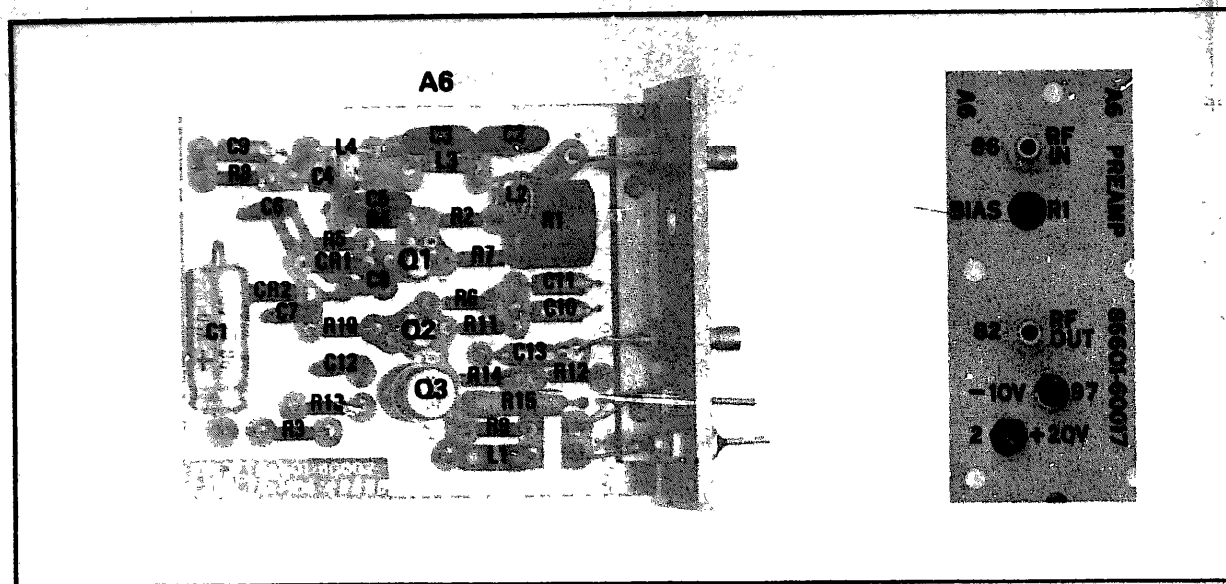


Figure 8-18. Preamplifier Component Locations



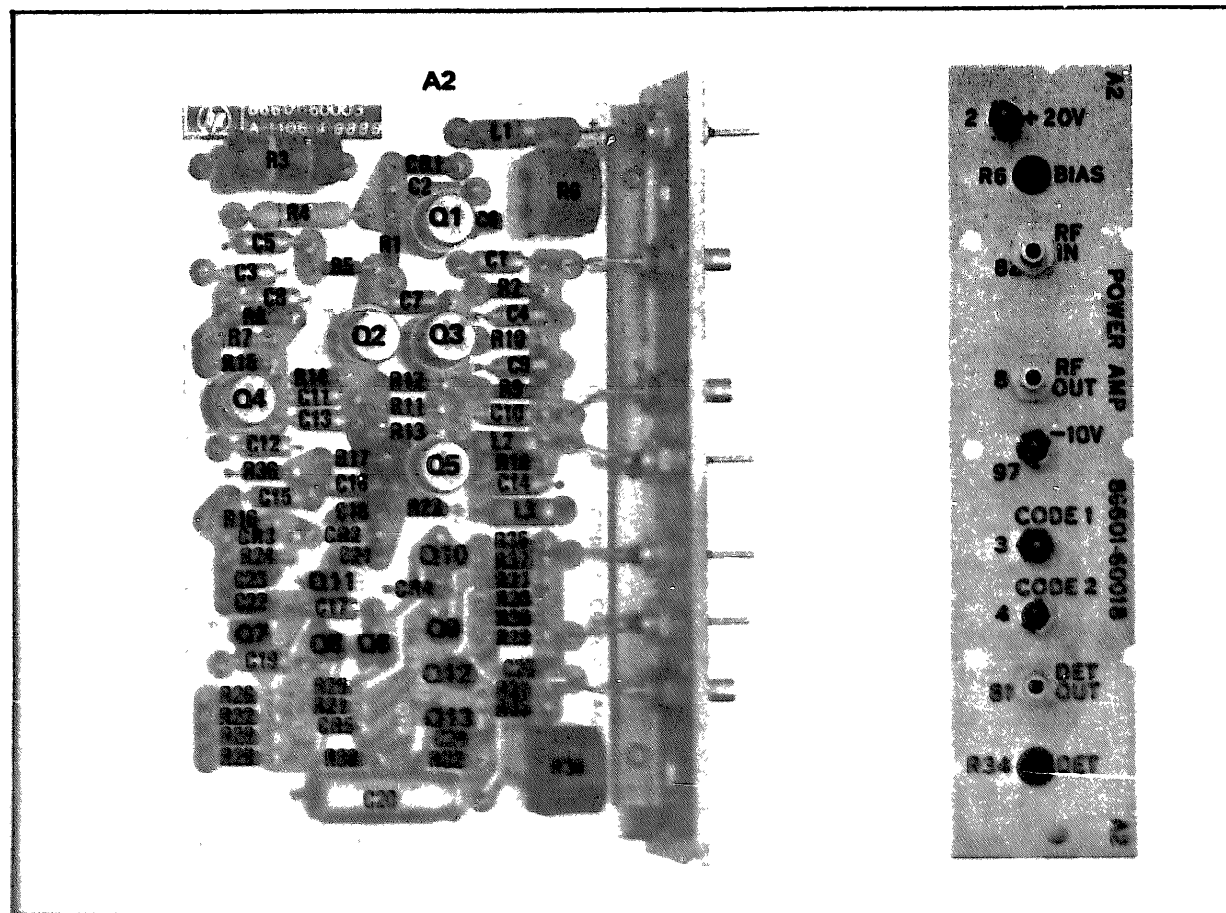


Figure 8-19. Power Amplifier and AGC Component Locations



REFERENCE DESIGNATIONS

W13-16	A2
A6	C1-29
C1-15	CR1-4
CR1,2	L1-3
L1-4	Q1-13
Q1-3	R1-38
R1-15	

NOTES:
1. REFER TO TABLE 8-1 FOR EXPLANATION OF SYMBOLS

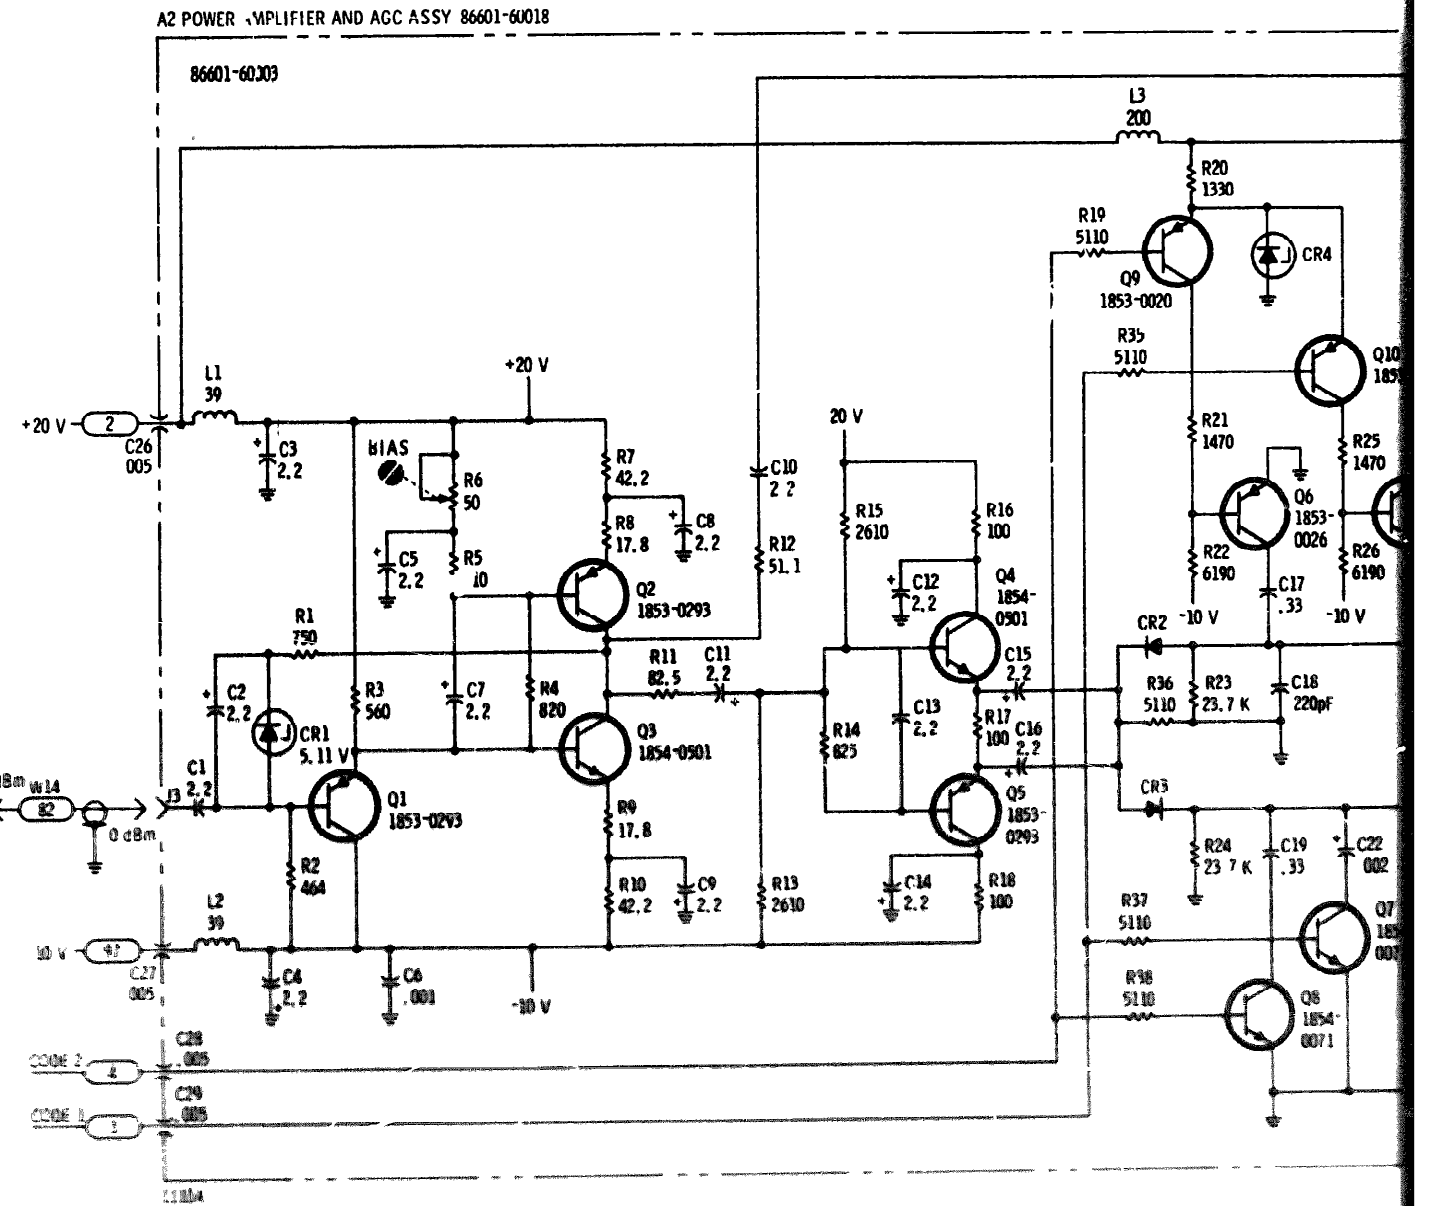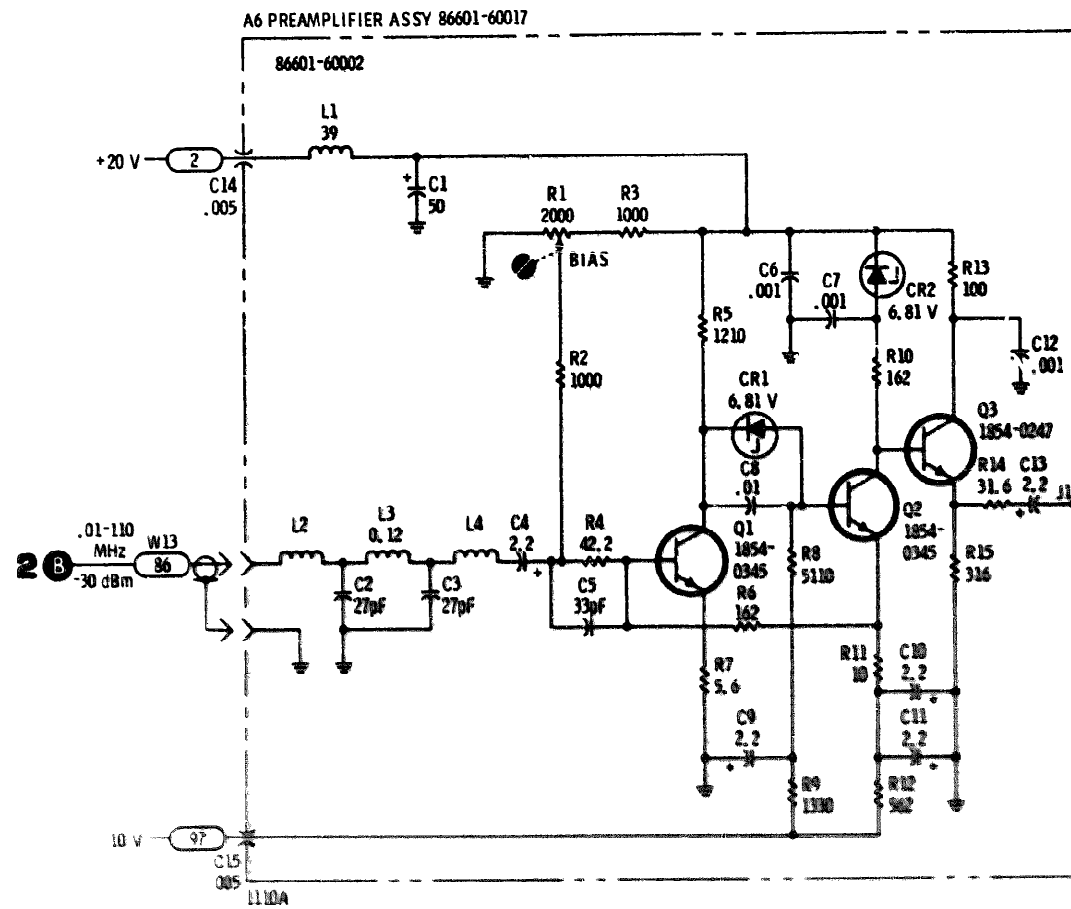


Service

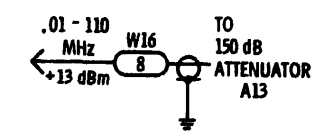

3
A2, A6

A2 POWER AMPLIFIER AND AGC ASSY 86601-60018

NOTES
1. REFER TO TABLE 8-1 FOR EXPLANATION OF SYMBOLS

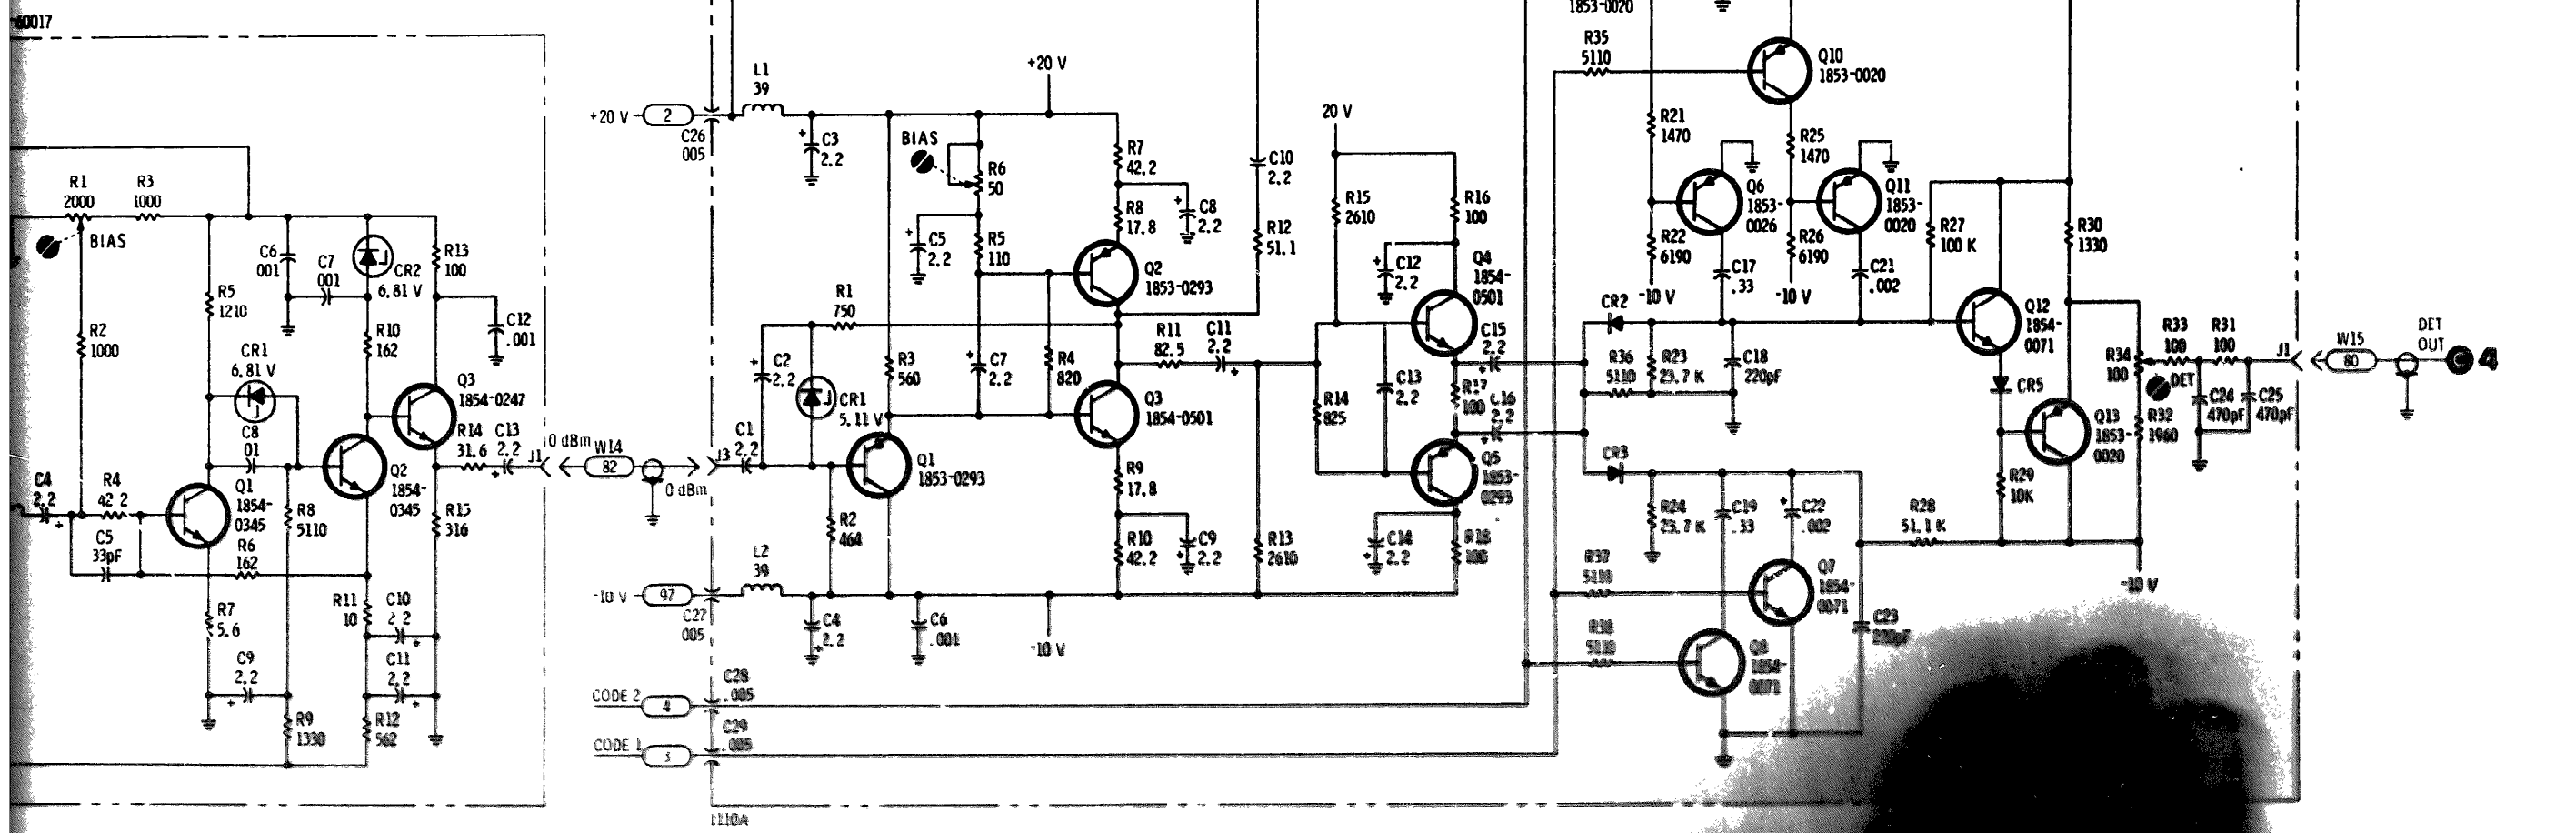

3
A2, A6

and PWE Amp Schematics

SERVICE SHEET 4

Normally, the cause of a malfunction in the Model 86601A will be isolated to a circuit board or assembly as a result of performing the tests specified in the troubleshooting tree.

When the cause of trouble has been isolated to the A3 assembly, it must be removed from the well and reconnected to provide access to test points and components.

When the cause of trouble has been isolated to the A9 assembly it may be extended for maintenance with an extender board.

TEST EQUIPMENT REQUIRED

Digital Voltmeter
Marked Card Programmer
Spectrum Analyzer

Extender Cable
Power Supply

NOTE

A voltage designated as a high in this text will be $> +2.2V$ unless otherwise noted and a low will be $< +0.8V$.

REFERENCE AMPLIFIER ASSEMBLY A9

The output rf level from the A2 Power Amplifier is controlled by a dc reference from the A9 assembly.

The voltage source for the reference level is operational amplifier U1. When the instrument is in the CW mode the source voltage is $-2V$. The dc level at the output of U1 is coupled to the feedback amplifier, A3, in one of two ways.

In local operation the LCL/RMT input (XA9 pin A) is high. Q2 is turned off and Q1 is turned on to energize K6. The output of U1 is applied to a voltage divider network (R14, A1R1 and A1R2). The front panel VERNIER control (A1R1) is capable of controlling the rf output of the A2 power amplifier assembly from $+13$ dBm to 0 dBm. At an output rf level of $+13$ dBm the dc level to the feedback amplifier is $-1V$.

In remote operation the LCL/RMT input (XA9 pin A) is low. Q1 is turned off and Q2 is turned on to energize K5. The dc level to the A3 assembly is now controlled by K1 through K4 which are, in turn, controlled by the 1A, 2A, 4A, and 8A input lines. As an example, if the programmed output is $+13$ dBm, the inputs on 1A, 2A, 4A and 8A are all low; K1 through K4 are all energized and $-1V$ is coupled to the A3 assembly. If an output of $+12$ dBm is programmed in, input line 1A now goes high, Q9 is turned off, relay K1 is de-energized, and Q11 is turned on to provide a ground return for R10. Resistors R8, R10 and R11 reduce the reference level to the feedback amplifier by the amount required to ensure a 1 dB decrease of the rf output from the A2 power amplifier assembly.

Relays K2, K3, K4 and associated component, operate in the same manner as K1 except that the associated resistive networks are weighted to produce 2, 4 and 8 dB of attenuation to the A2 rf output.

The front panel rf output meter is functional in both local and remote modes. The DET output from A2 is filtered in the A3 assembly and then applied to the meter driver stage (Q10) in the A9 assembly.

SERVICE SHEET 4 (cont'd)

FEEDBACK AMPLIFIER ASSEMBLY A3

Differential amplifier U1 has as its inputs the negative dc reference from the reference assembly and the DET output of the A2 assembly. These two inputs are compared and the difference determines the output of U1 at pin 6.

The output from U1 is coupled through Q8 and Q9 to the modulator assembly (A6) where it is used as a gain control. This gain control level directly affects the A2 power amplifier rf and AGC output levels. When the rf output of the A2 assembly reaches the programmed level the loop is stabilized and the output of U1 is a steady dc level (CW mode).

In the AM mode the amplitude modulating signal is superimposed on the reference level from the AS assembly. The amplitude modulating signal also appears at the output of U1 and it is used to modulate the center frequency in the A5 assembly.

As long as the output frequency of the Model 86601A is greater than 4 MHz the frequency rolloff of the feedback amplifier is controlled by R15 and C9.

Code 1 and code 2 signals from the mainframe DCU alter the response time of the circuit in the following manner:

When the selected output frequency is below 4 MHz (but above 400 kHz), the code 1 line is high and Q7 is turned on to provide a ground return for C7. This increases the time constant of the circuit and improves the response at the selected frequency.

Note that Q1 is also turned on to provide a ground return for C6 to maintain leveling accuracy.

When an output frequency below 800 kHz is selected the code 2 line also goes high to turn on Q6. This provides a ground return for C8 to further increase the response time of the circuit.

The code 1 and code 2 levels ensure that the rf output level remains constant over the entire frequency range of the instrument.

NOTES

1. Verify the presence of dc operating voltages before taking other measurements. If dc voltages are not present, check connections to the mainframe. If interconnections are good refer to the mainframe manual and make necessary repairs.
2. After making repairs in either of the circuits shown, the adjustment procedure specified in Section V of this manual should be performed.
3. These procedures assume that the cause of malfunction has been isolated to the A3 or A9 assemblies as a result of performing the tests specified in the troubleshooting trees.

TEST PROCEDURE

One of the following conditions exists:

The Model 86601A rf output is present but the output meter does not operate properly - proceed to Test 1.

SERVICE SHEET 4 (cont'd)

The Model 86601A output level in local mode is properly controlled by the VERNIER control but remote 1 dB step programming is inaccurate - proceed to Test 1-c.

The Model 86601A output level is programmable but the VERNIER control does not properly control the output level - proceed to Test 1-d.

Neither the VERNIER control (local) or the 1 dB step attenuator (remote) operate properly - proceed to Test 1e.

Test 1-a. Extend the AS assembly from the chassis on an extender board. With the Model 86601A VERNIER and OUTPUT RANGE controls set for a $+13$ dBm output measure the dc level at XA9 pin K. The dc level should be about -550 mV. Set the Model 86601A output to -10 dBm. The dc level at XA9 pin K should be about -225 mV. If the voltage is not present proceed to Test 1-b.

If the dc levels at XA9 pin K are as specified use the digital voltmeter to check the dc level at XA7-2 pin 7. With the Model 86601A output set to $+13$ dBm the dc level should be about $+5.05$ V. Turn the VERNIER control full counterclockwise - the dc level should increase to about $+5.2$ V.

If the dc level at XA7-1 pin 7 is not present the meter or wiring to the $+5.25V$ input is defective.

If the dc level at XA7-2 pin 7 is present, but does not vary as the VERNIER control is rotated, Q10 or associated components are defective.

If the dc level at XA7-2 pin 7 is present and varies as the VERNIER control is rotated, but the Model 86601A output meter does not change, the meter is defective.

Test 1-b. Recheck for the dc levels specified for XA9 pin K at the white-orange MTR lead on the A3 assembly. If the levels are now present, check the interconnections to the A9 assembly. If the dc levels still are not present proceed to Test Procedure 2.

Test 1-c. In the local mode set the instrument for a 30 MHz $+13$ dBm output. Monitor the output with the spectrum analyzer and set the analyzer controls to display the peak of the signal at the top graticule line.

In the remote mode program 1, 2, 4 and 8 dB steps of attenuation. Observe the Model 86601A output meter and the analyzer display. If one or more of the steps do not produce the desired results check the logic levels at XA9 pins E, F, H and/or J against the levels shown in Table 8-3. If these levels are correct, one or more of the relay/relay driver circuits is defective. Example: If the 1 dB step is defective, check Q9, Q11, K1 and associated components.

If the logic levels at XA9 pins E, F, H and J are not correct, trouble is in the logic circuit (see Service Sheet 5), the mainframe, or the programming device.

SERVICE SHEET 4 (cont'd)

Table 8-3. 1dB Attenuation Checks

Attenuation (dB)	XA9 Pins			
dB	E	F	H	J
0	L	L	L	L
1	L	L	L	H
2	L	L	H	L
3	L	L	H	H
4	L	H	L	L
5	L	H	L	H
6	L	H	H	L
7	L	H	H	H
8	H	L	L	L
9	H	L	L	H

Test 1-d. With the instrument turned on in the local mode check for continuity between XA9 pins 10 and L. If a direct short does not exist between these pins check Q1 and K6.

If the direct short between XA9 pins 10 and L is present check A9R14, A1R1, A1R2 and interconnections.

Test 1-e. Perform the adjustment procedures specified in paragraphs 5-14 and 5-15. If the adjustments cannot be made A9U is probably defective.

TEST PROCEDURE

Test 2-a. Disconnect the input from CNTRL IN. Connect a low voltage power supply through a 1000 ohm resistor to CONTROL IN (-ground). With the front panel VERNIER control set full clockwise adjust the power supply for a +13 dBm output.

Measure the voltage at U1 pin 3 (-0.8V) and U1 pin 4 (0.9V). If the voltages are correct, proceed to test 2-b.

If the level at U1 pin 4 is incorrect refer to Service Sheet 3.

If the level at U1 pin 3 is incorrect, refer to TEST PROCEDURE 1 of this Service Sheet.

Test 2-b. Measure the voltage at U1 pin 6 (should be approximately 850 mV). If the voltage is correct, check Q8, Q9 and associated components. If the voltage is incorrect, check U1 and associated components.

Test 2-c. Verify that the rf output meter is tracking the DET output to the meter driver at XA7-2 pin 8.

Set the front panel VERNIER control for output meter readings of 1.0V, 0.6V, and 0.2V. The dc level at XA7-2 pin 8 should be $-0.6 \pm 0.1V$, $-0.35 \pm 0.1V$ and $-0.1 \pm .05V$ respectively.

Repeat the tests with the rf output set to 4.1, 2.1 and 0.1 MHz. The dc levels specified at XA7-2 pin 8 should be the same at all three frequencies; if they are not, determine which code line is not functioning properly and check the associated transistor switching circuit.

A2, A6 Pre-amplifier and Power Amplifier Assemblies

SERVICE SHEET 3

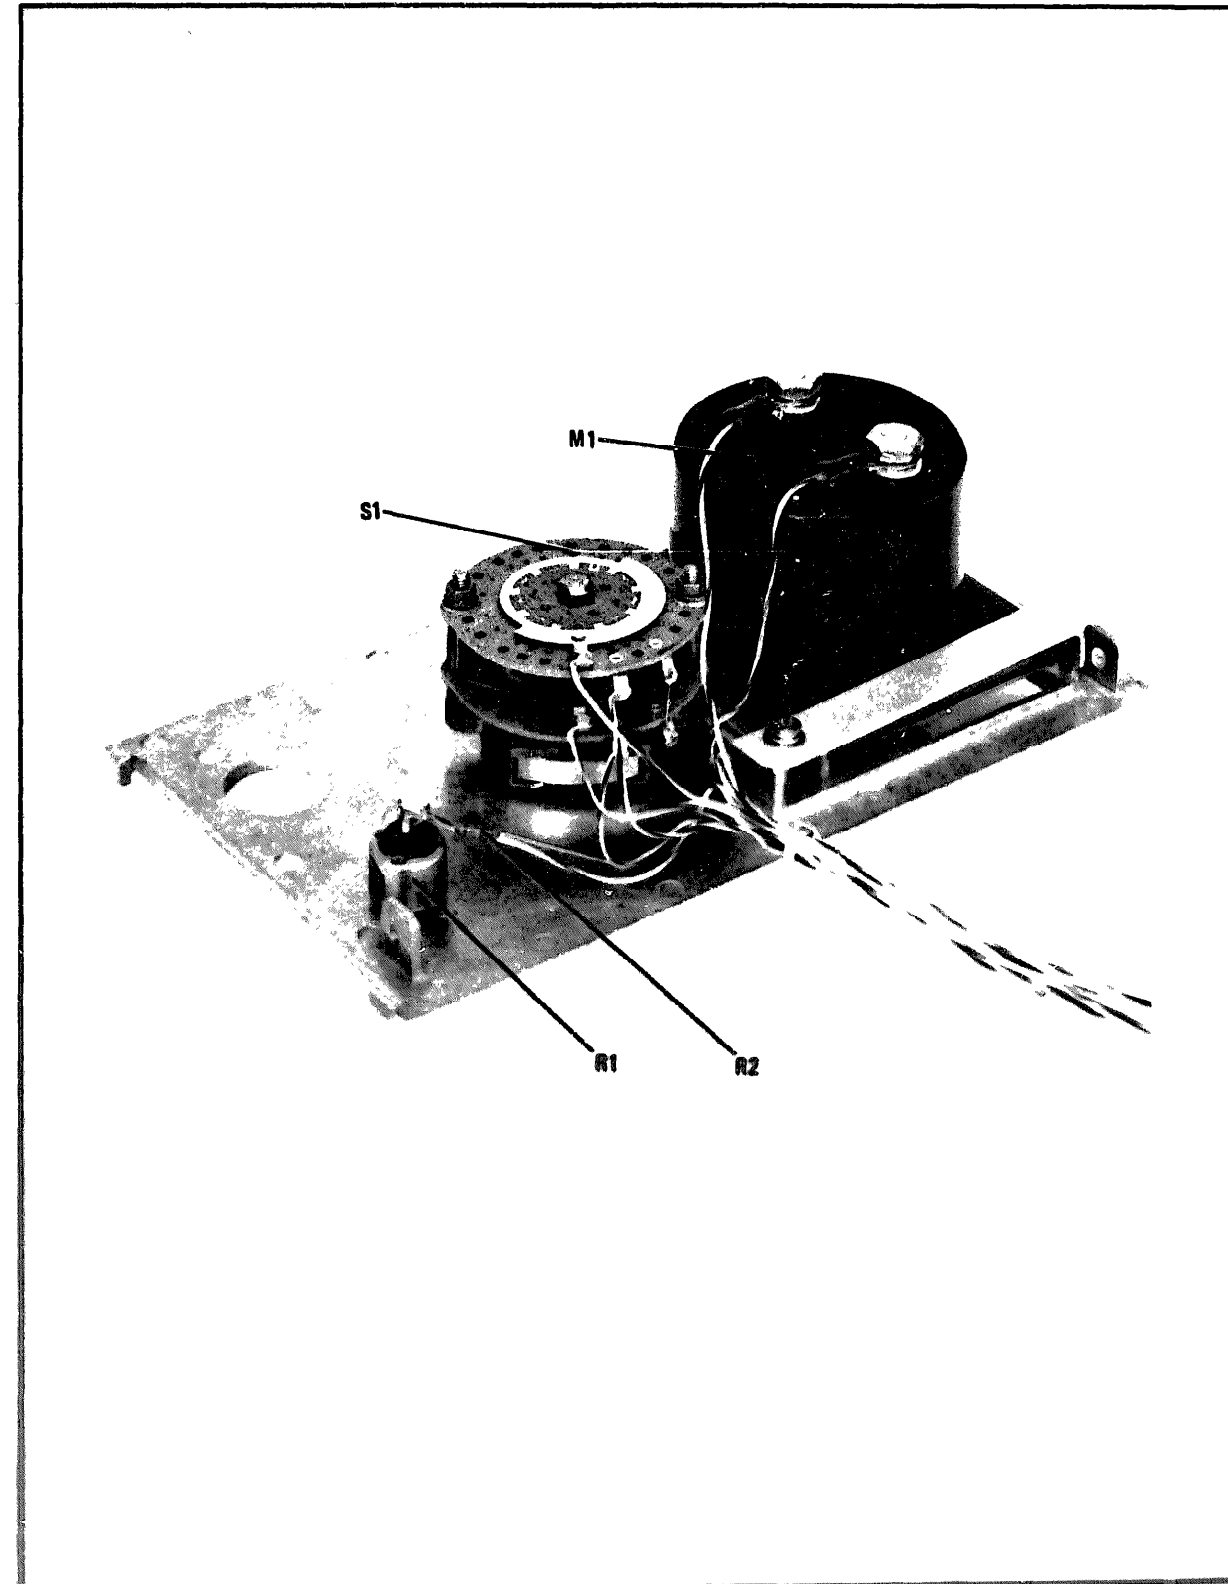


Figure 8-21. Front Panel Component Locations

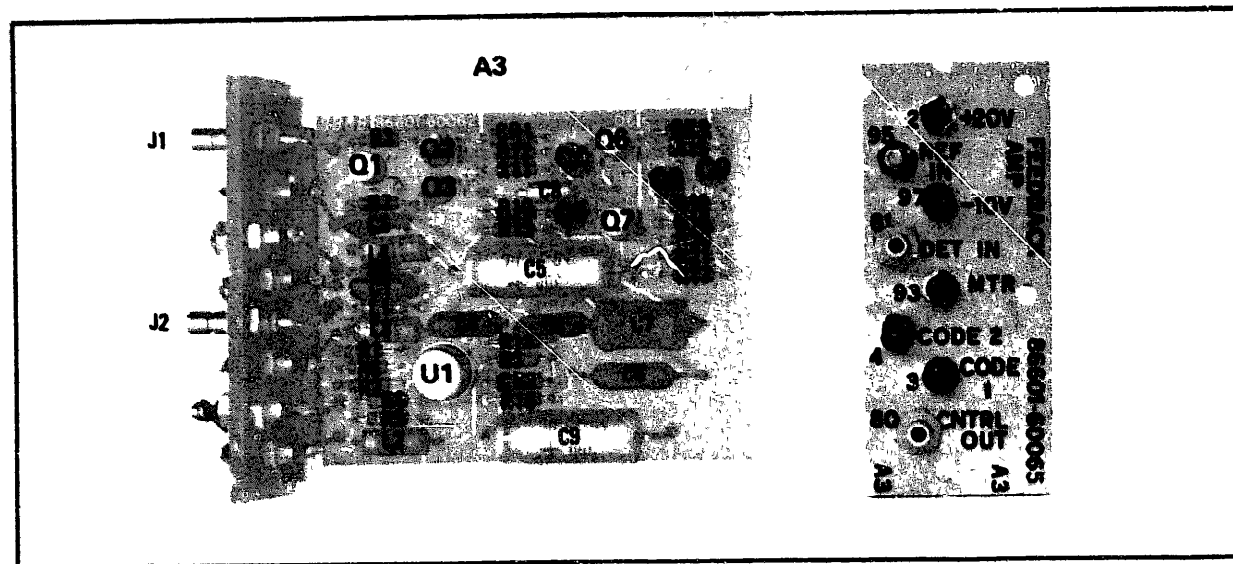


Figure 8-22. Feedback Amplifier Component Locations

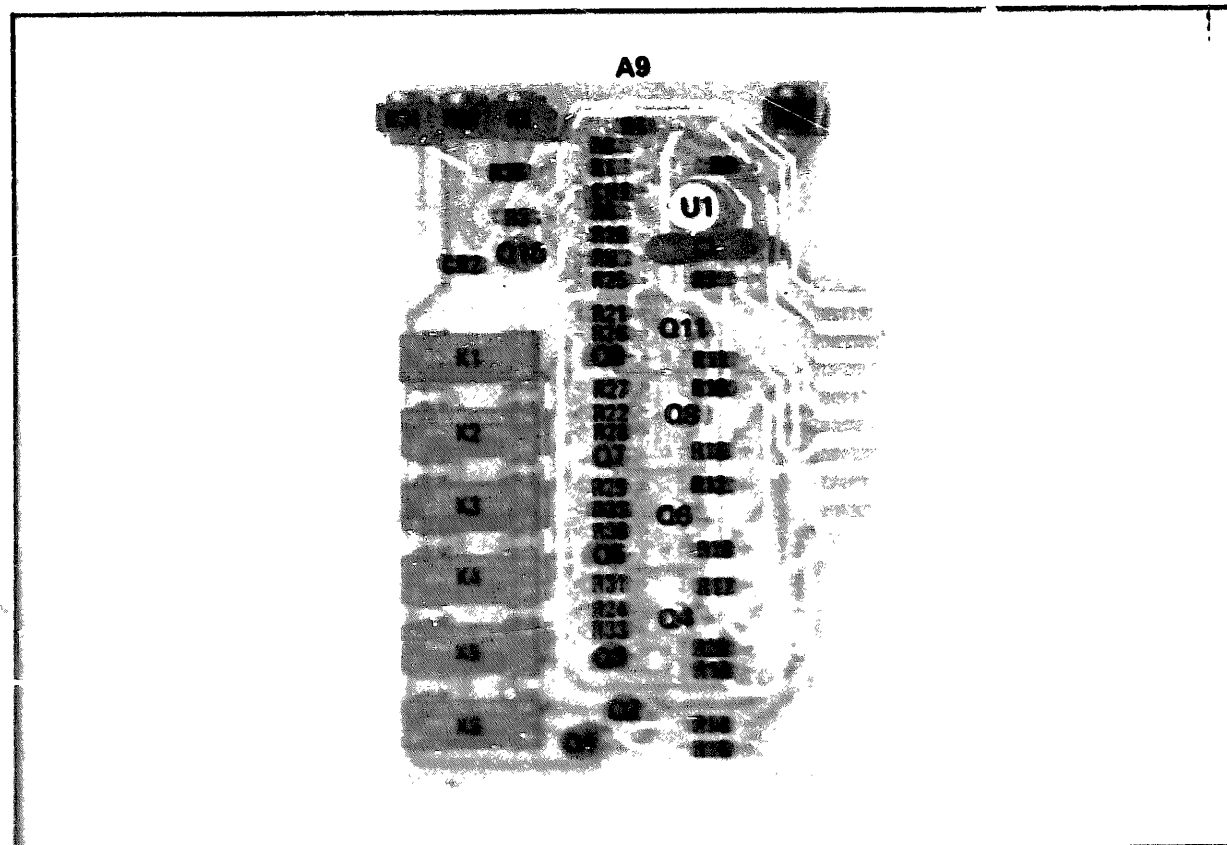


Figure 8-23. Reference Assembly Component Locations

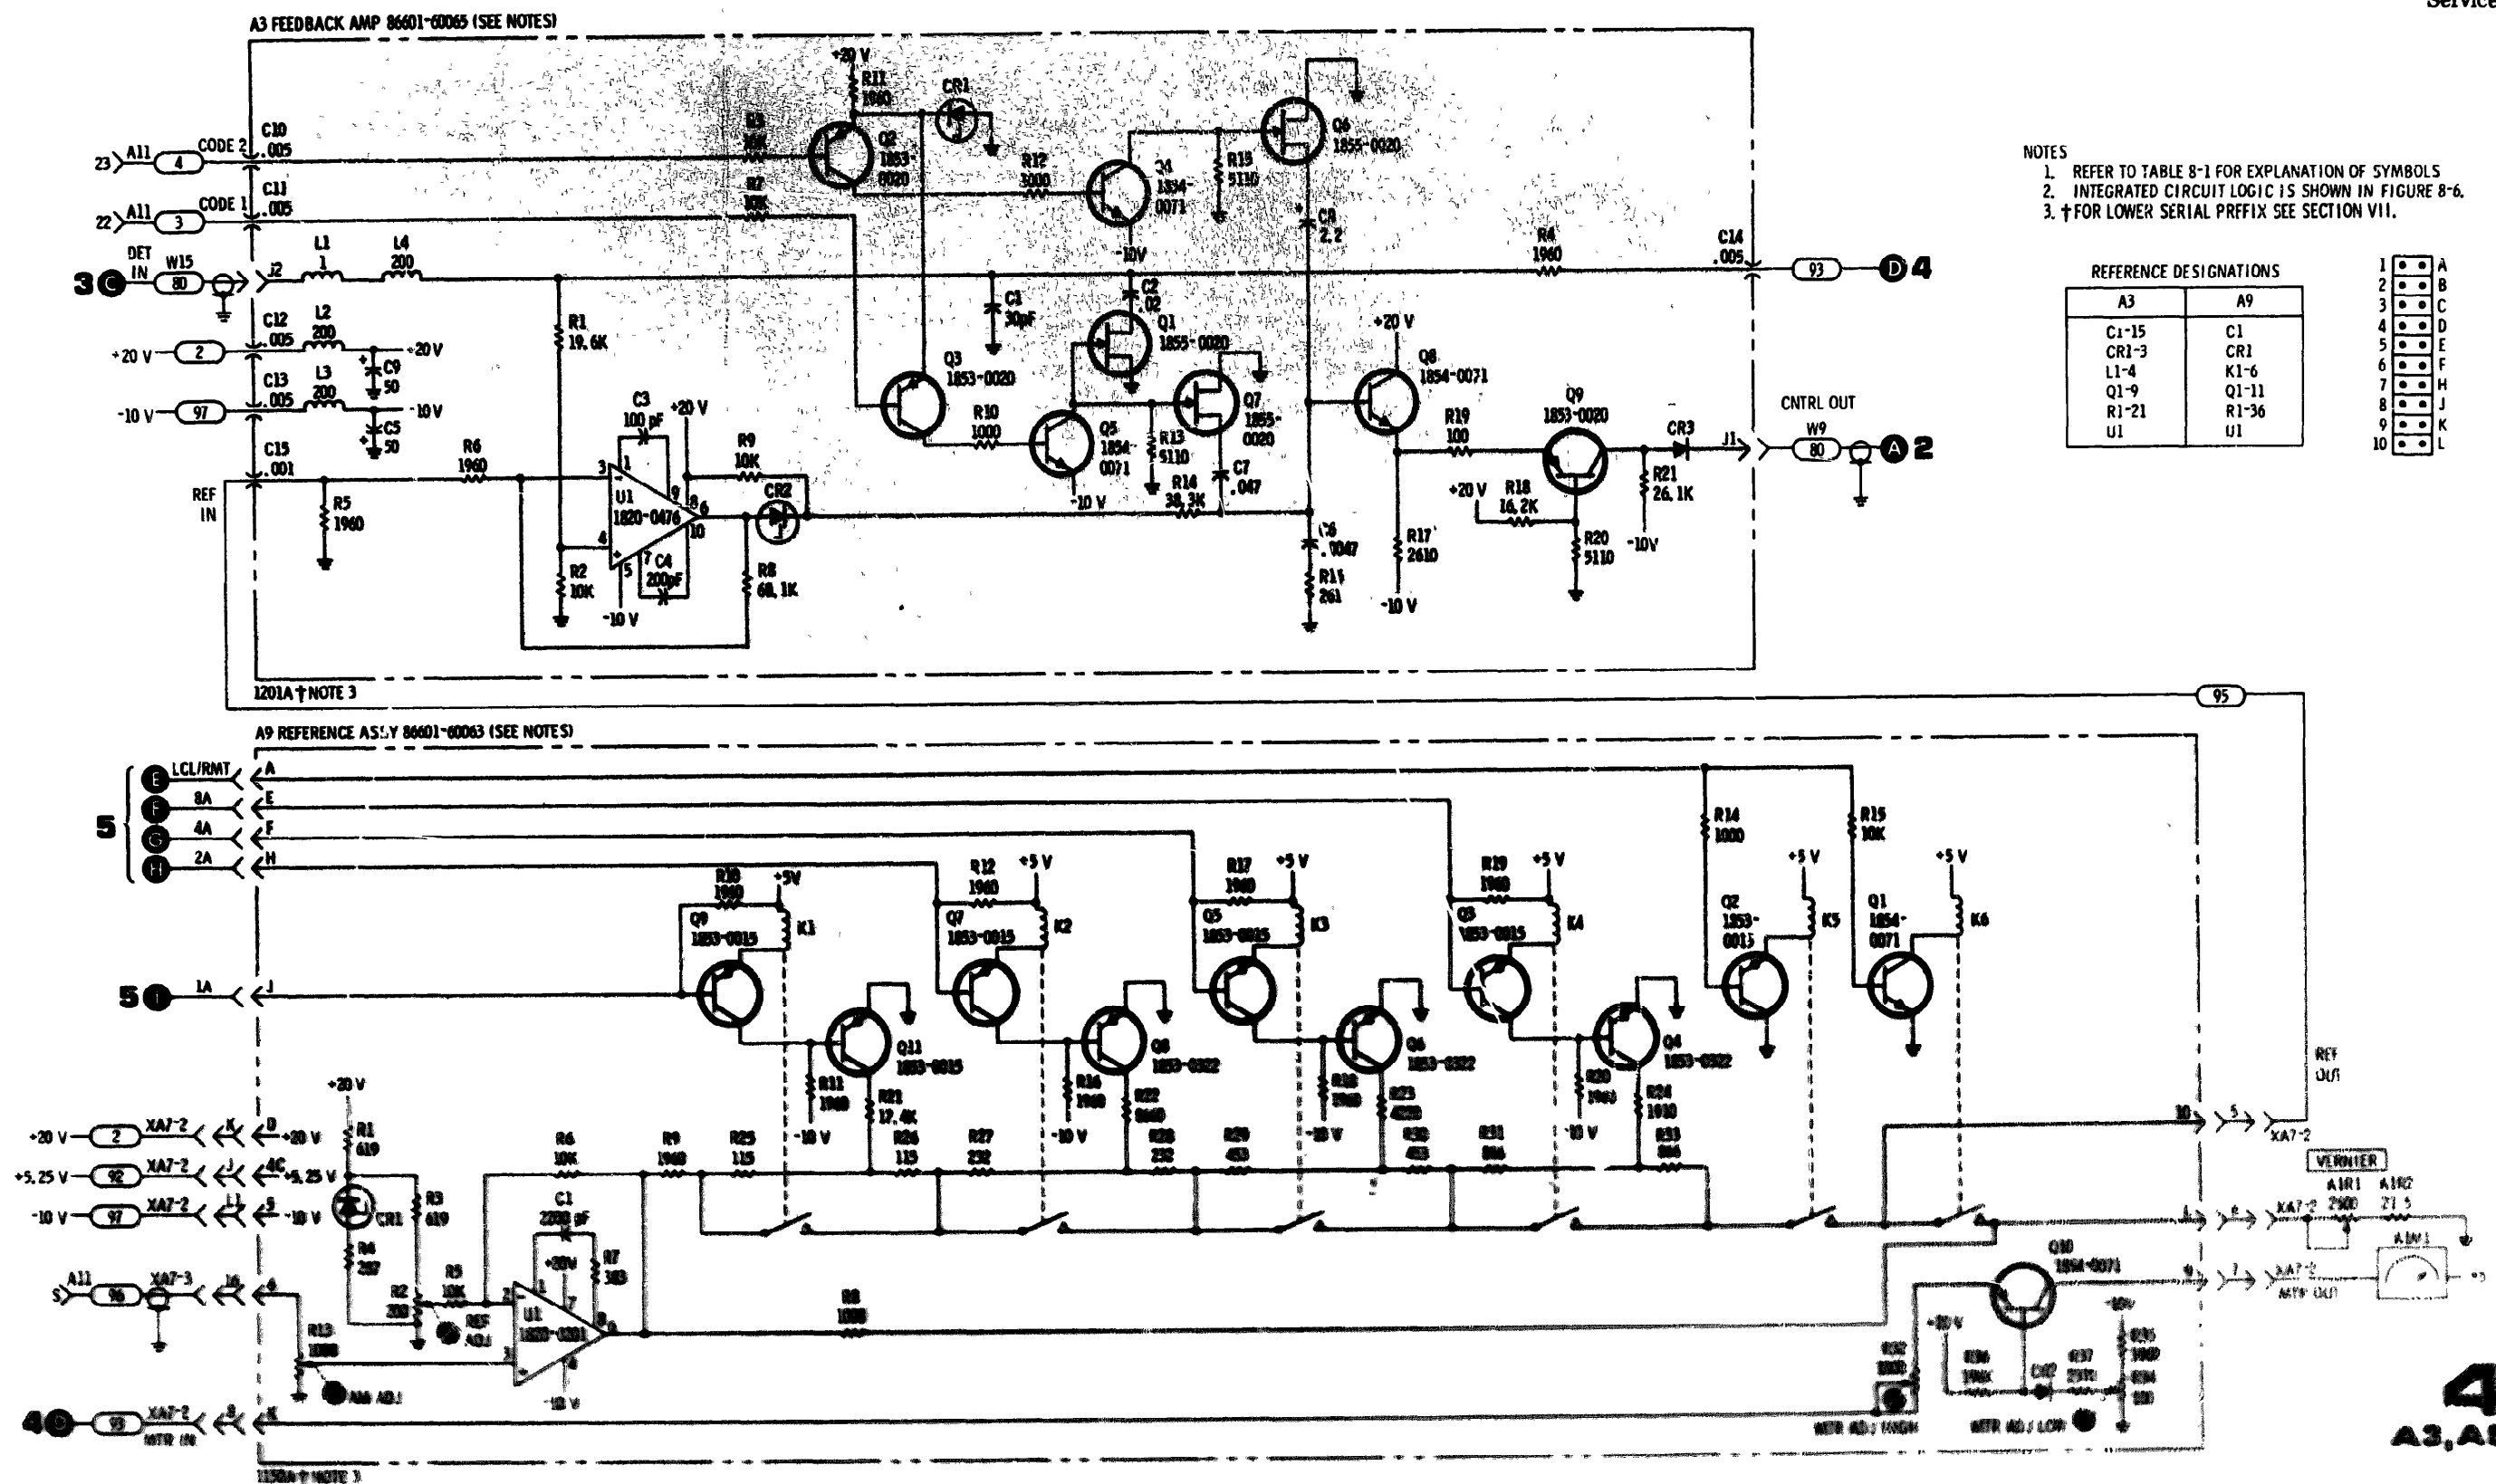


Figure 8-24 Feedback Amplifier and Reference Assy Schematic

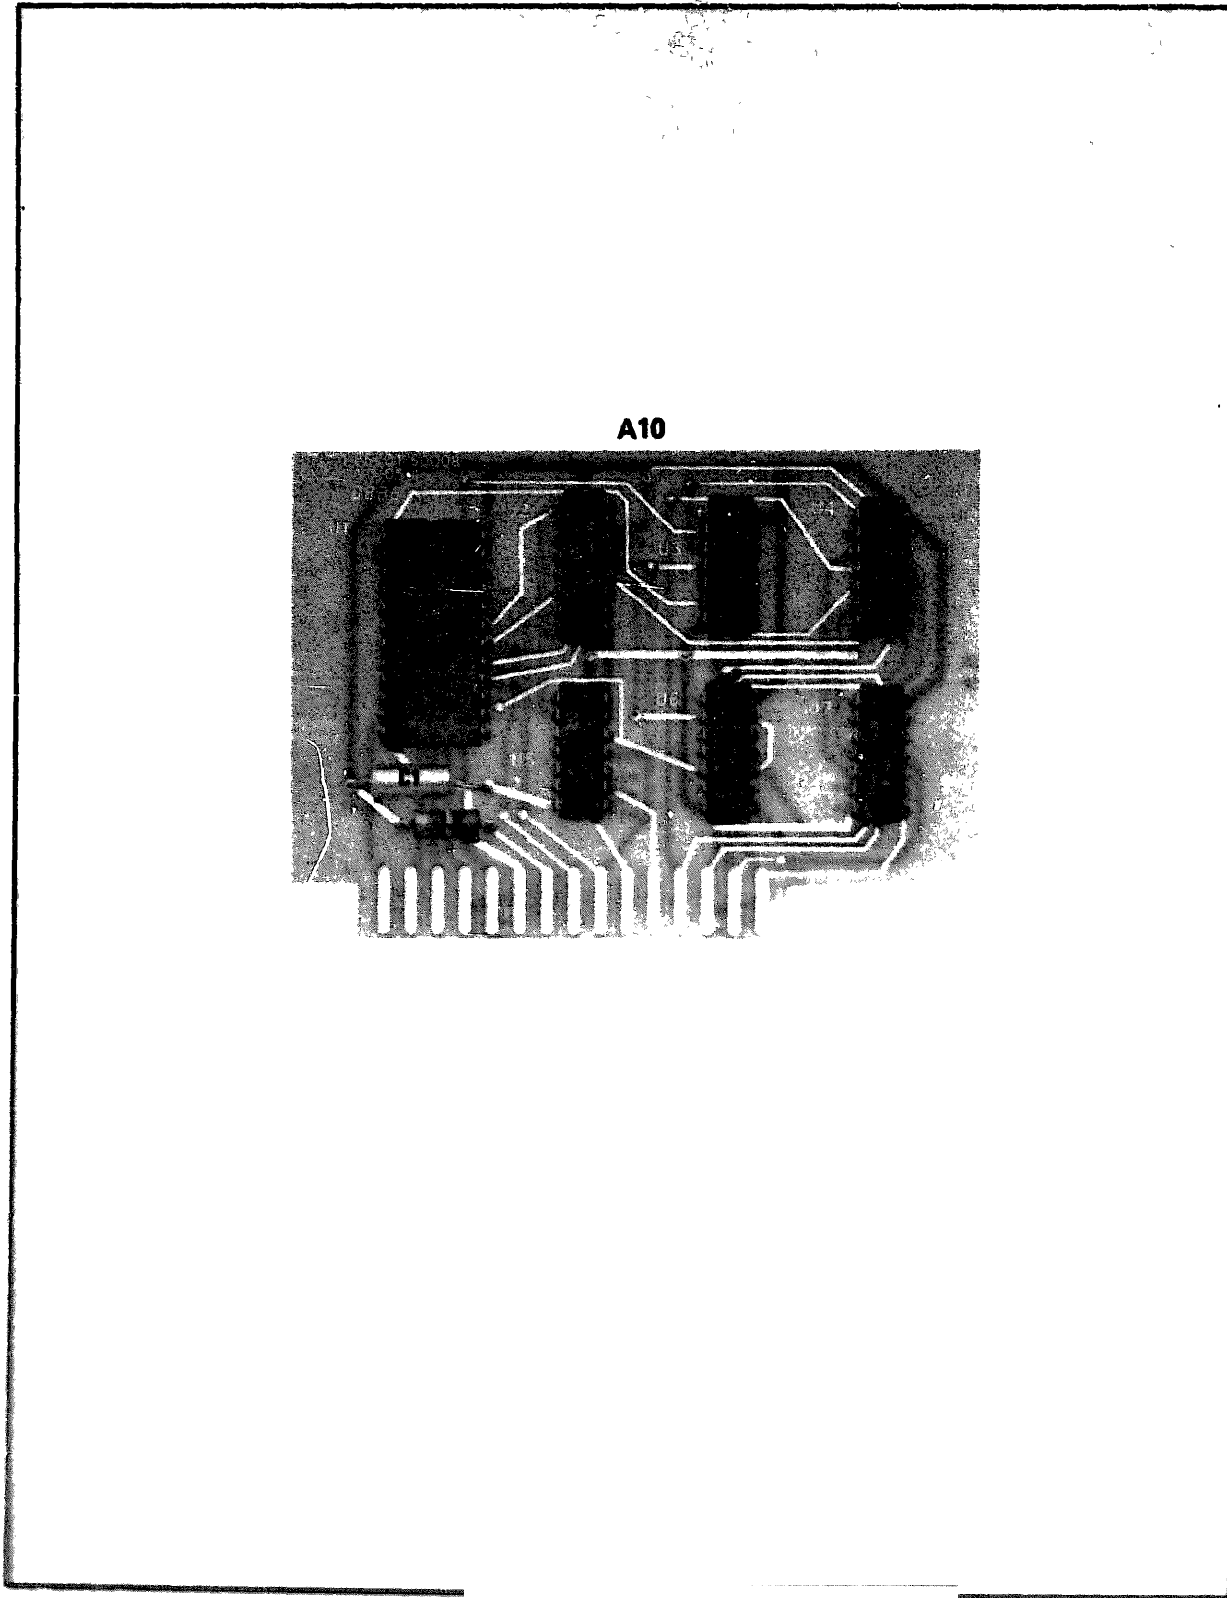


Figure 8-25. Logic Assembly Component Locations

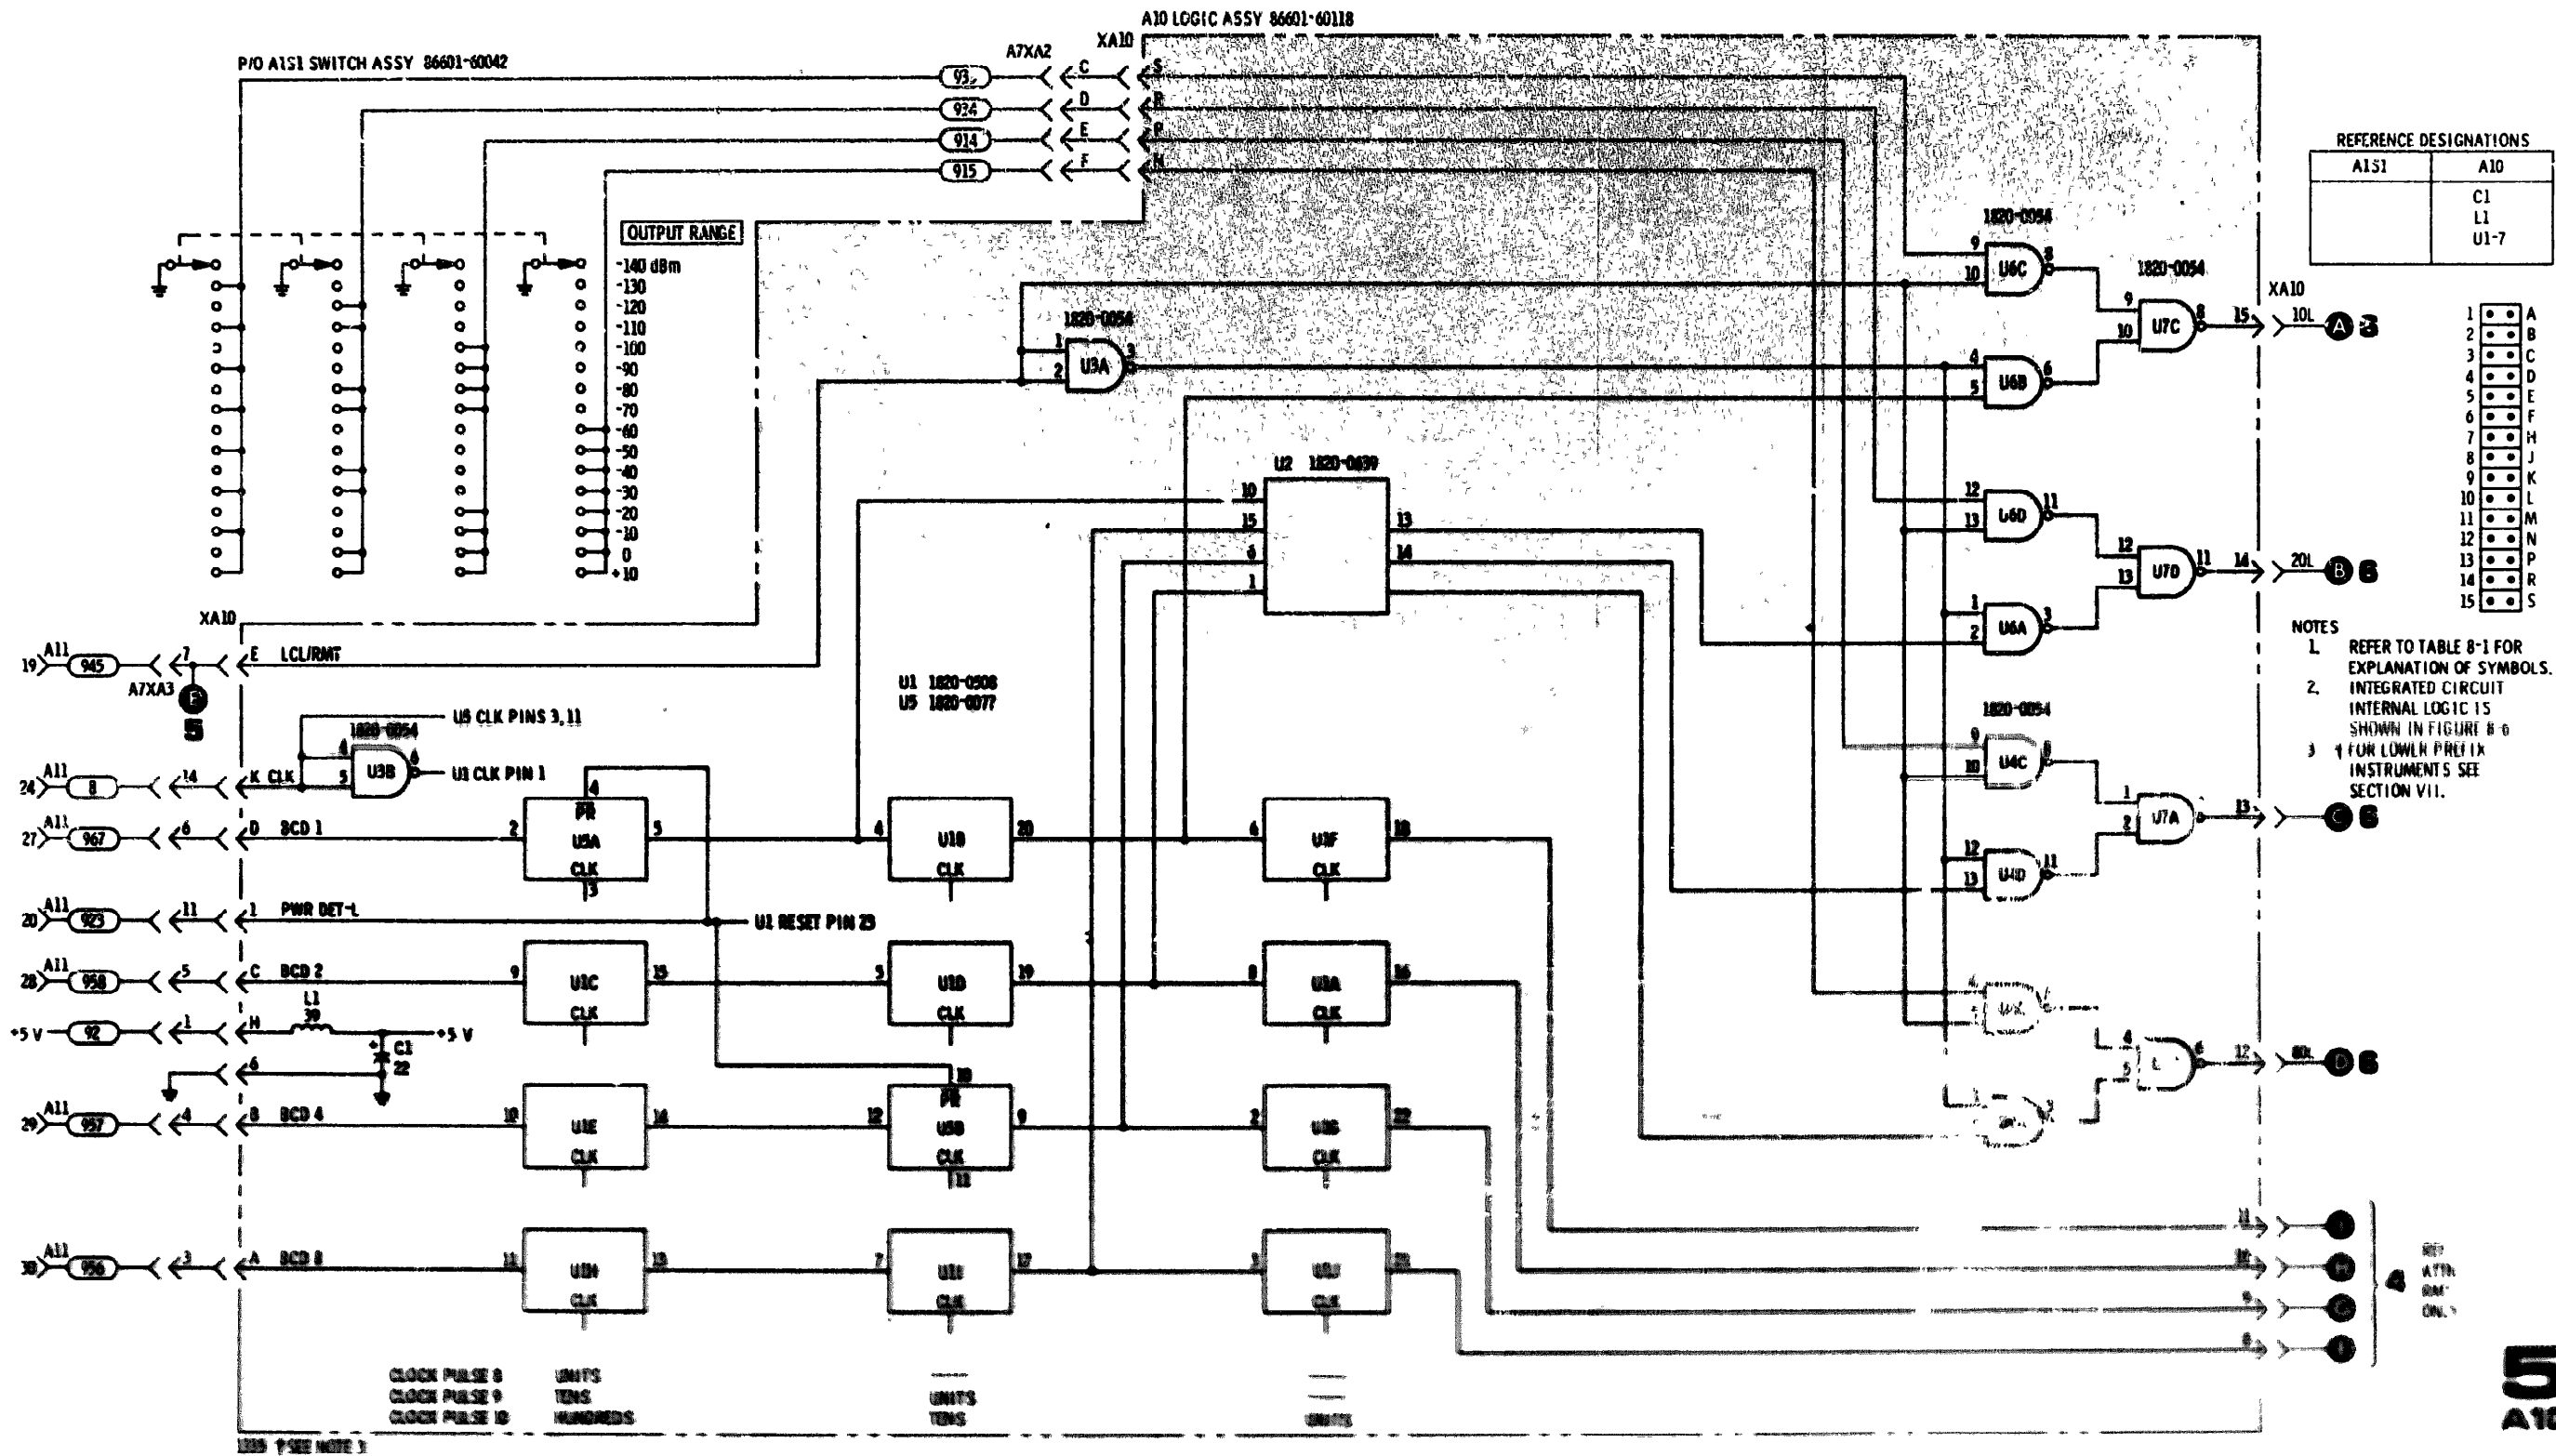


Figure 8-26 Logic and Driver Circuit Schematics

SERVICE SHEET 6

Normally, causes of malfunction in the Model 86601A will be isolated to a circuit board or assembly as a result of performing the tests specified in the troubleshooting tree.

When trouble has been isolated to the A8 assembly, the defective assembly should be extended from the chassis with an extender board to provide access to test points and components.

EQUIPMENT REQUIRED:

- Digital Voltmeter
- Extender Cable

ATTENUATOR AND DRIVER ASSEMBLIES

The programmable attenuator is a five-section relay operated attenuator. There are one 10 dB, one 20 dB and three 40 dB sections in the attenuator. Two of the 40 dB attenuator sections are in series to provide 80 dB of attenuation.

NOTE

The programmable attenuator is not considered a field repairable item. If found defective it should be returned to the factory for repairs, or a replacement may be ordered as a module exchange item.

The A8 attenuator driver assembly consists of four identical transistor switching circuits. These switching circuits are controlled by the binary (1 - 2 - 4 - 8) inputs from the A10 logic assembly. Since the switching circuits are all identical, only the binary 1 (10 dB) circuit will be discussed.

When the binary input at XA8 pin M is low Q15 and Q11 are turned off, Q16 and Q12 are turned on, and -21V is applied to the 10 dB section of the 150 dB programmable attenuator through XA8 pin 4. The 10 dB section of the attenuator is bypassed (no attenuation provided).

When the binary input at XA8 pin M is high Q16 and Q12 are turned off, Q15 and Q11 are turned on, and +21V is applied to the 10 dB section of the 150 dB programmable attenuator through XA8 pin 4. The 10 dB section of the attenuator is enabled and 10 dB of attenuation is inserted into the rf output signal path.

The 150 dB programmable attenuator sections are selected by binary 1 - 2 - 4 - 8 inputs to the A8 assembly from 0000 to 1111 to provide 16 discrete 10 dB steps.

NOTE

The programmed attenuation must be subtracted from +13 dBm in order to determine the rf output level of the Model 86601A. Example: with 120 dB of attenuation programmed in, the rf output will be -116 dBm.

TEST PROCEDURE

Table 8-4 provides input and output level information for the attenuator driver assembly. Make the checks in local mode.

Table 8-4. Attenuator Driver Levels

OUTPUT RANGE (dBm)	XA8 pins							
	M	L	K	J	4	3	2	1
-140	H	H	H	H	H	H	H	H
-130	L	H	H	H	L	H	H	H
-120	H	L	H	H	H	L	H	H
-110	L	L	H	H	L	L	H	H
-100	H	H	L	H	H	H	L	H
- 90	L	H	L	H	L	H	L	H
- 80	H	L	L	H	H	L	L	H
- 70	L	L	L	H	L	L	L	H
- 60	H	H	H	L	H	H	H	L
- 50	L	H	H	L	L	H	H	L
- 40	H	L	H	L	H	L	H	L
- 30	L	L	H	L	L	L	H	L
- 20	H	H	L	L	H	H	L	L
- 10	L	H	L	L	L	H	L	L
0	H	L	L	L	H	L	L	L
+ 10	L	L	L	L	L	L	L	L


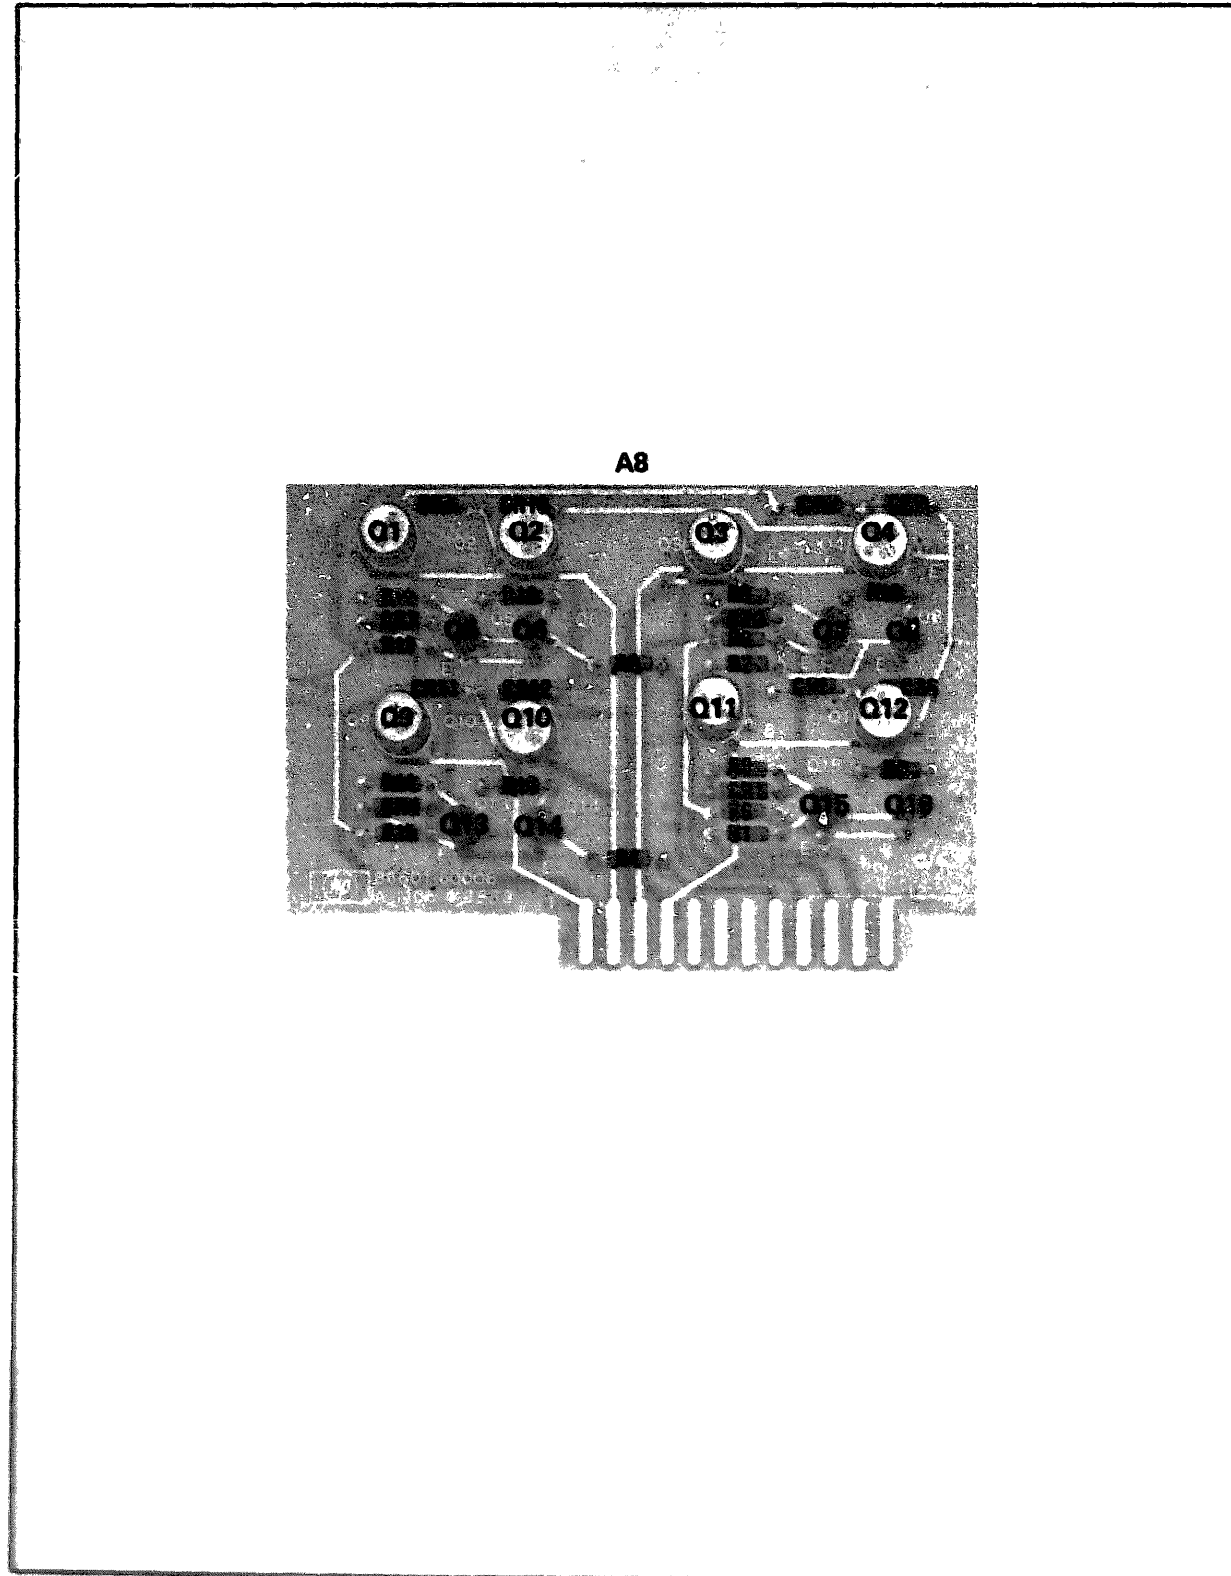



Figure 8-27. *Actuator Driver Component Locations*

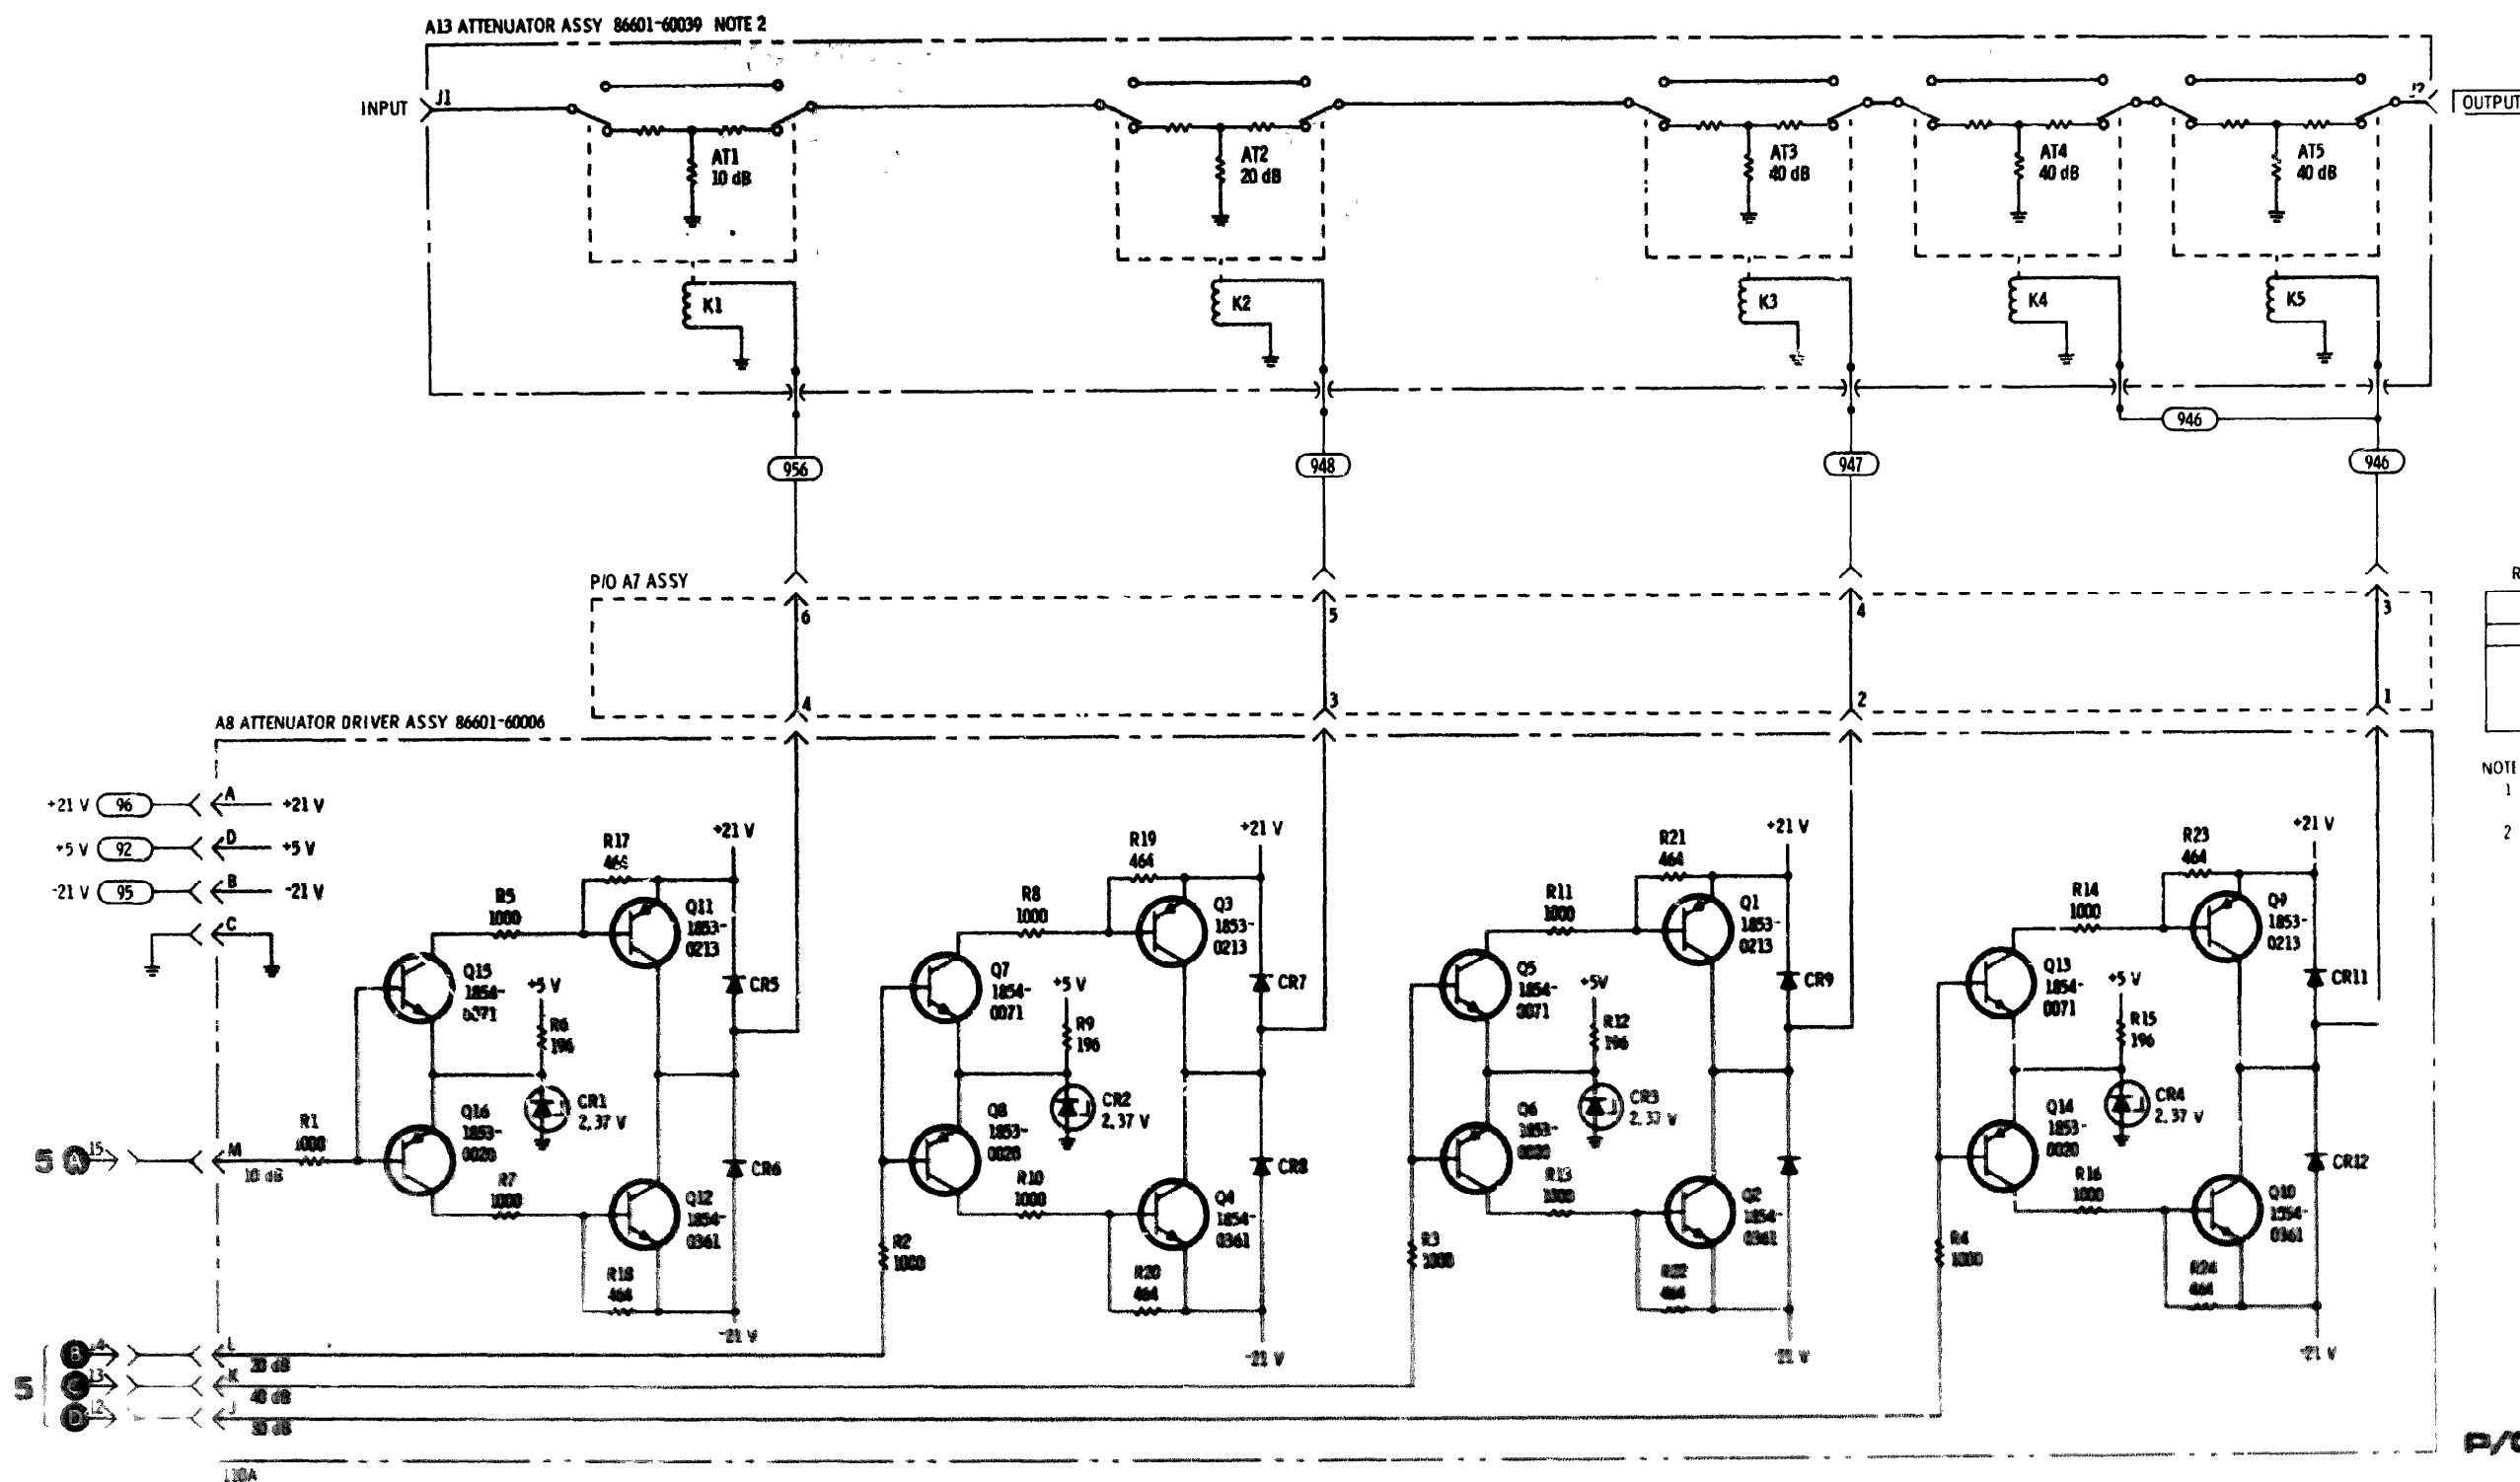

REFERENCE DESIGNATIONS

P/O A7	A13
A8	
CR1-12	
Q1-16	
R1-24	

- NOTES
- REFER TO TABLE B-1 FOR EXPLANATION OF SYMBOLS
 - FACTORY REPAIR ONLY



6
P/O A7, A8, A13

Figure 8-28. Attenuator Driver Schematic

APPENDIX A

REFERENCES

- DA Pam 310-4** Index of Technical **Man**uals, Technical Bulletins, Supply Manuals (Types 7, 8, and 9), Supply Bulletins, and Lubrication Orders.
- DA Pam 310-7** **US Army Equipment Index of Mod**ification Work Orders.
- TB 43-0118 Field Instructions for **Painting and Preserv**ing Electronics Command Equipment **ment Including Camouflage Pattern** Painting of Electrical Equipment Shelters.
- TM 38-750 **The Army Maintenance Manage**ment System (**TAMMS**).
- TM 750-244-2 **Procedures for Destruction of Electronics Ma**terial to Prevent Enemy Use (**Electronics Command**).
- TM 11-6625-2837-14-1 **Operator's, Organizational, DS and GS Maintenance Manual for Signa** Generator, **Hewlett-Packard Model 8660C Including Extension M**odule, **Hewlett-Packard Model 11661B**.

APPENDIX D

MAINTENANCE ALLOCATION

Section I. INTRODUCTION

D-1. General.

This appendix provides a summary of the maintenance operations for R.F. Section Plug-In HP 86601A. It authorizes categories of maintenance for specific maintenance functions on repairable item and components and the tools and equipment required to perform each function. This appendix may be used **as an aid in planning** maintenance operations.

D-2. Maintenance Function.

Maintenance functions will be limited to and defined as follows:

a. Inspect. To determine the serviceability of an item by comparing its physical, mechanical, and/or electrical characteristics with established standards through examination.

b. Test. To verify serviceability and to detect incipient failure by measuring the mechanical or electrical characteristics of an item and comparing those characteristics with prescribed standards.

c. Service. Operations required periodically to keep an item in proper operating condition, i.e., to clean (decontaminate), to preserve, to drain, to paint, or to replenish fuel, lubricants, hydraulic fluids, or compressed air supplies.

d. Adjust. To maintain, within prescribed limits, by bringing into proper or exact position, or by setting the operating characteristics to the specified parameters.

e. Align. To adjust specified variable elements of an item to bring about optimum or desired performance.

f. Calibrate. To determine and cause corrections to be made or to be adjusted on instruments or test measuring and diagnostic equipments used in precision measurement. Consists of comparisons of two instruments, one of which is a certified standard of known accuracy, to detect and adjust any discrepancy in the accuracy of the instrument being compared.

g. Install. The act of assembling, seating, or fixing into position an item, part, module (component or assembly) in a manner to allow the proper functioning of the equipment or system.

h. Replace. The act of substituting a serviceable like type part, subassembly, or module (component or assembly) for an unserviceable counterpart.

i. Repair. The application of maintenance services (**inspect, test, service, adjust, align, calibrate, replace**) or other maintenance actions (**welding, grinding, riveting, straightening, facing, remachining, or resurfacing**) to restore serviceability to an item by correcting specific damage, fault, malfunction, or failure in a part, subassembly, module (component or assembly), end item, or system.

j. Overhaul. That maintenance effort (service/action) necessary to restore an item to a completely serviceable/operational condition as prescribed by maintenance standards (i.e., DMWR) in appropriate technical publications. Overhaul is normally the highest degree of maintenance performed by the Army. Overhaul does not normally return an item to like new condition.

k. Rebuild. Consists of those services/actions necessary for the restoration of unserviceable equipment to a like new condition in accordance with original manufacturing standards. Rebuild is the highest degree of materiel maintenance applied to Army equipment. The rebuild operation includes the act of returning to zero those age measurements (hours, miles, etc.) considered in classifying Army equipments/components.

D-3. Column Entries.

a. Column 1, Group Number. Column 1 lists group numbers, the purpose of which is to identify components, assemblies, subassemblies, and modules with the next higher assembly.

b. Column 2, Component/Assembly. Column 2 contains the noun names of components, assemblies, subassemblies, and modules for which maintenance is authorized.

c. Column 3, Maintenance Functions. Column 3 lists the functions to be performed on the item listed in column 2. When items are listed without maintenance functions it is noted for purposes of having the group numbers in the M.I.C. and E.P.M.T. associate.

d. Column 4, Maintenance Category. Column 4 specifies, by the listing of a "worktime" figure in the appropriate subcolumn(s), the lowest level of maintenance authorized to perform the function listed in column 3. This figure represents the active time required to perform that maintenance function at the indicated category of maintenance. If the number or complexity of the tasks within the listed maintenance function vary at different maintenance categories, appropriate "worktime" figures will be shown for each category. The number of task-hours specified by the "worktime" figure represents the average time required to restore an item (assembly, subassembly, component, module, end item or system) to a serviceable condition under typical field operating conditions. This time includes preparation time, troubleshooting time, and quality assurance/quality control time in addition to the time required to perform the specific tasks identified for the maintenance functions authorized in the maintenance allocation chart. Subcolumns of column 4 are as follows:

- C-Operator/Crew
- O-Organizational
- F-Direct Support
- H-General Support
- D-Depot

e. Column 5, Tools and Equipment. Column 5 specifies by code, those common tool sets (not individual tools) and special tools, test, and support equipment required to perform the designated function.

f. Column 6, Remarks. Column 6 contains an alphabetic code which leads to the remark in section IV,

Remarks, which is pertinent to the item opposite the particular code.

D-4. Tool and Test Equipment Requirements
(Sect. III).

a. Tool or Test Equipment Reference Code. The numbers in this column coincide with the numbers used in the tools and equipment column of the MAC. The numbers indicate the applicable tool or test equipment for the maintenance functions.

b. Maintenance Category. The codes in this column indicate the maintenance category allocated the tool or test equipment.

c. Nomenclature. This column lists the noun name and nomenclature of the tools and test equipment required to perform the maintenance functions.

d. National/NATO Stock Number. This column lists the National/NATO stock number of the specific tool or test equipment.

e. Tool Number. This column lists the manufacturer's part number of the tool followed by the Federal Supply Code for manufacturers (5-digit) in parentheses.

D-5. Remarks (Sect. IV).

a. Reference Code. This code refers to the appropriate item in section II, column 6.

b. Remarks. This column provides the required explanatory information necessary to clarify items appearing in Section II.

(Next printed page is D-)

SECTION II MAINTENANCE ALLOCATION CHART
FOR

R.F. SECTION PLUG-IN HP 86601A

TM 11-6625-2837-14&P-6

(1)
GROUP
NUMBER

(1) GROUP NUMBER	(2) COMPONENT/ASSEMBLY	(3) MAINTENANCE FUNCTION	(4) MAINTENANCE CATEGORY					(5) TOOLS AND EQPT.	(6) REMARKS
			C	C	F	H	D		
00	R.F. SECTION PLUG-IN HP 86601A	Inspect Test Test Adjust Install Replace Repair Overhaul		0.2 0.3				Visual Simple, oper- ational 1 thru 7 8 27 27 8 1 thru 26	

SECTION III TOOL AND TEST EQUIPMENT REQUIREMENTS
FOR

TM 11-6625-2837-14&P-6

R.F. SECTION PLUG-IN HP 86601A

TOOL OR TEST EQUIPMENT REF CODE	MAINTENANCE CATEGORY	NOMENCLATURE	NATIONAL/NATO STOCK NUMBER	TOOL NUMBER
1	H, D	ANALYZER, SPECTRUM TS-723/U	6625-00-668-9418	
2	H, D	GENERATOR, SIGNAL AN/USM-205	6625-00-788-9672	
3	H, D	MULTIMETER, ME-26/U	6625-00-913-9781	
4	H, D	OSCILLOSCOPE AN/USM-281	6625-00-106-9622	
5	H, D	VOLTMETER AN/GSM-64	6625-00-022-7894	
6	H, D	VOLTMETER AN/URM-145	6625-00-973-3986	
7	H, D	VOLTMETER ME-30/U	6625000-643-1670	
8	H, D	TCOL KIT TK-100/G	5180-00-605-0075	
9	D	ANALYZER, SPECTRUM HP 141T		
10	D	PLUG-IN HP 8552B		
11	D	PLUG-IN HP 8553B		
12	D	PLUG-IN HP 8554B		
13	D	PLUG-IN HP 8556A		
14	D	GENERATOR, SIGNAL HP 203A		
15	D	GENERATOR, SIGNAL HP 8444A		
16	D	VOLTMETER HP 3406A		
17	D	VOLTMETER HP 8406A		
18	D	ATTENUATOR HP H38-355D		
19	D	DETECTOR HP 8471A		
20	D	DISCRIMINATOR, FM HP 5210A		
21	D	DUMMY LOAD HP 1250-0207		
22	D	MARKED CARD PROGRAMMER HP 3260A		
23	D	MIXER, DOUBLE BALANCED HP 13514A		
24	D	POWER SUPPLY HP 721		
25	D	PROBE HP 10004		
26	D	SERVICE KIT HP 11672A		
27	O	TOOLS AND TEST EQUIPMENT AVAILABLE TO THE REPAIRER BECAUSE OF HIS/HER ASSIGNED MISSION.		

APPENDIX E

REPAIR PARTS AND SPECIAL TOOLS LISTS

Refer to Section VI, Replaceable Parts, for all maintenance repair parts.

RECOMMENDED CHANGES TO EQUIPMENT TECHNICAL MANUALS



SOMETHING WRONG WITH THIS MANUAL?

THEN... JOT DOWN THE DOPE ABOUT IT ON THIS FORM, TEAR IT OUT, FOLD IT AND DROP IT IN THE MAIL!

FROM: (YOUR UNIT'S COMPLETE ADDRESS)

Commander
Stateside Army Depot
ATTN: AMSTA-US
Stateside, N.J. 07703

DATE 10 July 1975

PUBLICATION NUMBER

TM 11-5840-340-20P

DATE

23 Jan 78

TITLE

Radar Set AN/PRC-76

BE EXACT... PIN-POINT WHERE IT IS

IN THIS SPACE TELL WHAT IS WRONG AND WHAT SHOULD BE DONE ABOUT IT:

PAGE NO.	PARA-GRAPH	FIGURE NO.	TABLE NO.
33			
44		19	
45			

For item 2, change the NSN to read: 5835-00-134-9186.
Reason: Accuracy.

Identify the cover on the junction box (item no. 5).
Reason: It is a separate item and is not called out on figure 19.

Add the cover of the junction box as an item in the listing for figure 19.
Reason: Same as above.

TEAR ALONG DOTTED LINE

S
A
M
B
L
E

TYPED NAME, GRADE OR TITLE AND TELEPHONE NUMBER

SEC I. M. DeSpirito 999-1776

SIGN HERE:

SEC I. M. DeSpirito

DA FORM 2028-2

P.S.—IF YOUR UNIT WANTS TO KNOW ABOUT YOUR MANUALS, "SOMETHING" MAKE A CARBON COPY OF THIS AND GIVE IT TO YOUR MESSAGE CENTER.

FILL IN YOUR
UNIT'S ADDRESS

FOLD BACK

DEPARTMENT OF THE ARMY

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE, \$300

POSTAGE AND FEES PAID
DEPARTMENT OF THE ARMY
GOG-314



Commander
US Army Communications and
Electronics Materiel Readiness Command
ATTN: DRSEL-ME-MQ
Fort Monmouth, New Jersey 07703

TEAR ALONG DOTTED LINE

FOLD BACK

RECOMMENDED CHANGES TO EQUIPMENT TECHNICAL MANUALS



SOMETHING WRONG WITH THIS MANUAL?

THEN... JOT DOWN THE DOPE ABOUT IT ON THIS FORM, TEAR IT OUT, FOLD IT AND DROP IT IN THE MAIL!

FROM: (YOUR UNIT'S COMPLETE ADDRESS)

DATE

PUBLICATION NUMBER

DATE

TITLE

TM 11-6625-2937-14&P-6

23 OCT 79

R.F. Section Plug-In
HP 86601A

BE EXACT... PIN-POINT WHERE IT IS

IN THIS SPACE TELL WHAT IS WRONG AND WHAT SHOULD BE DONE ABOUT IT:

PAGE NO.	PARA-GRAPH	FIGURE NO.	TABLE NO.
----------	------------	------------	-----------

TEAR ALONG DOTTED LINE

DA FORM 2028-2

THIS FORM IS OBSOLETE AND SHOULD NOT BE USED. IT IS BEING REPRODUCED FOR INFORMATIONAL PURPOSES ONLY. THE ORIGINAL FORM IS DA FORM 2028-2, 1 OCT 78.

FILL IN YOUR
UNIT'S ADDRESS

FOLD HERE

DEPARTMENT OF THE ARMY

OFFICE AND FREE USE
DEPARTMENT OF THE ARMY
FORM 307



OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE, \$300

Commander
US Army Communications and
Electronics Material Readiness Command
ATTN: 2152L-02-M3
Fort Monmouth, New Jersey 07701

FOLD HERE

CALL TO YOUR
UNIT'S ADDRESS

FOLD BACK

DEPARTMENT OF THE ARMY

POSTAGE AND FEE PAID
DEPARTMENT OF THE ARMY
DD-44



OFFICIAL BUSINESS
Penalty for Private Use, \$300

Commander
US Army Communications and
Electronic Material Readiness Command
ATTN: DESER-MS-010
Fort Monmouth, New Jersey 07703

FOLD FRONT

By Order of the Secretary of the Army:

E.C. MEYER
General, United States Army
Chief of Staff

Official:

J. C. PENNINGTON
Major General, United States Army
The Adjutant General

DISTRIBUTION

Active Army:

TSG (1)
USAARENBD (1)
USAINSOM (2)
TRADOC (2)
DARCOM (1)
TECOM (2)
OS Maj Comd (2)
USACC (2)
HISA (Ft Monmouth) (21)
Armsins (1)
USASIGS (10)
Svc Colleges (1)
Ft Hanchuan (5)
Ft Richardson (CERCOM Ofc) (1)
Ft Carson (5)
Ft Gillem (10)
WSMR (1)

USAERDAA (1)
USAERDAW (1)
Army Dep (1) except
LBAD (10)
SAAD (30)
TOAD (14)
SHAD (3)
USA Dep (1)
Sig Sec USA Dep (1)
Units org under fol TOE:
(1 copy each unit)
29-154
29-196
(2 copies each unit)
29-297
29-610

ARNG: None


USAR: None


For explanation of abbreviations used, see AR 310-50.

END




8-1-83

DATE

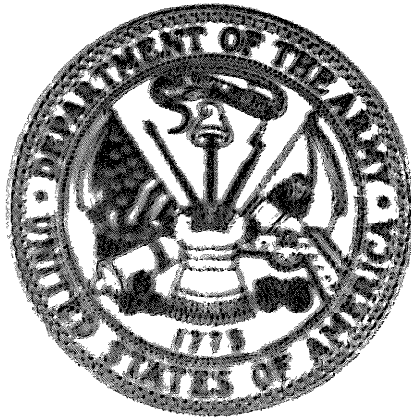

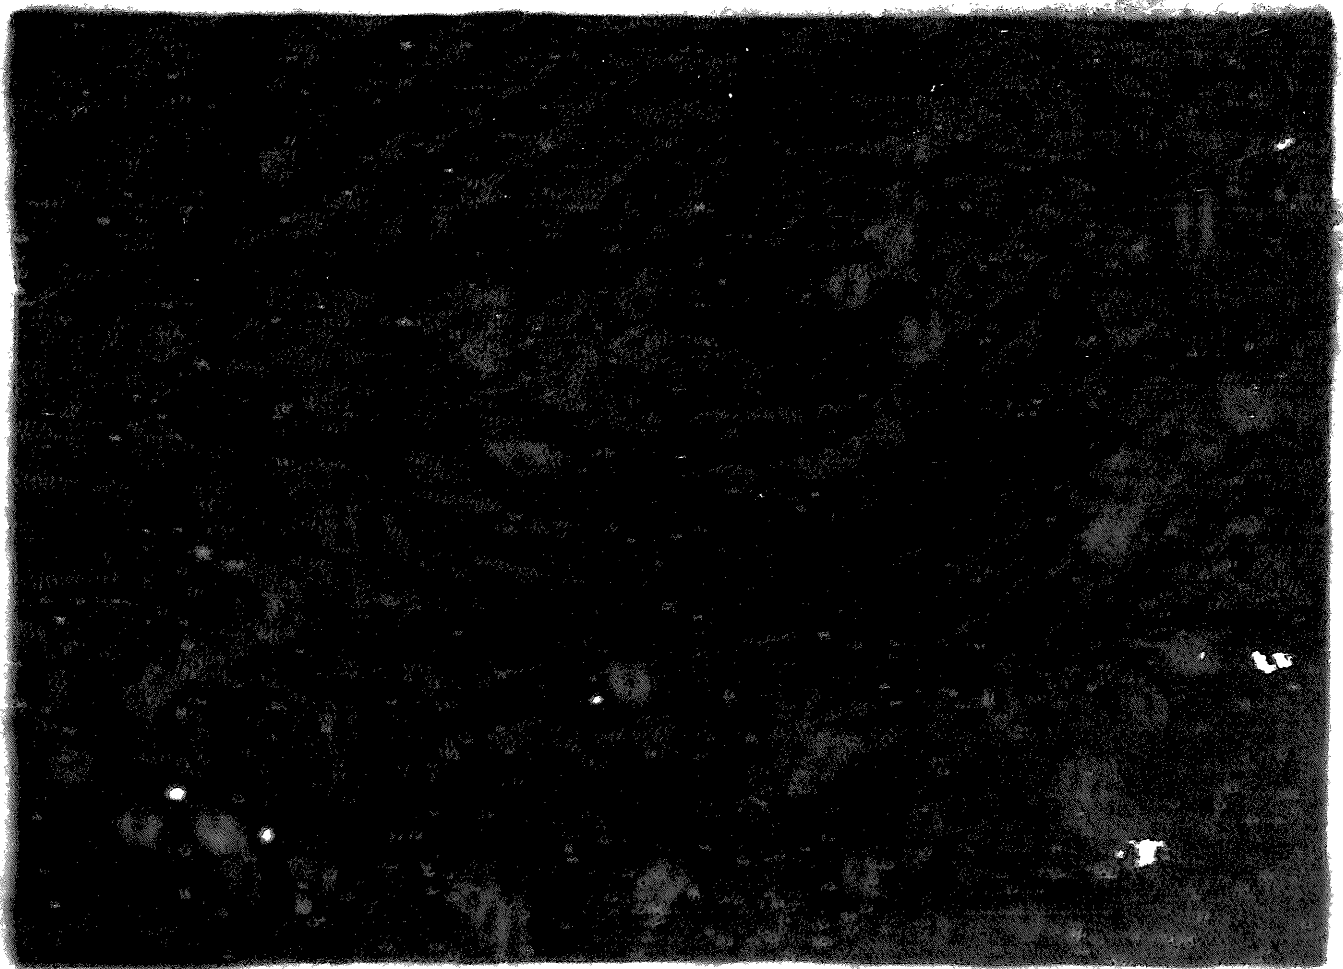

DEPARTMENT OF THE ARMY
MICROFORM TEST TARGET

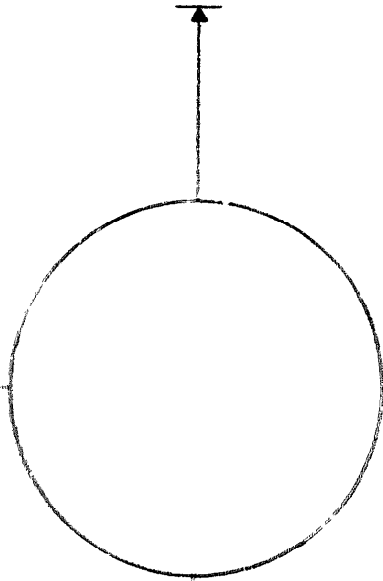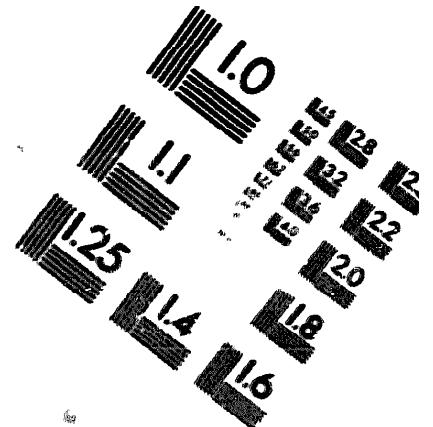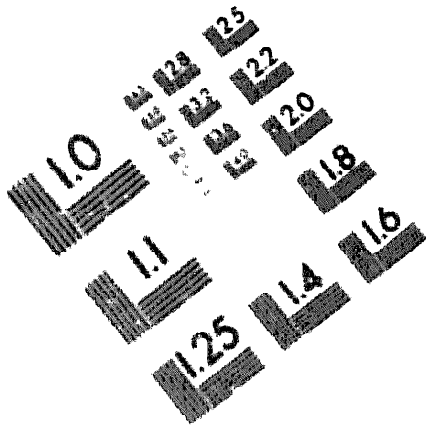

150 MM

1 mm (ap = 0.25 mm)

ABCDEFGHIJKLMN OPQRSTU VWXYZ
abcdefghijklmnopqrstuvwxyz
12345678901234567890

2 mm (ap = 0.50 mm)

ABCDEFGHIJKLMN OPQRSTU VWXYZ
abcdefghijklmnopqrstuvwxyz
12345678901234567890

3 mm (ap = 0.75 mm)

ABCDEFGHIJKLMN OPQRSTU VWXYZ
abcdefghijklmnopqrstuvwxyz
12345678901234567890

4 mm (ap = 1.00 mm)

ABCDEFGHIJKLMN OPQRSTU VWXYZ
abcdefghijklmnopqrstuvwxyz
12345678901234567890

1 mm (ap = 0.25 mm)

ABCDEFGHIJKLMN OPQRSTU VWXYZ
abcdefghijklmnopqrstuvwxyz
12345678901234567890

2 mm (ap = 0.50 mm)



ABCDEFGHIJKLMN OPQRSTU VWXYZ
abcdefghijklmnopqrstuvwxyz
12345678901234567890

3 mm (ap = 0.75 mm)

ABCDEFGHIJKLMN OPQRSTU VWXYZ
abcdefghijklmnopqrstuvwxyz
12345678901234567890

4 mm (ap = 1.00 mm)

ABCDEFGHIJKLMN OPQRSTU VWXYZ
abcdefghijklmnopqrstuvwxyz
12345678901234567890

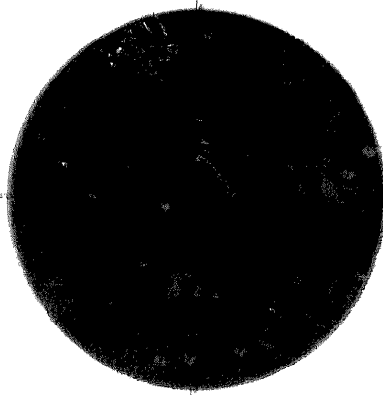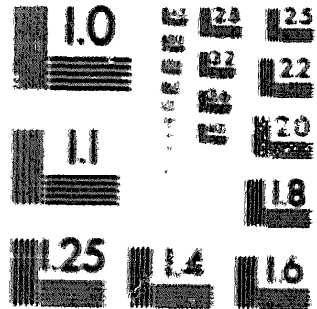

200 MM

